

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082818\
 Data File : VV007235.D
 Acq On : 28 Aug 2018 21:20
 Operator : SY/MD
 Sample : J4628-20
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB3G5

Quant Time: Aug 29 04:26:27 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 29 04:00:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	216925	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	217633	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	85834	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	72079	4.68	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.60%
7) Chloroethane-d5	1.58	69	61763	4.98	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.60%
11) 1,1-Dichloroethene-d2	2.13	63	98302	3.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.80%
20) 2-Butanone-d5	3.97	46	196998	51.24	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.48%
24) Chloroform-d	4.41	84	151730	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.60%
26) 1,2-Dichloroethane-d4	5.09	65	78433	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.20%
32) Benzene-d6	5.10	84	286231	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
36) 1,2-Dichloropropane-d6	6.12	67	95549	4.75	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.00%
41) Toluene-d8	7.37	98	208947	3.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.80%
43) trans-1,3-Dichloropropene-	7.67	79	28446	3.98	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	79.60%
46) 2-Hexanone-d5	8.15	63	68684	36.53	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	73.06%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	72913	4.66	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	79648	4.83	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.60%


Target Compounds					Ovalue
13) Acetone	2.21	43	13123	6.81 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082818\
Data File : VV007235.D
Acq On : 28 Aug 2018 21:20
Operator : SY/MD
Sample : J4628-20
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB3G5

Quant Time: Aug 29 04:26:27 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 29 04:00:48 2018
Response via : Initial Calibration

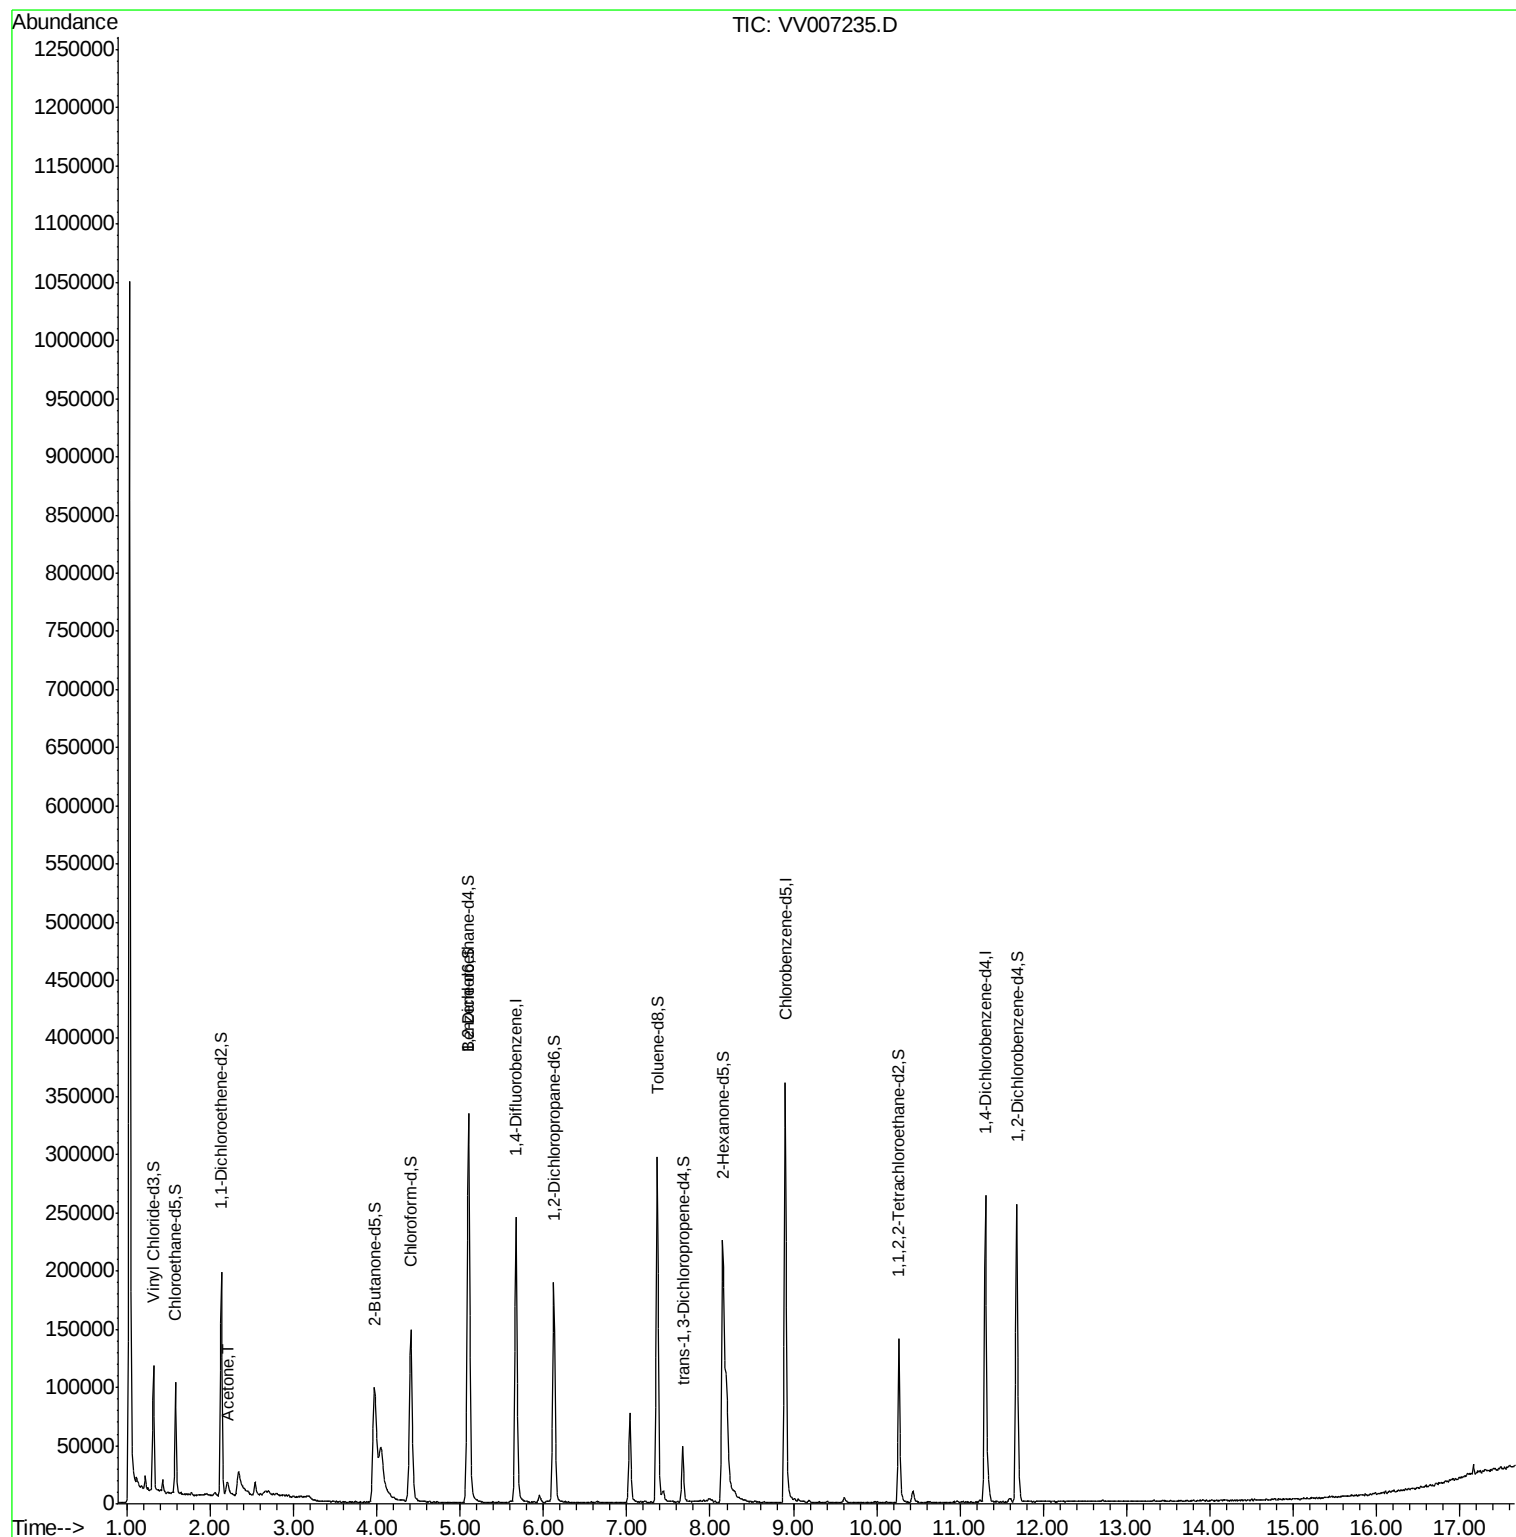

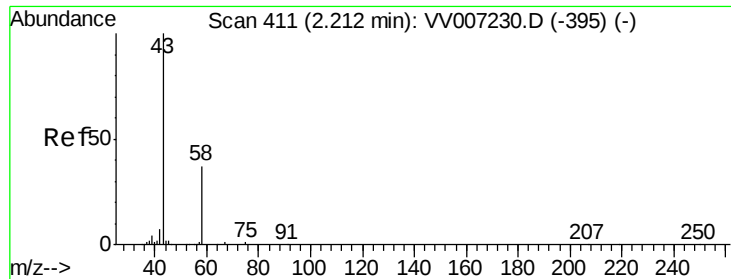

#13

Acetone

Concen: 6.81 ug/L

RT: 2.21 min Scan# 409

Delta R.T. -0.01 min

Lab File: VV007235.D

Acq: 28 Aug 2018 21:20

Instrument :
MSVOA_V
ClientSampleId :
DB3G5

Tot Ion: 43 Resp: 13123

Ion Ratio Lower Upper

43 100

58 35.9 0.0 70.2

