

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082818\
 Data File : VV007236.D
 Acq On : 28 Aug 2018 21:47
 Operator : SY/MD
 Sample : J4628-24
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB3G7

Quant Time: Aug 29 04:28:00 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 29 04:00:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	226291	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	227566	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	92139	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	72891	4.54	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.80%
7) Chloroethane-d5	1.58	69	63560	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.20%
11) 1,1-Dichloroethene-d2	2.13	63	97642	3.51	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.20%
20) 2-Butanone-d5	3.98	46	153117	38.18	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	76.36%
24) Chloroform-d	4.41	84	148993	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.80%
26) 1,2-Dichloroethane-d4	5.09	65	74256	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.80%
32) Benzene-d6	5.10	84	280069	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.60%
36) 1,2-Dichloropropane-d6	6.12	67	94280	4.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.60%
41) Toluene-d8	7.37	98	209191	3.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.40%
43) trans-1,3-Dichloropropene-	7.67	79	28295	3.79	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.80%
46) 2-Hexanone-d5	8.15	63	61071	31.07	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	62.14%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	72194	4.41	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	81370	4.60	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	96162	47.81	ug/L 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082818\
Data File : VV007236.D
Acq On : 28 Aug 2018 21:47
Operator : SY/MD
Sample : J4628-24
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB3G7

Quant Time: Aug 29 04:28:00 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 29 04:00:48 2018
Response via : Initial Calibration

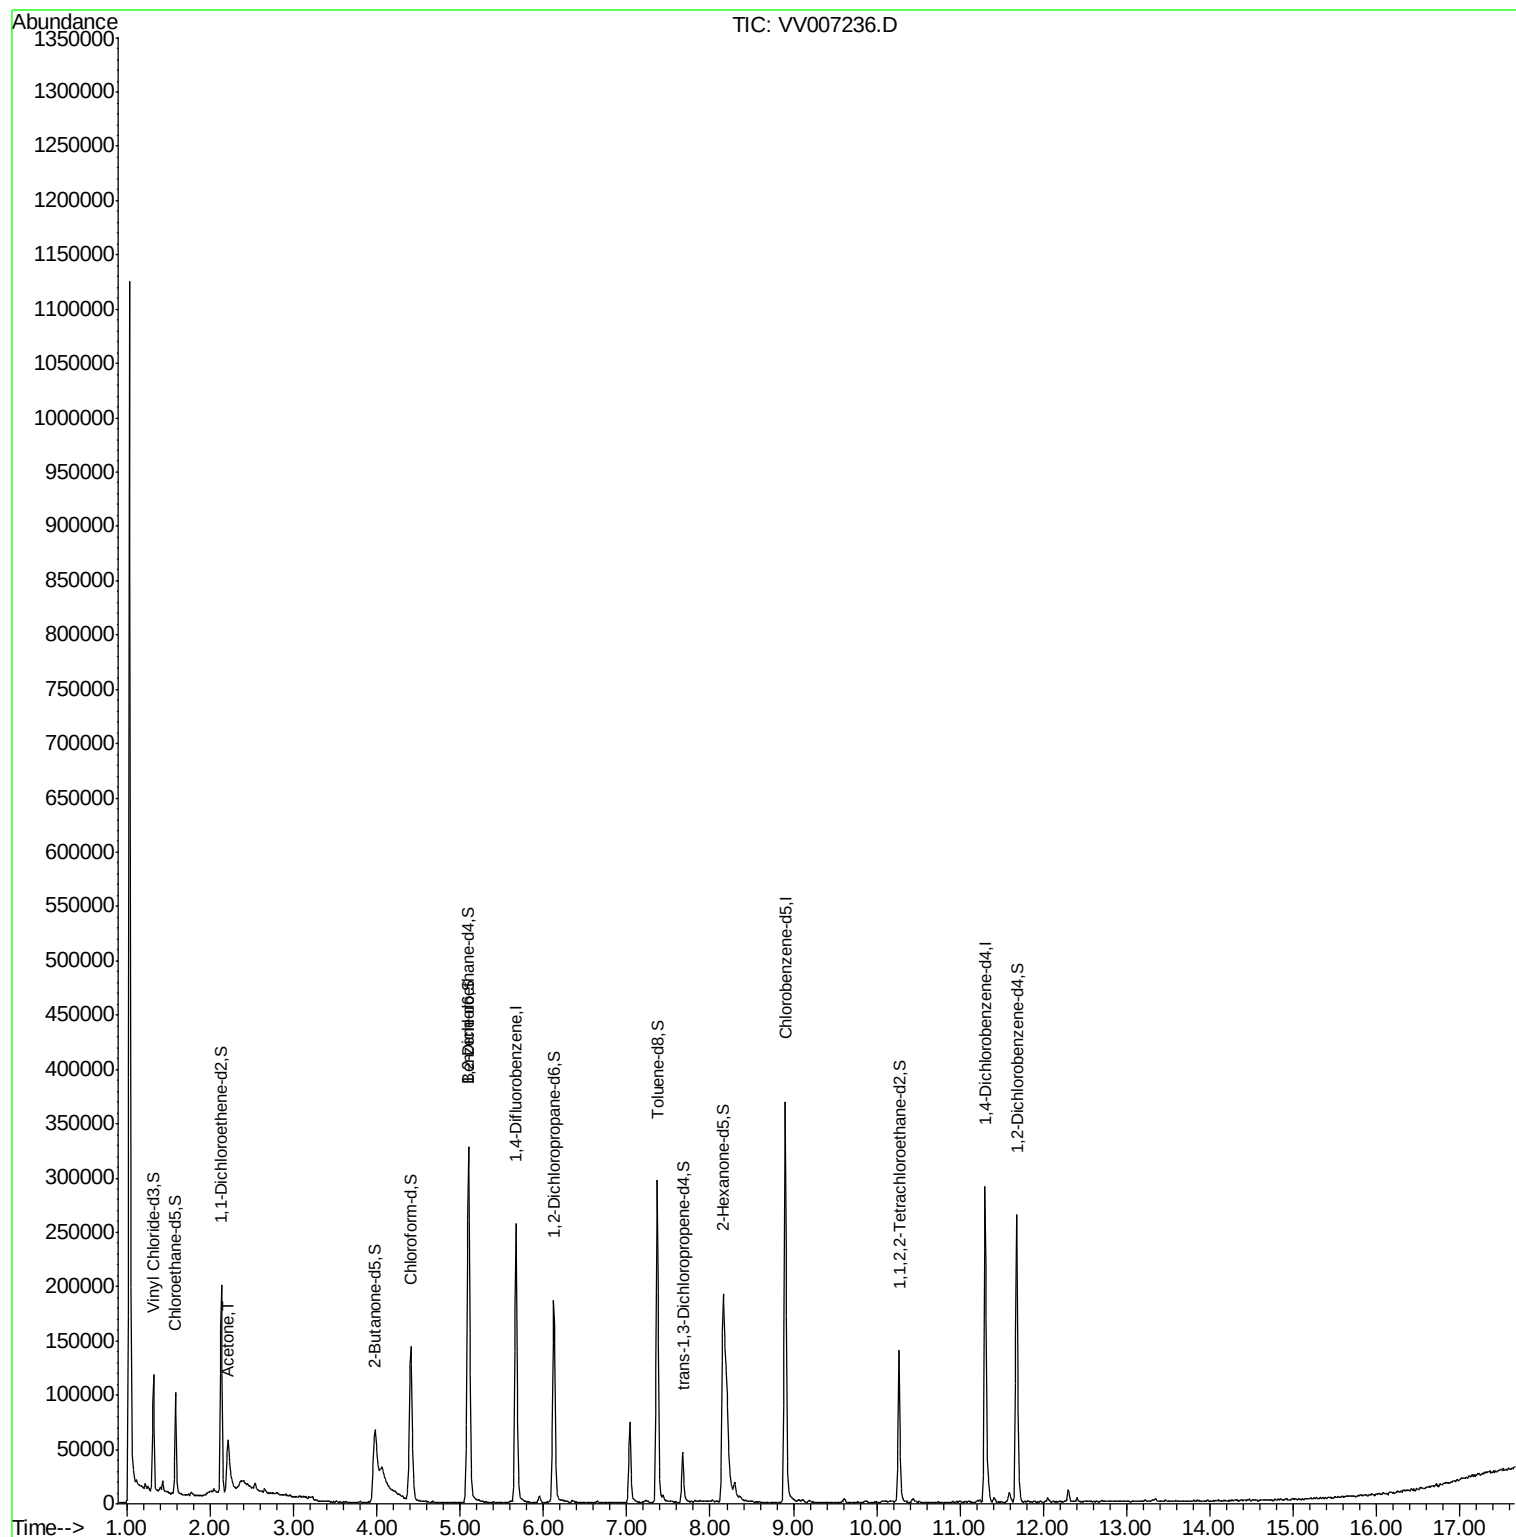

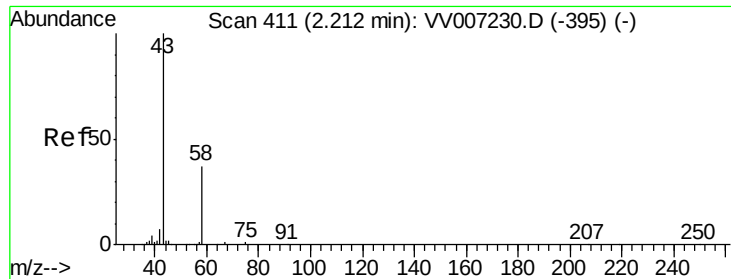

#13

Acetone

Concen: 47.81 ug/L

RT: 2.21 min Scan# 411

Delta R.T. 0.00 min

Lab File: VV007236.D

Acq: 28 Aug 2018 21:47

Instrument :
MSVOA_V
ClientSampleId :
DB3G7

Tot Ion: 43 Resp: 96162

Ion Ratio Lower Upper

43 100

58 35.4 0.0 70.2

