

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082818\
 Data File : VV007245.D
 Acq On : 29 Aug 2018 01:51
 Operator : SY/MD
 Sample : J4647-12
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAB76

Quant Time: Aug 29 04:49:38 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082818WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Aug 29 04:00:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	230580	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	237144	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	88366	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	71389	4.36	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.20%
7) Chloroethane-d5	1.58	69	63796	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.80%
11) 1,1-Dichloroethene-d2	2.13	63	99137	3.50	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.00%
20) 2-Butanone-d5	3.97	46	206327	50.49	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.98%
24) Chloroform-d	4.41	84	156225	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.60%
26) 1,2-Dichloroethane-d4	5.09	65	79777	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
32) Benzene-d6	5.10	84	288516	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.60%
36) 1,2-Dichloropropane-d6	6.12	67	98205	4.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.60%
41) Toluene-d8	7.37	98	212203	3.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.40%
43) trans-1,3-Dichloropropene-	7.67	79	29395	3.77	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.40%
46) 2-Hexanone-d5	8.15	63	73220	35.74	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	71.48%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	75952	4.46	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	80961	4.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	6562	3.20 ug/L	72
42) Toluene	7.44	91	15036	0.22 ug/L	99
47) Tetrachloroethene	8.02	164	11879	0.81 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082818\
Data File : VV007245.D
Acq On : 29 Aug 2018 01:51
Operator : SY/MD
Sample : J4647-12
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAB76

Quant Time: Aug 29 04:49:38 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082818WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Aug 29 04:00:48 2018
Response via : Initial Calibration

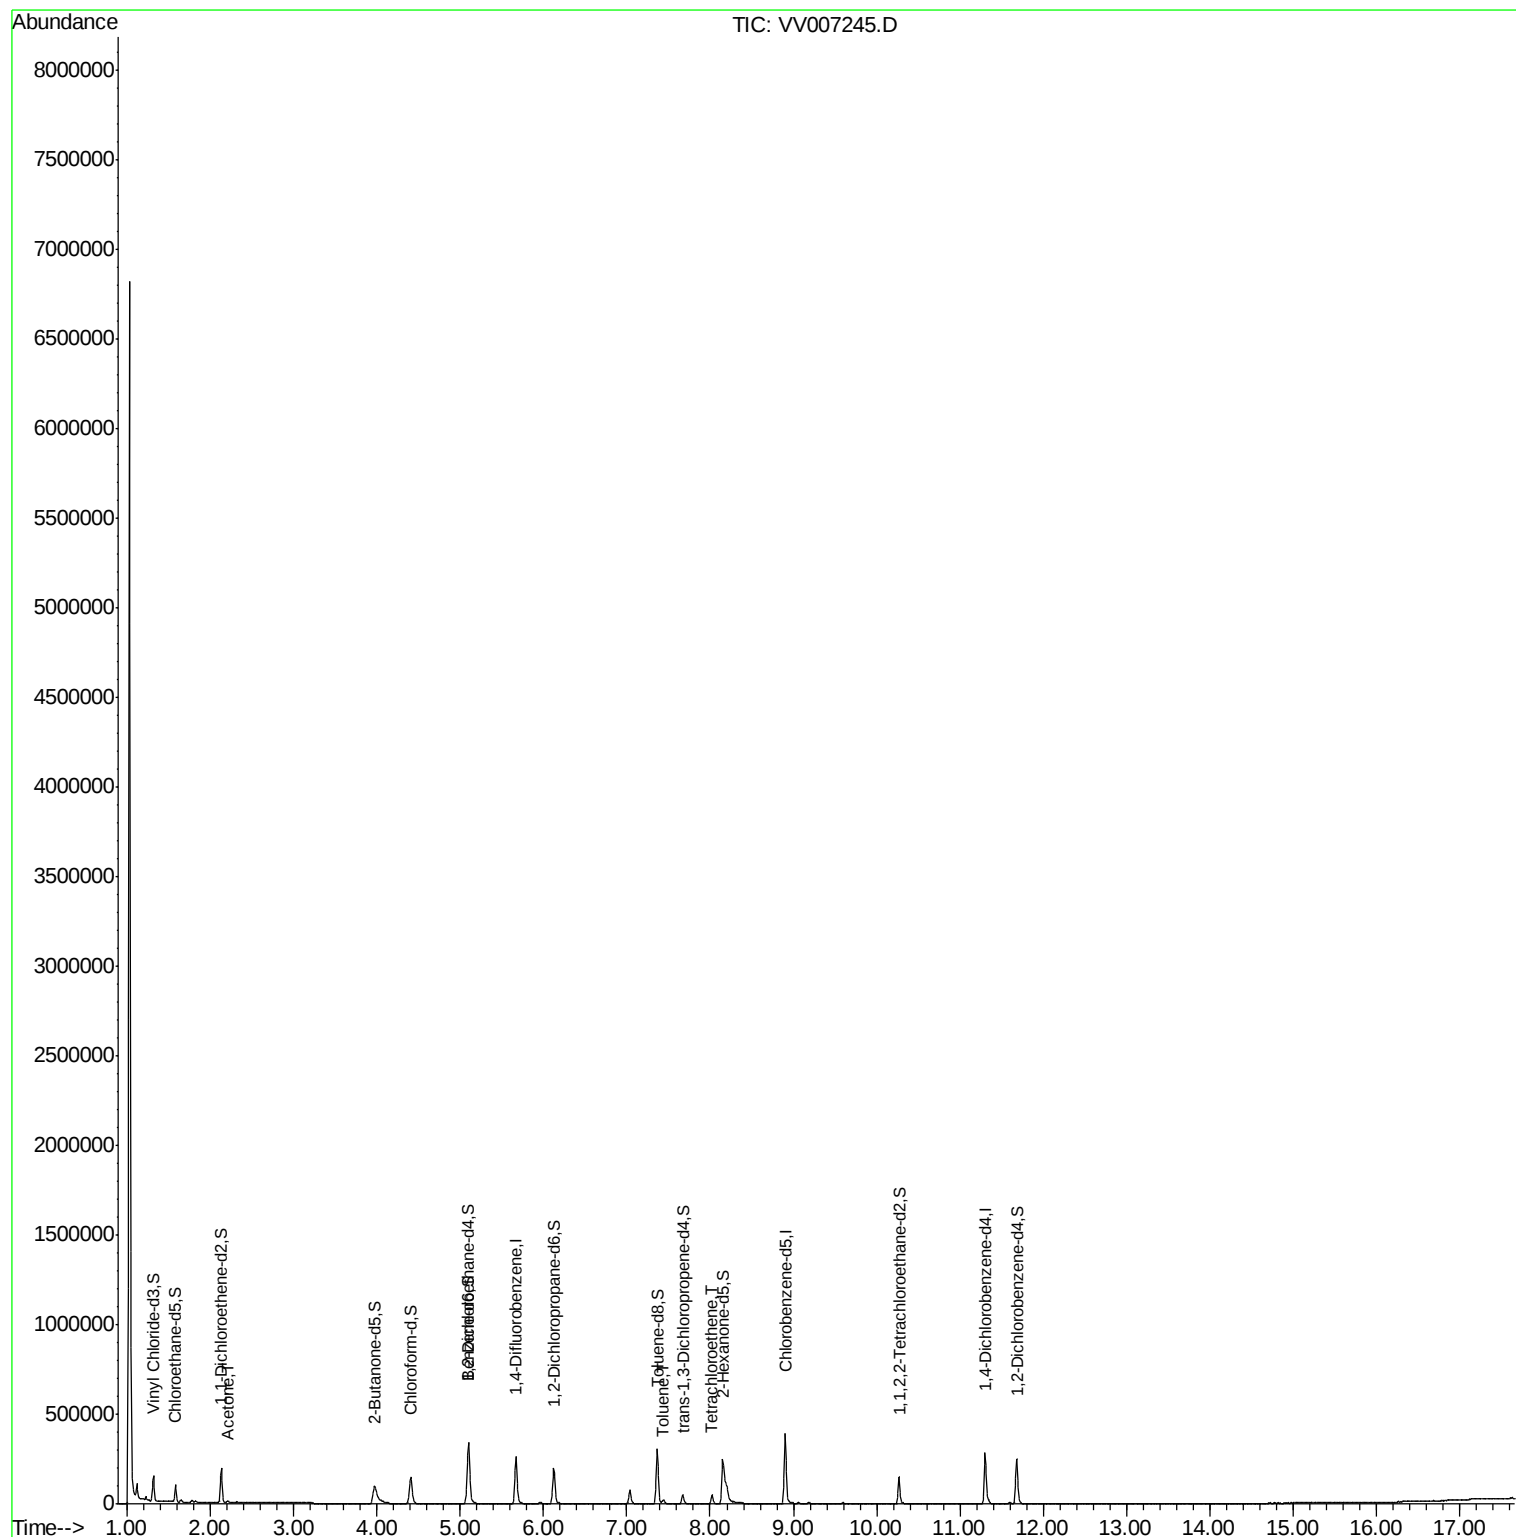

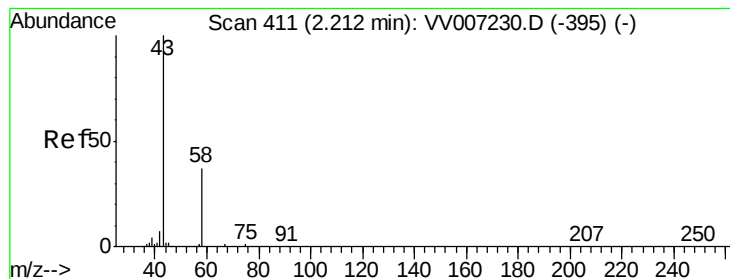

#13

Acetone

Concen: 3.20 ug/L

RT: 2.21 min Scan# 410

Delta R.T. -0.00 min

Lab File: VV007245.D

Acq: 29 Aug 2018 01:51

Instrument :

MSVOA_V

ClientSampleId :


GAB76

Tot Ion: 43 Resp: 6562

Ion Ratio Lower Upper




43 100

58 51.5 0.0 70.2

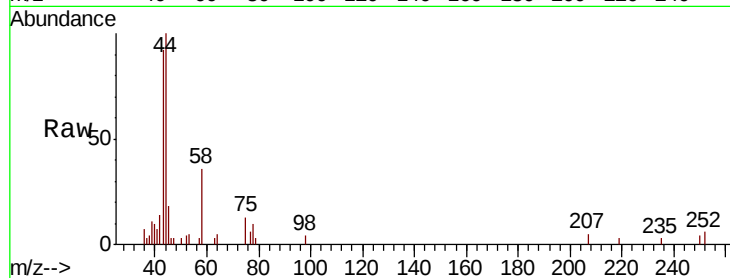

Abundance Ion 43.05 (42.75 to 43.75): VV007230.D (-395) (-)

Ion 58.05 (57.75 to 58.75): VV007230.D (-395) (-)

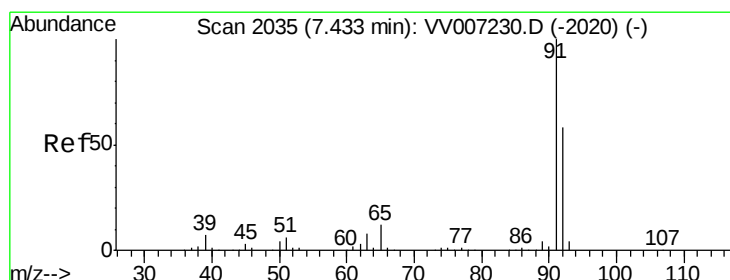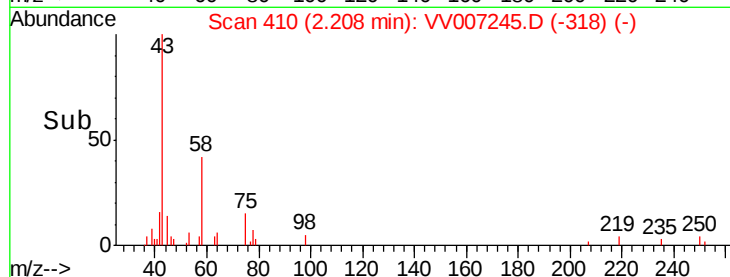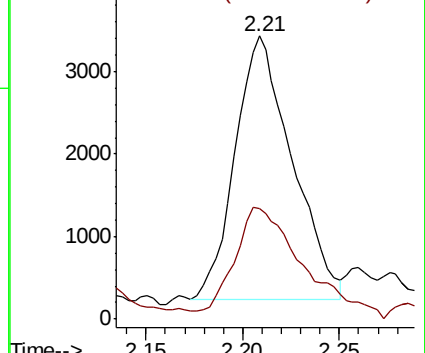

#42

Toluene

Concen: 0.22 ug/L

RT: 7.44 min Scan# 2036

Delta R.T. 0.00 min

Lab File: VV007245.D


Acq: 29 Aug 2018 01:51

Tgt Ion: 91 Resp: 15036

Ion Ratio Lower Upper



91 100


92 57.8 41.1 76.3

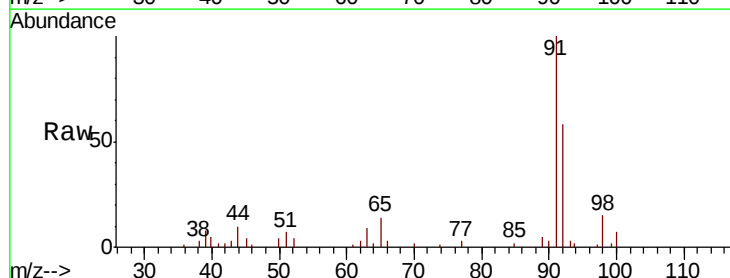

Abundance Ion 91.15 (90.85 to 91.85): VV007230.D (-2020) (-)

Ion 92.15 (91.85 to 92.85): VV007230.D (-2020) (-)

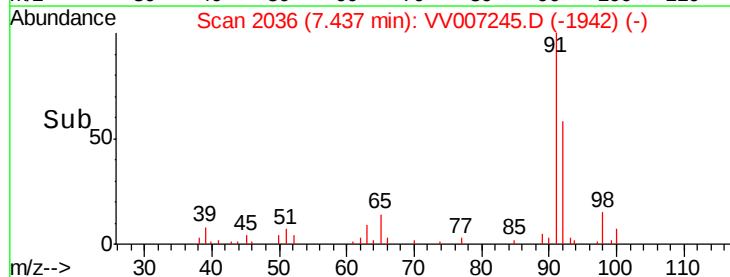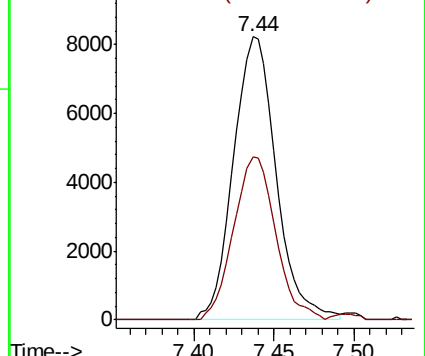

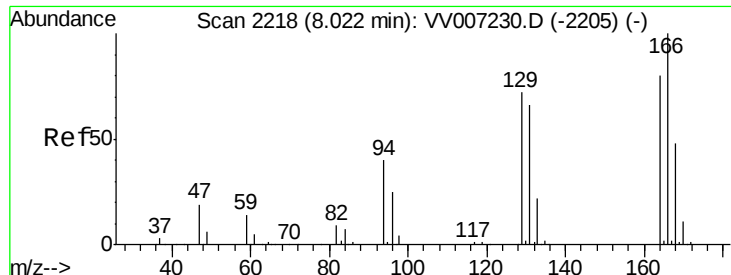

#47

Tetrachloroethene

Concen: 0.81 ug/L


RT: 8.02 min Scan# 2218

Delta R.T. -0.00 min

Lab File: VV007245.D

Acq: 29 Aug 2018 01:51

Instrument :
MSVOA_V
ClientSampleId :
GAB76

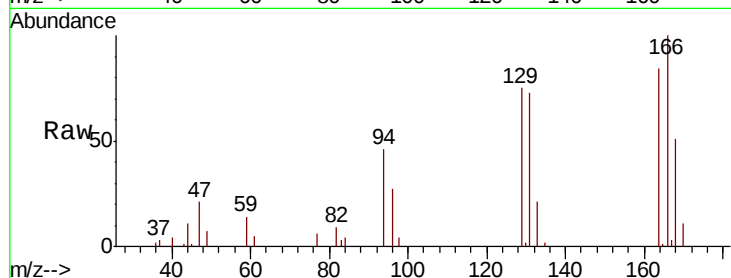

Tot Ion:164 Resp: 11879

Ion Ratio Lower Upper

164 100

129 89.0 62.7 116.5

131 86.8 60.1 111.7

166 118.5 86.4 160.4

Abundance Ion 163.90 (163.60 to 164.60): V
Ion 128.95 (128.65 to 129.65): V
Ion 130.95 (130.65 to 131.65): V
Ion 165.90 (165.60 to 166.60): V

