


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082818\
 Data File : VV007220.D
 Acq On : 28 Aug 2018 09:04
 Operator : SY/MD
 Sample : BFB67
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB67

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082818WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Aug 29 04:00:48 2018

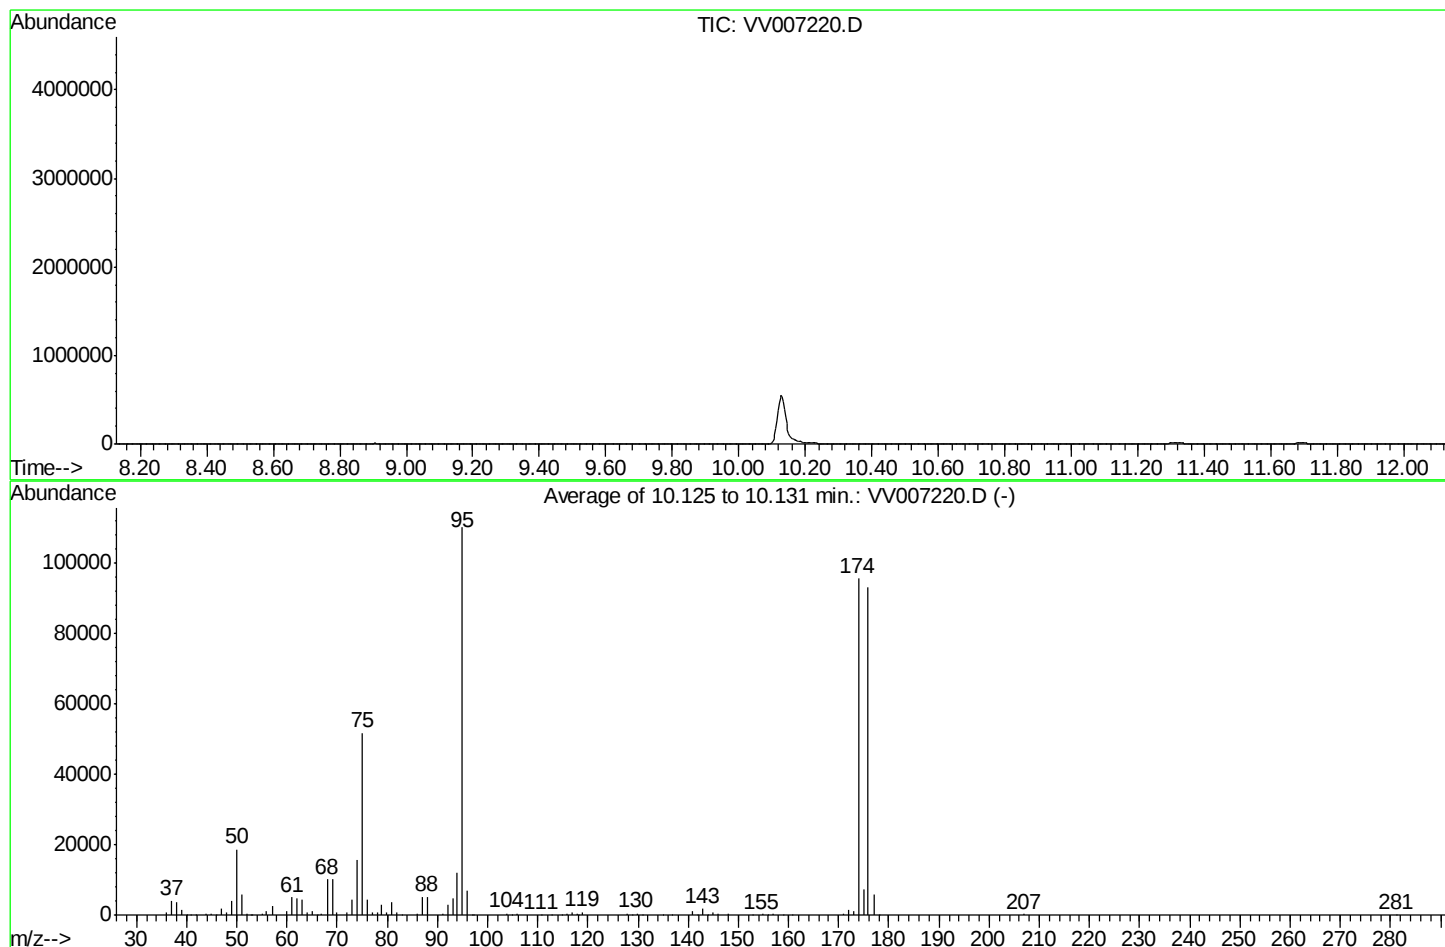

AutoFind: Scans 2872, 2873, 2874; Background Corrected with Scan 2858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	18704	PASS
75	95	30	80	46.9	51677	PASS
95	95	100	100	100.0	110157	PASS
96	95	5	9	6.3	6950	PASS
173	174	0.00	2	1.0	979	PASS
174	95	50	120	86.7	95506	PASS
175	174	5	9	7.5	7148	PASS
176	174	95	101	97.4	93000	PASS
177	176	5	9	6.1	5657	PASS

Scan 2858 (10.080 min): VV007220.D
BFB67

m/z	Abundance
39.90	469.0
44.00	1065.0
44.90	137.0
76.90	100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
36.00	627.0
37.00	4039.0
38.00	3701.0
39.00	1463.0
40.00	622.0
43.90	1524.0
45.00	620.0
45.90	143.0
46.90	1699.0
48.00	590.0
49.00	3821.0
50.00	18608.0
51.00	5924.0
51.90	270.0
52.90	308.0
55.10	353.0
55.90	1296.0
57.00	2331.0
60.00	1022.0
61.00	4841.0
62.00	4434.0
63.00	4288.0
64.00	740.0
65.10	1067.0
66.90	300.0
68.00	9801.0
69.00	10073.0
70.00	830.0
71.90	703.0
73.00	4344.0
74.00	16024.0
75.00	51096.0
76.00	4469.0
76.90	866.0
78.10	720.0
78.90	3015.0
79.90	846.0
80.90	3733.0
82.00	676.0
82.80	107.0
85.80	224.0
86.90	4848.0
88.00	4702.0
91.00	291.0
92.00	3217.0
93.00	4501.0
94.00	11867.0
95.00	109952.0
96.00	7076.0
96.80	232.0
103.90	424.0
104.80	132.0
105.80	374.0
110.80	111.0
114.70	107.0
115.90	321.0
116.90	593.0
117.90	458.0
118.90	892.0
127.80	301.0
129.00	126.0
129.80	326.0
130.80	119.0
134.90	183.0
136.90	131.0
140.90	825.0
142.90	1852.0
145.00	673.0
145.80	212.0
147.90	287.0
152.90	122.0
154.90	318.0
157.00	271.0
160.80	140.0
170.90	377.0
171.90	1650.0
172.90	929.0
173.90	92960.0
175.00	7307.0
175.90	90432.0
176.90	5534.0
178.00	169.0
207.00	220.0
281.20	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
36.00	694.0
37.00	4079.0
38.00	3931.0
39.00	1587.0
40.00	601.0
40.80	142.0
43.90	1642.0
45.10	696.0
45.80	187.0
47.00	1737.0
48.00	637.0
49.00	3989.0
50.00	19168.0
51.00	5802.0
51.90	252.0
52.90	229.0
55.00	337.0
55.90	1321.0
57.00	2496.0
60.00	1096.0
61.00	5238.0
62.00	4777.0
63.00	4487.0
64.00	765.0
65.00	1047.0
66.10	107.0
66.90	327.0
68.00	10241.0
69.00	10476.0
70.00	839.0
71.90	696.0
73.00	4451.0
74.00	16191.0
75.00	53080.0
76.00	4438.0
77.00	826.0
78.10	735.0
78.90	3148.0
79.90	854.0
80.90	3870.0
82.00	765.0
82.80	144.0
85.80	266.0
86.90	4971.0
87.90	5175.0
90.90	295.0
92.00	3190.0
93.00	4760.0
94.00	12495.0
95.00	112888.0
96.00	7061.0
96.90	223.0
103.90	446.0
104.80	126.0
105.80	423.0
115.90	399.0
116.90	697.0
117.90	349.0
118.90	937.0
127.80	358.0
128.90	153.0
129.80	426.0
130.80	117.0
134.90	197.0
136.90	151.0
141.00	992.0
142.90	1830.0
143.90	111.0
145.00	672.0
145.80	261.0
147.90	214.0
152.80	116.0
154.90	336.0
157.00	235.0
160.80	147.0
170.90	347.0
171.90	1612.0
172.90	978.0
173.90	97904.0
175.00	7322.0
175.90	95424.0
177.00	5729.0
178.00	192.0
207.00	220.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67

m/z	Abundance
36.00	790.0
37.00	3910.0
38.00	3684.0
39.00	1551.0
40.00	540.0
40.90	182.0
41.90	122.0
43.90	1606.0
45.10	764.0
45.80	183.0
47.00	1692.0
48.00	612.0
49.00	3774.0
50.00	18336.0
51.00	5459.0
51.90	237.0
53.10	133.0
55.00	252.0
56.00	1244.0
57.00	2542.0
60.00	1002.0
61.00	5055.0
62.00	4769.0
63.00	4321.0
64.00	666.0
65.00	1041.0
66.10	132.0
66.90	318.0
68.00	10029.0
69.00	10360.0
70.00	752.0
71.90	663.0
73.00	4331.0
74.00	15289.0
75.00	50856.0
76.00	4138.0
77.10	820.0
78.00	581.0
78.90	3132.0
79.90	849.0
80.90	3541.0
82.00	771.0
82.80	148.0
85.90	271.0
86.90	4969.0
87.90	5523.0
90.90	294.0
92.00	2850.0
93.00	4760.0
94.00	11974.0
95.00	107632.0
96.00	6715.0
97.20	221.0
103.90	454.0
104.80	122.0
105.80	387.0
112.70	126.0
115.90	414.0
116.90	771.0
118.10	273.0
118.90	833.0
127.80	354.0
128.80	157.0
129.80	437.0
130.80	143.0
134.90	201.0
136.80	149.0
141.00	1052.0
141.80	109.0
142.90	1563.0
143.90	128.0
145.00	640.0
145.90	267.0
147.90	190.0
152.80	111.0
154.80	310.0
155.80	118.0
157.00	194.0
159.00	106.0
160.90	162.0
171.00	293.0
171.90	1565.0
172.90	1031.0
173.90	95656.0
174.90	6815.0
175.90	93144.0
176.90	5708.0
178.00	174.0
207.00	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB67