


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV082819\
 Data File : VV012430.D
 Acq On : 28 Aug 2019 17:46
 Operator : SY/MD
 Sample : BFB55
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB55

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082819WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Aug 29 02:14:42 2019

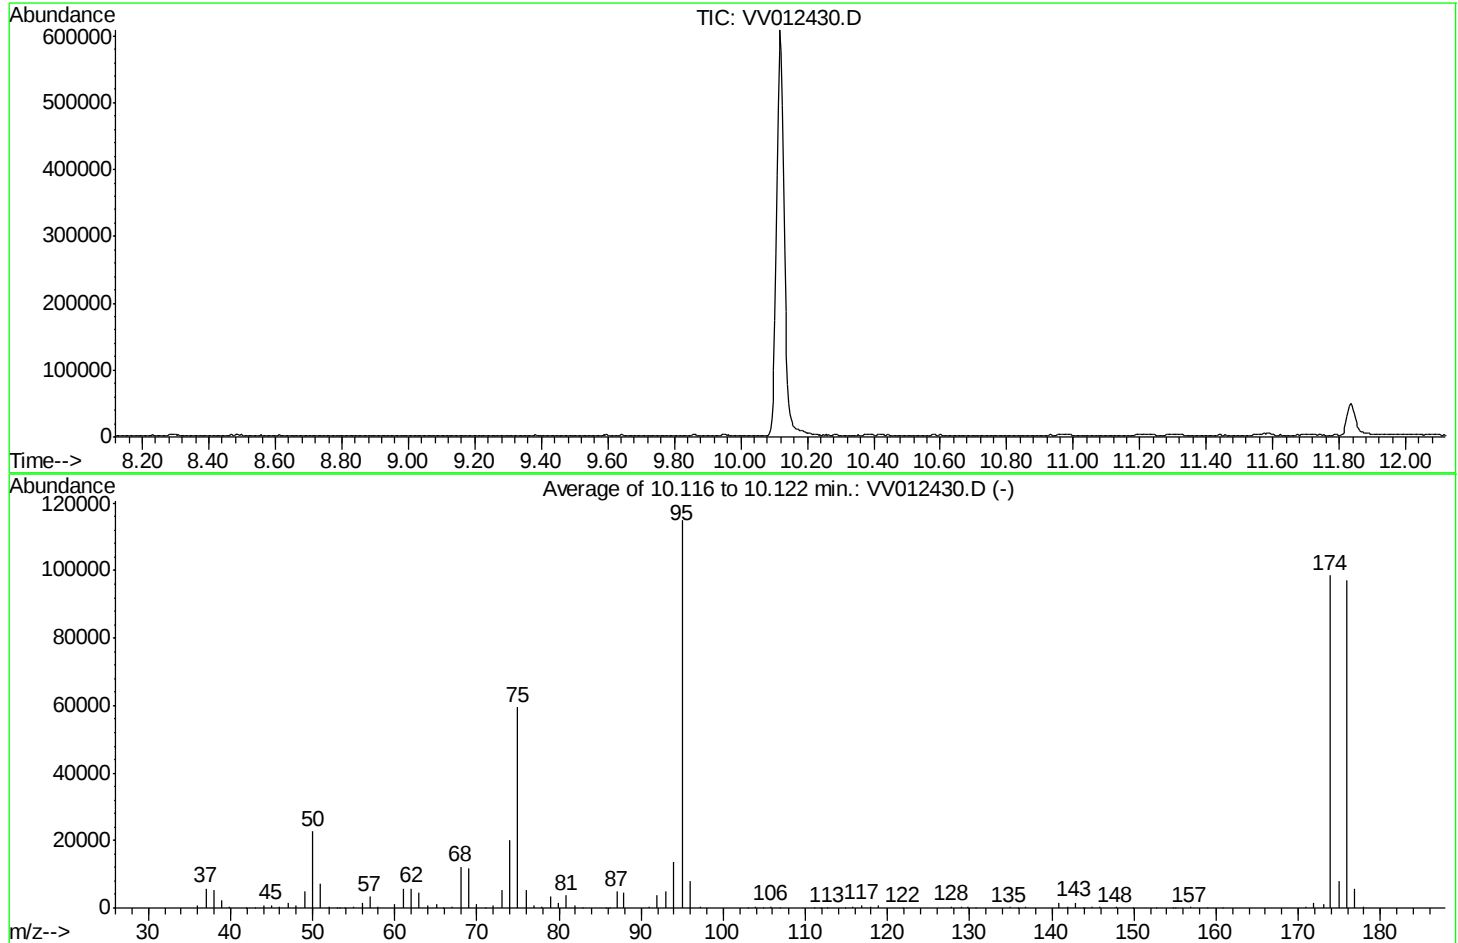

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	22656	PASS
75	95	30	80	51.7	59392	PASS
95	95	100	100	100.0	114904	PASS
96	95	5	9	7.1	8135	PASS
173	174	0.00	2	1.2	1221	PASS
174	95	50	120	85.7	98482	PASS
175	174	5	9	8.0	7910	PASS
176	174	95	101	98.8	97314	PASS
177	176	5	9	5.9	5713	PASS

m/z	Abundance
36.00	1034.0
37.00	5959.0
38.00	5347.0
39.00	2525.0
40.00	1170.0
41.80	148.0
43.10	109.0
44.00	1341.0
45.00	1091.0
46.00	282.0
47.00	1518.0
47.90	645.0
49.00	5035.0
50.00	23072.0
51.00	7226.0
52.10	384.0
52.90	118.0
53.30	103.0
53.90	130.0
55.00	424.0
56.00	1580.0
57.00	3311.0
58.00	237.0
59.90	1078.0
61.00	5595.0
62.00	5731.0
63.00	4766.0
64.00	802.0
65.10	1134.0
65.90	167.0
66.90	449.0
68.00	12294.0
69.00	11495.0
70.00	1076.0
72.00	622.0
73.00	5310.0
74.00	19888.0
75.00	59296.0
76.00	5212.0
77.00	892.0
77.90	497.0
78.90	3839.0
79.90	1237.0
80.90	3579.0
81.90	972.0
85.70	143.0
87.00	4668.0
87.90	4522.0
90.90	472.0
91.90	3472.0
93.00	5077.0
94.00	13813.0
95.00	113576.0
96.00	7935.0
97.20	231.0
103.90	395.0
104.90	141.0
105.80	424.0
106.80	176.0
111.00	160.0
111.90	111.0
112.60	130.0
114.80	123.0
115.80	477.0
116.90	1019.0
117.90	412.0
118.90	713.0
121.90	103.0
127.80	489.0
129.00	216.0
129.80	486.0
130.80	141.0
134.90	253.0
135.80	171.0
136.90	258.0
140.90	1331.0
141.90	254.0
142.90	1631.0
143.80	148.0
144.00	128.0
144.80	473.0
145.80	237.0
147.80	308.0
149.80	159.0
152.70	127.0
155.00	281.0
156.90	248.0
158.80	144.0
160.80	131.0
170.90	249.0
171.90	1675.0
173.10	1813.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

173.90	95160.0
174.90	7713.0
175.90	94000.0
176.90	5602.0
177.90	184.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
36.00	1036.0
37.00	6112.0
38.00	5307.0
39.00	2461.0
39.90	1171.0
41.90	166.0
42.90	104.0
44.00	1420.0
45.00	1053.0
46.00	229.0
47.00	1658.0
48.00	647.0
49.00	5093.0
50.00	23528.0
51.00	7402.0
52.10	316.0
52.90	171.0
53.80	154.0
55.00	402.0
56.00	1723.0
57.00	3482.0
58.00	246.0
59.90	1208.0
61.00	5747.0
62.00	6016.0
63.00	4873.0
64.00	915.0
65.10	1211.0
65.90	178.0
66.90	442.0
68.00	12635.0
69.00	11908.0
70.00	1000.0
71.00	111.0
71.90	629.0
73.00	5536.0
74.00	20736.0
75.00	61552.0
76.00	5385.0
77.00	946.0
77.80	564.0
78.90	3648.0
80.00	1425.0
80.90	3817.0
81.90	973.0
82.90	113.0
85.70	167.0
86.20	240.0
87.00	4984.0
87.90	4475.0
90.90	493.0
92.00	3859.0
93.00	5052.0
94.00	14186.0
95.00	118784.0
96.00	8429.0
97.20	223.0
103.80	389.0
104.90	156.0
105.90	417.0
106.80	138.0
111.10	122.0
111.90	122.0
112.70	136.0
114.80	191.0
115.80	456.0
116.80	984.0
117.90	439.0
118.90	754.0
127.80	519.0
128.90	213.0
129.80	500.0
130.70	107.0
134.90	285.0
135.80	194.0
136.90	261.0
140.90	1519.0
141.90	231.0
142.90	1709.0
143.80	162.0
144.80	554.0
145.80	196.0
147.80	318.0
149.90	167.0
152.70	156.0
155.00	252.0
156.90	282.0
158.90	176.0
160.90	183.0
171.00	234.0
171.90	1777.0
173.10	1850.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

173.90	101592.0
174.90	8221.0
175.90	100488.0
176.90	5875.0
177.90	225.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

m/z	Abundance
36.00	980.0
37.00	5611.0
38.00	4845.0
39.00	2243.0
39.90	1043.0
41.80	188.0
42.80	111.0
44.00	1411.0
44.90	920.0
46.00	179.0
47.00	1680.0
47.90	665.0
49.00	4735.0
50.00	21368.0
51.00	6786.0
52.00	257.0
53.00	204.0
53.80	148.0
55.00	369.0
56.00	1541.0
57.00	3236.0
58.00	218.0
59.90	1139.0
61.00	5479.0
62.00	5619.0
63.00	4512.0
64.00	916.0
65.00	1152.0
65.90	172.0
66.90	386.0
68.00	11629.0
69.00	11440.0
70.00	854.0
71.90	598.0
73.00	5290.0
74.00	19632.0
75.00	57328.0
76.00	4986.0
77.00	866.0
77.80	580.0
78.90	3174.0
80.00	1381.0
80.90	3739.0
81.90	899.0
82.90	162.0
86.10	272.0
87.00	4798.0
87.90	4178.0
90.90	532.0
92.00	3731.0
92.90	4853.0
94.00	13439.0
95.00	112352.0
96.00	8043.0
97.20	163.0
103.00	104.0
103.80	367.0
104.90	146.0
105.90	430.0
106.90	110.0
111.90	117.0
112.70	145.0
114.80	272.0
115.80	435.0
116.80	846.0
117.90	428.0
118.80	691.0
127.80	451.0
128.90	232.0
129.80	430.0
134.80	274.0
135.80	164.0
136.80	209.0
140.90	1446.0
142.00	162.0
142.80	1508.0
143.80	132.0
144.90	566.0
145.90	202.0
147.80	317.0
149.90	164.0
152.70	156.0
154.70	237.0
156.80	285.0
158.80	186.0
160.90	176.0
171.00	229.0
171.90	1686.0
173.90	98696.0
174.90	7798.0
175.90	97456.0
176.90	5662.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55

177.90

230.0

Instrument :

MSVOA_V

ClientSampleId :

BFB55

Scan 2794 (10.074 min): VV012430.D
BFB55

m/z	Abundance
36.10	133.0
39.90	831.0
41.10	125.0
44.00	579.0
45.00	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB55