

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082820\
 Data File : VV018137.D
 Acq On : 28 Aug 2020 15:30
 Operator : SY/MD
 Sample : L3800-21
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3J3

Quant Time: Aug 29 01:38:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 29 00:38:30 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	263403	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	261190	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	127230	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	80225	39.92	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.84%
7) Chloroethane-d5	1.58	69	74236	45.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	90.30%
11) 1,1-Dichloroethene-d2	2.12	63	130263	33.88	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.76%
21) 2-Butanone-d5	3.91	46	125873	95.63	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.63%
24) Chloroform-d	4.38	84	163253	44.62	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.24%
26) 1,2-Dichloroethane-d4	5.06	65	115108	48.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.88%
32) Benzene-d6	5.08	84	330589	45.93	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.86%
36) 1,2-Dichloropropane-d6	6.09	67	111659	47.45	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.90%
41) Toluene-d8	7.34	98	289936	44.79	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.58%
43) trans-1,3-Dichloropropene-	7.64	79	50392	47.21	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.42%
47) 2-Hexanone-d5	8.11	63	68953	91.31	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.31%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	142965	46.65	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.30%
64) 1,2-Dichlorobenzene-d4	11.65	152	127647	50.98	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.96%

Target Compounds


					Ovalue
5) Vinyl chloride	1.32	62	8219	3.512 ug/L #	38
12) 1,1-Dichloroethene	2.13	96	7538	4.266 ug/L #	1
17) trans-1,2-Dichloroethene	2.78	96	2297	1.265 ug/L	88
18) Methyl tert-butyl Ether	2.79	73	33828	5.632 ug/L	99
20) cis-1,2-Dichloroethene	3.94	96	477632	239.305 ug/L	98
25) Chloroform	4.41	83	8589	2.306 ug/L	100
34) Trichloroethene	5.94	95	336526	157.550 ug/L	98
46) Tetrachloroethene	8.00	164	508702	324.734 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV082820\
Data File : VV018137.D
Acq On : 28 Aug 2020 15:30
Operator : SY/MD
Sample : L3800-21
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3J3

Quant Time: Aug 29 01:38:33 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 29 00:38:30 2020
Response via : Initial Calibration

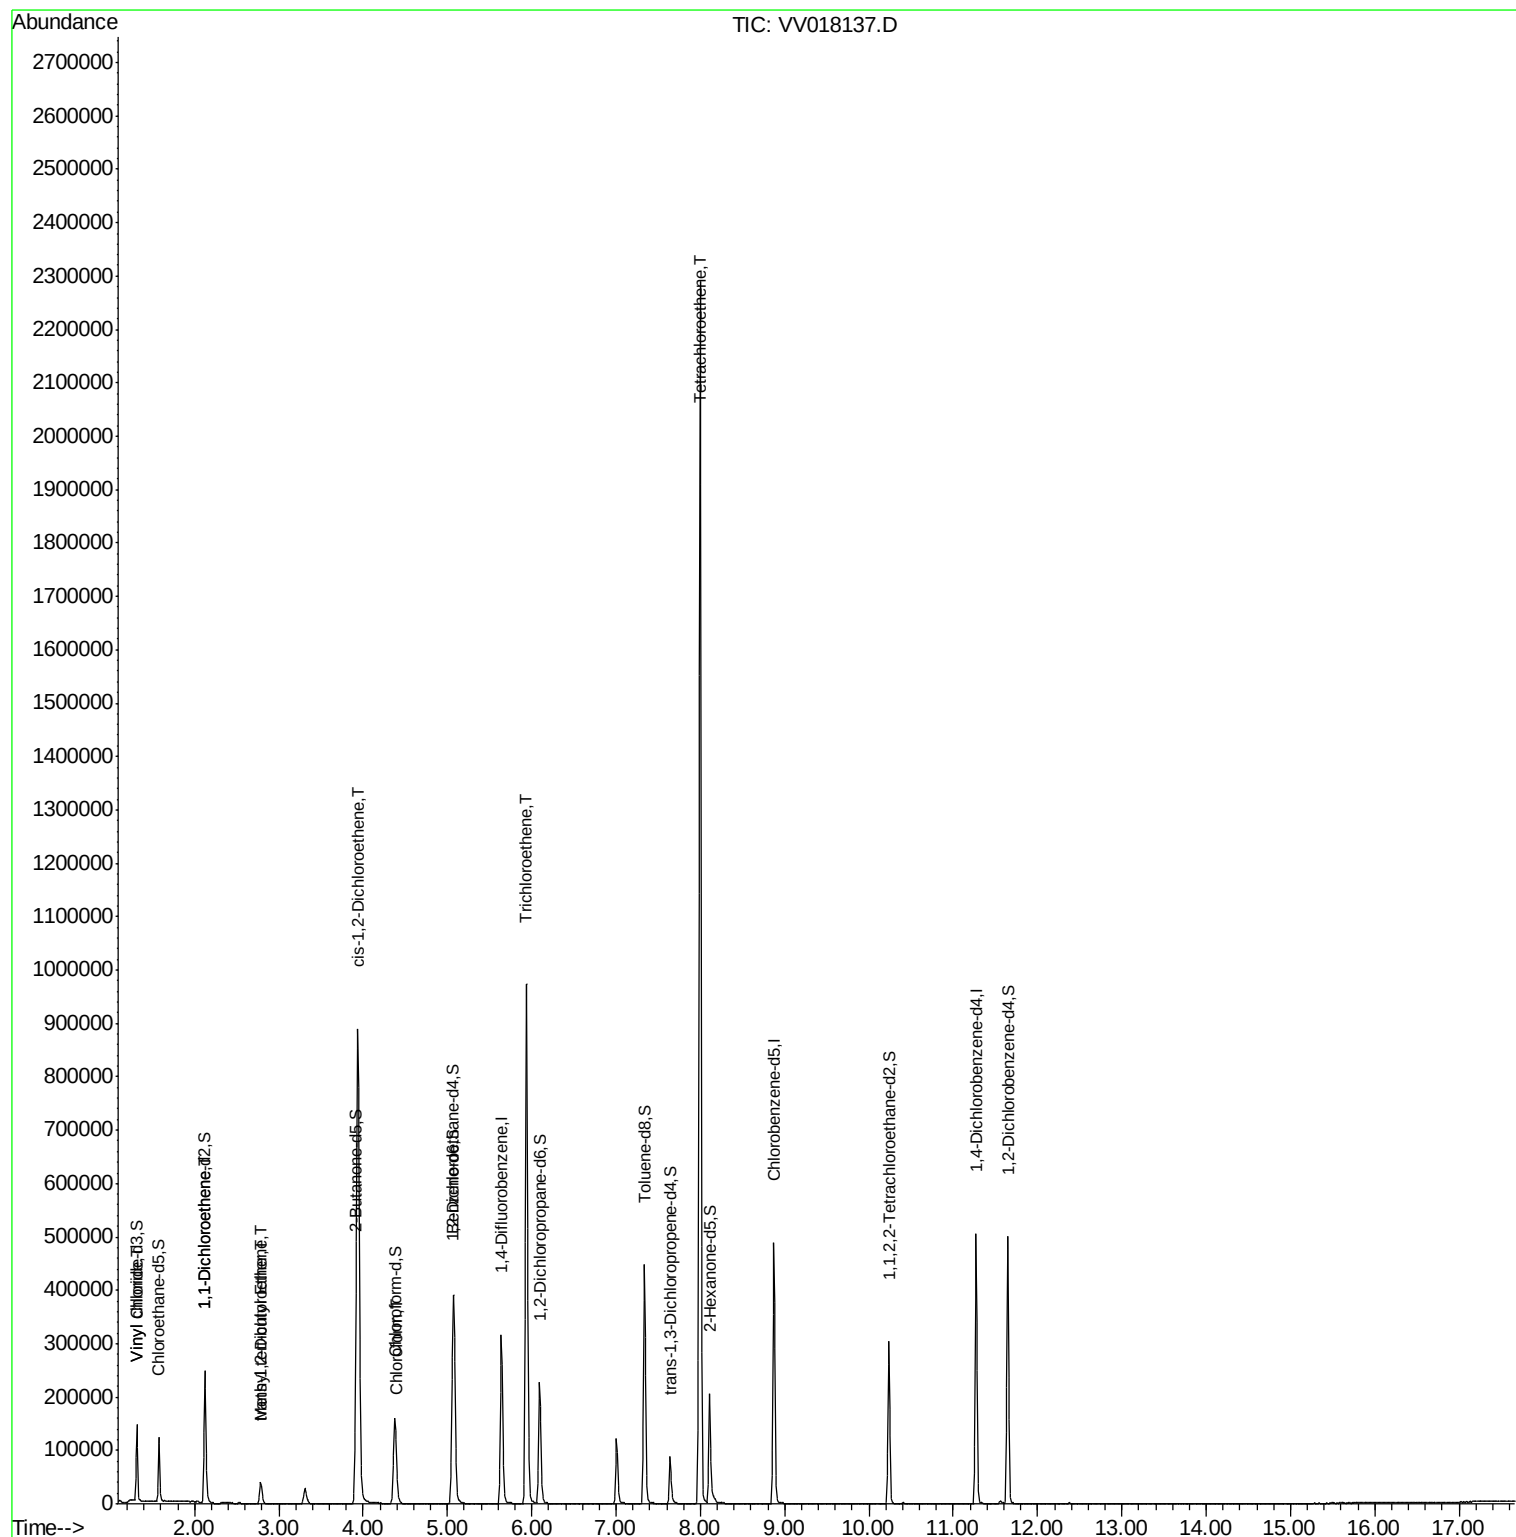

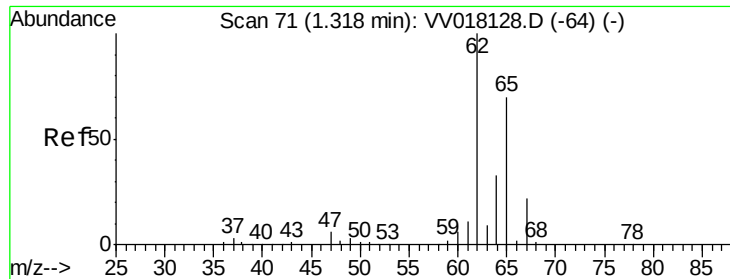

#5

Vinyl chloride

Concen: 3.512 ug/L

RT: 1.32 min Scan# 71

Delta R.T. 0.00 min

Lab File: VV018137.D

Acq: 28 Aug 2020 15:30

Instrument :

MSVOA_V

ClientSampled :





BG3J3

Tot Ion: 62 Resp: 8219

Ion Ratio Lower Upper

62 100

64 66.4 22.4 41.6#

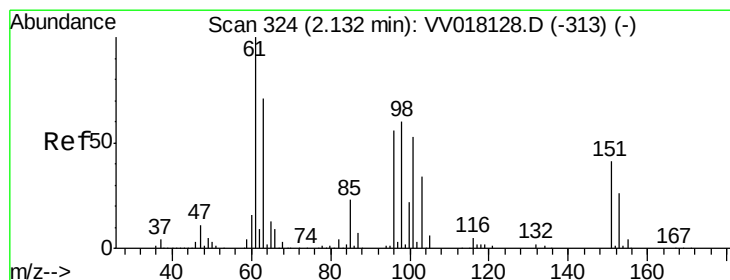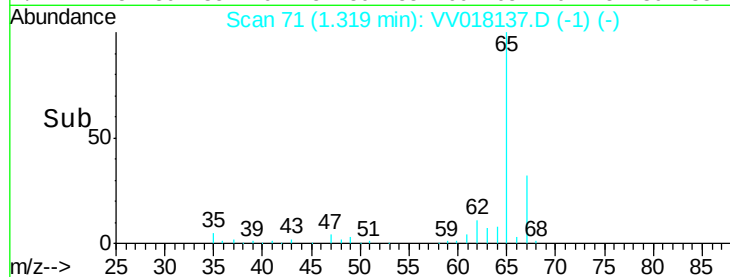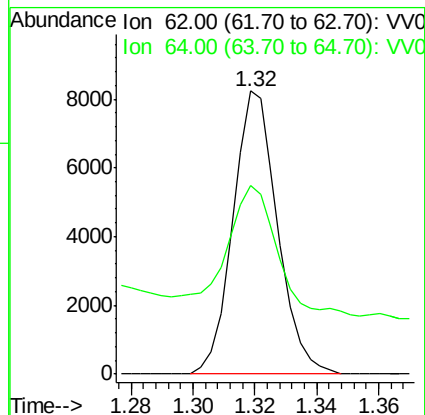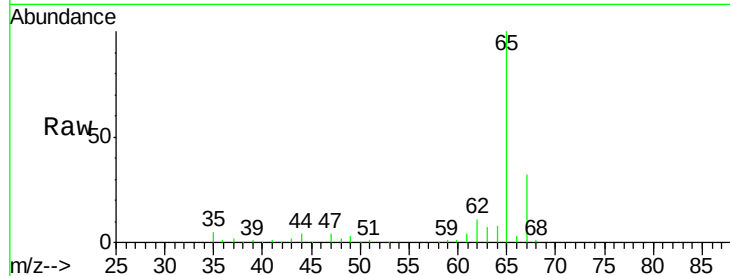

#12

1,1-Dichloroethene

Concen: 4.266 ug/L

RT: 2.13 min Scan# 324

Delta R.T. 0.00 min

Lab File: VV018137.D

Acq: 28 Aug 2020 15:30




Tgt Ion: 96 Resp: 7538


Ion Ratio Lower Upper

96 100

61 277.2 127.1 236.0#

63 1145.3 95.2 176.8#

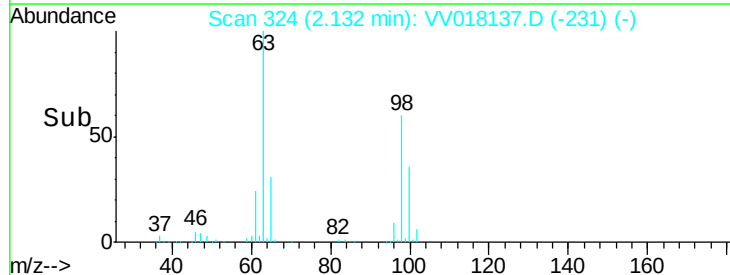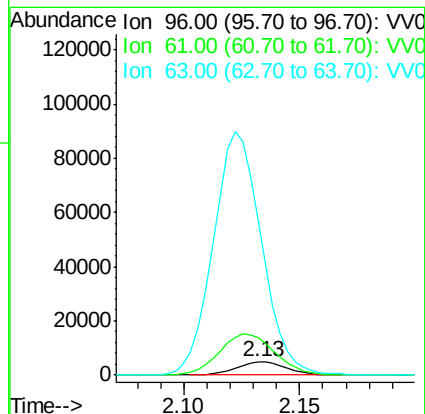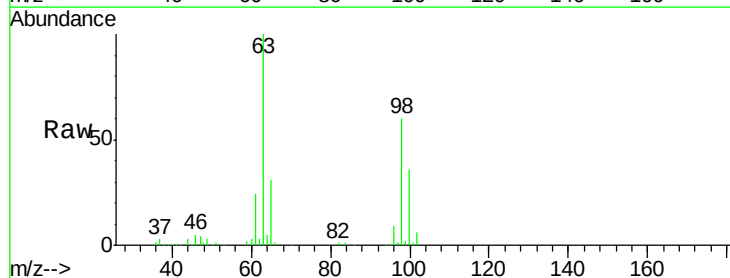

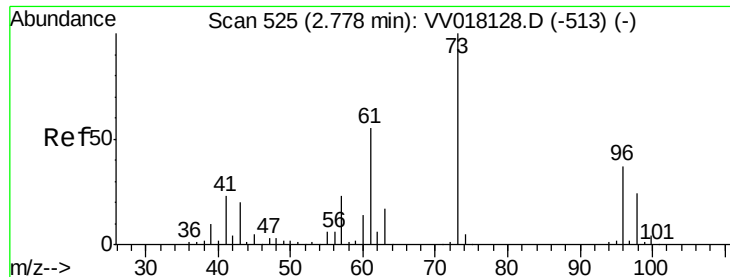

#17

trans-1,2-Dichloroethene

Concen: 1.265 ug/L

RT: 2.78 min Scan# 527

Delta R.T. 0.01 min

Lab File: VV018137.D

Acq: 28 Aug 2020 15:30

Instrument :


MSVOA_V

ClientSampleId :

BG3J3

Tot Ion: 96 Resp: 2297




Ion	Ratio	Lower	Upper
96	100		
61	126.6	102.4	190.2
98	60.0	44.4	82.5

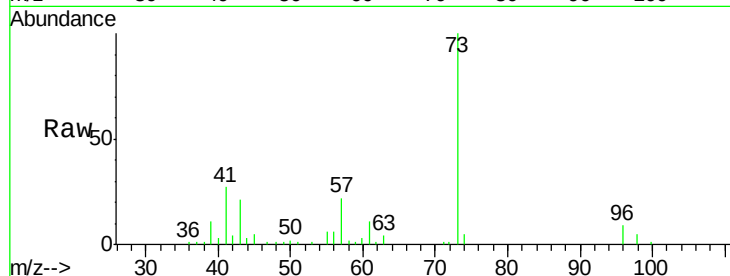

Abundance Ion 96.00 (95.70 to 96.70): VV0

Ion 61.00 (60.70 to 61.70): VV0

Ion 98.00 (97.70 to 98.70): VV0

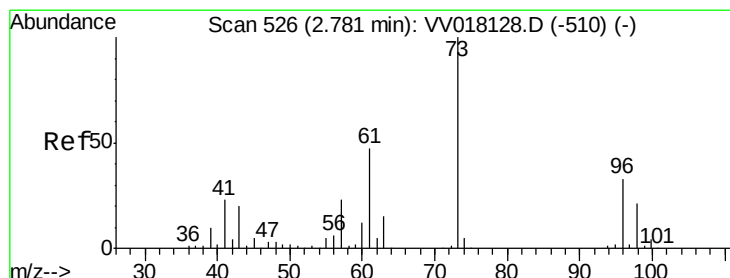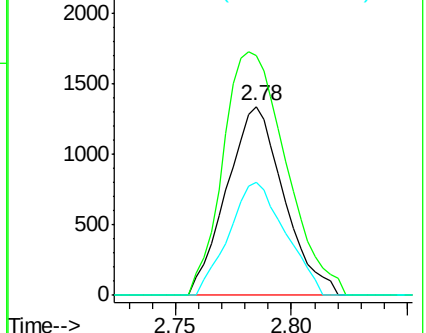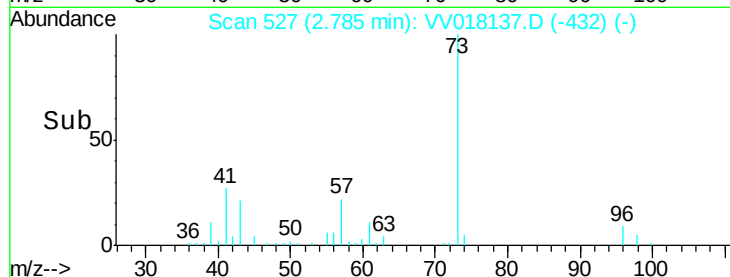

#18

Methyl tert-butyl Ether

Concen: 5.632 ug/L

RT: 2.79 min Scan# 528


Delta R.T. 0.01 min

Lab File: VV018137.D

Acq: 28 Aug 2020 15:30

Tgt Ion: 73 Resp: 33828



Ion	Ratio	Lower	Upper
73	100		
43	19.8	15.9	23.9
57	21.9	18.1	27.1

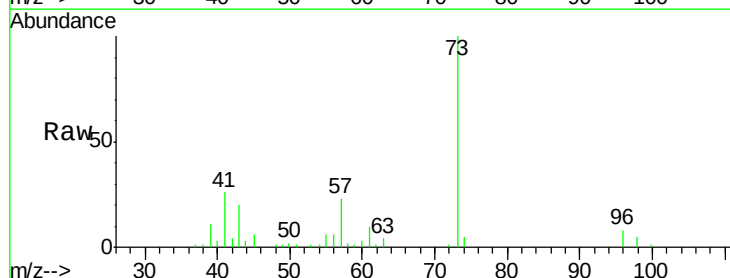


Abundance Ion 73.00 (72.70 to 73.70): VV0

Ion 43.00 (42.70 to 43.70): VV0

Ion 57.00 (56.70 to 57.70): VV0

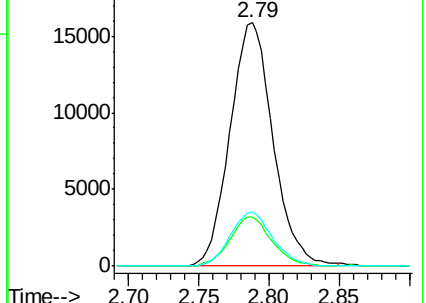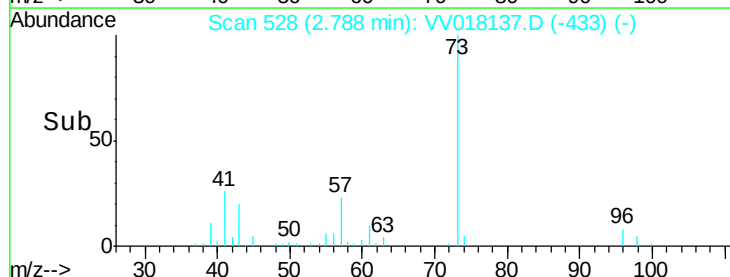




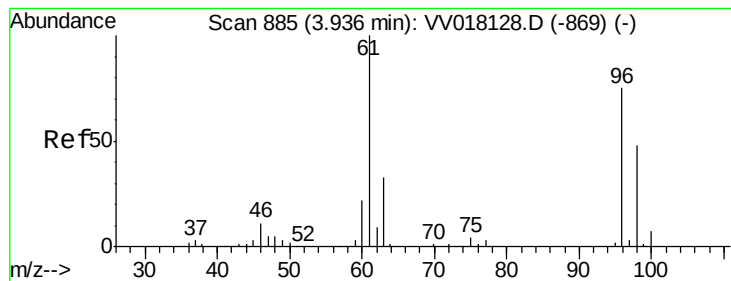


#20

cis-1,2-Dichloroethene
Concen: 239.305 ug/L
RT: 3.94 min Scan# 886
Delta R.T. 0.00 min
Lab File: VV018137.D
Acq: 28 Aug 2020 15:30

Instrument :
MSVOA_V
ClientSampled :
BG3J3




Tot Ion: 96 Resp: 477632
Ion Ratio Lower Upper
96 100
61 133.5 95.0 176.4
68 0.0 0.0 0.0

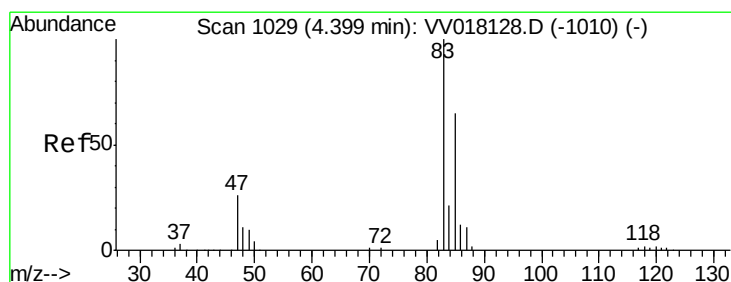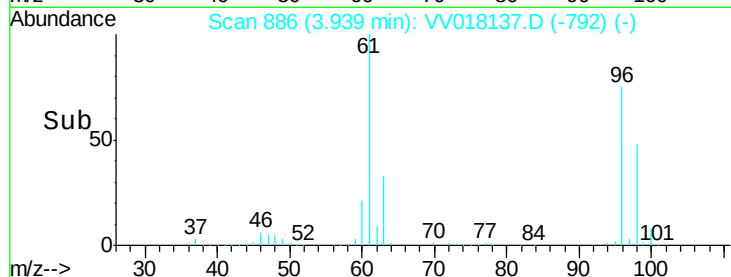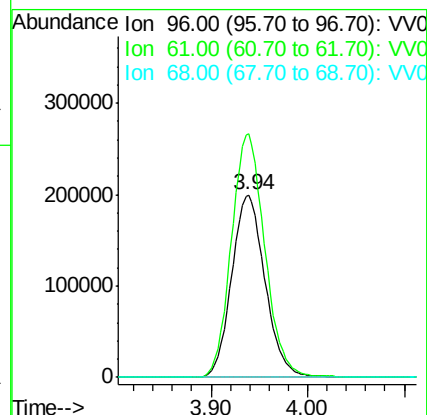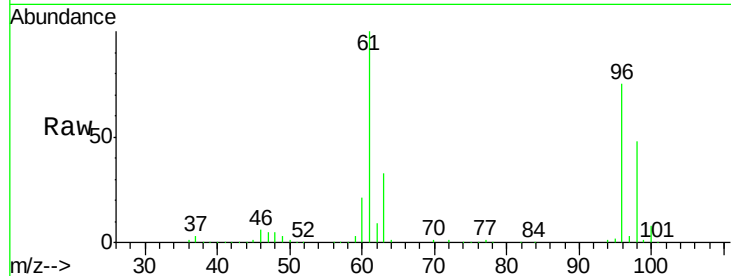


#25

Chloroform
Concen: 2.306 ug/L
RT: 4.41 min Scan# 1031
Delta R.T. 0.01 min
Lab File: VV018137.D
Acq: 28 Aug 2020 15:30

Tgt Ion: 83 Resp: 8589
Ion Ratio Lower Upper
83 100
85 64.6 45.5 84.5

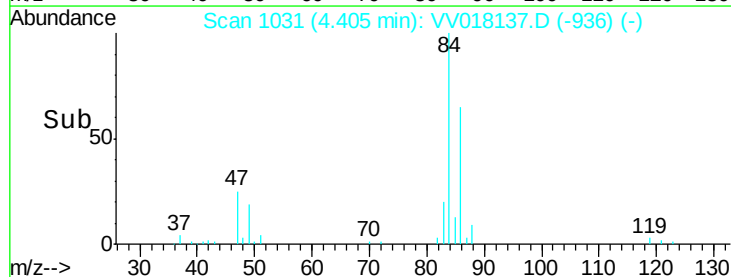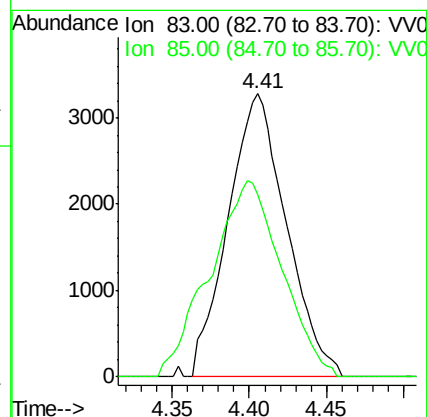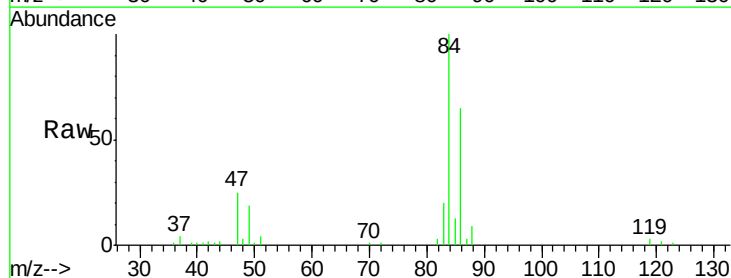

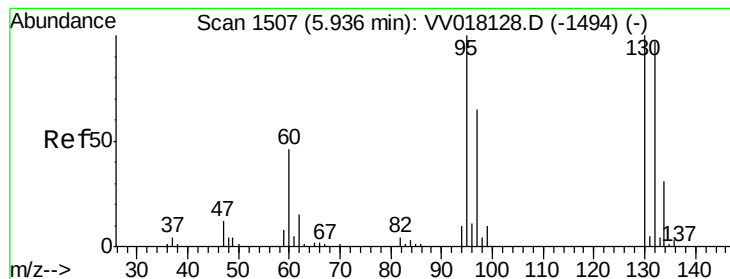

#34

Trichloroethene

Concen: 157.550 ug/L

RT: 5.94 min Scan# 1508

Delta R.T. 0.00 min

Lab File: VV018137.D

Acq: 28 Aug 2020 15:30

Instrument :

MSVOA_V

ClientSampled :

BG3J3

Tot Ion: 95 Resp: 336526


Ion Ratio Lower Upper

95 100

97 64.9 46.0 85.4

132 97.1 65.8 122.2

130 100.9 69.2 128.6



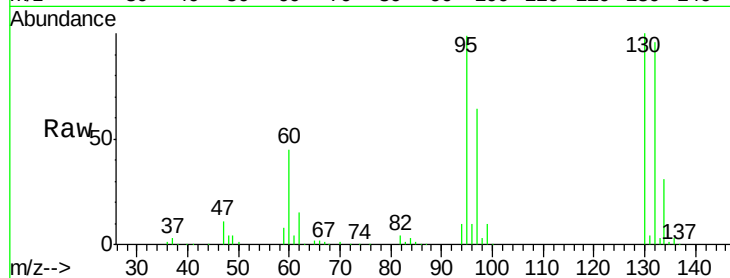


Abundance Ion 95.00 (94.70 to 95.70): VV0

Ion 97.00 (96.70 to 97.70): VV0

Ion 132.00 (131.70 to 132.70): V

Ion 130.00 (129.70 to 130.70): V

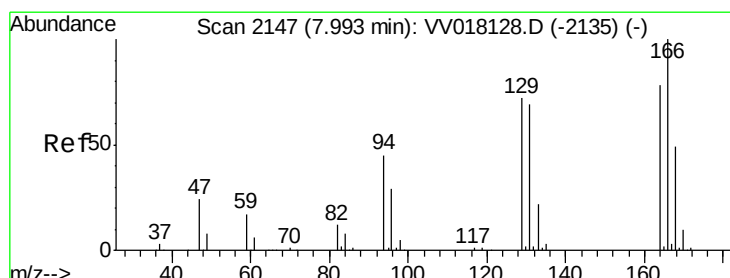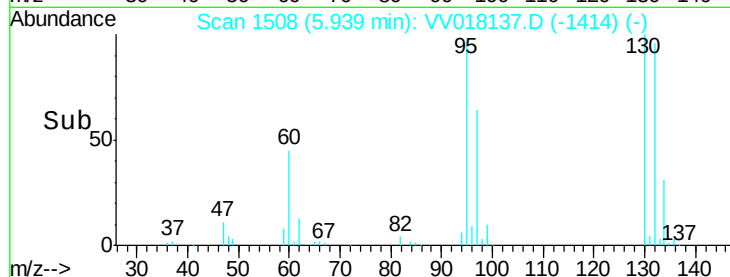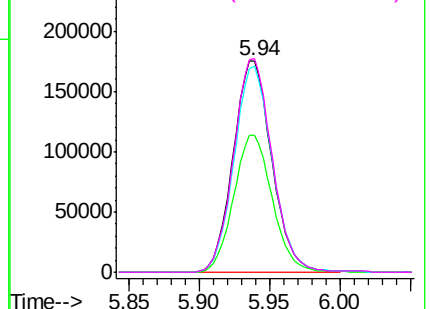

#46

Tetrachloroethene

Concen: 324.734 ug/L

RT: 8.00 min Scan# 2148

Delta R.T. 0.00 min

Lab File: VV018137.D

Acq: 28 Aug 2020 15:30

Tgt Ion: 164 Resp: 508702


Ion Ratio Lower Upper

164 100

129 91.5 64.8 120.3

131 89.2 64.5 119.9

166 127.3 88.9 165.1

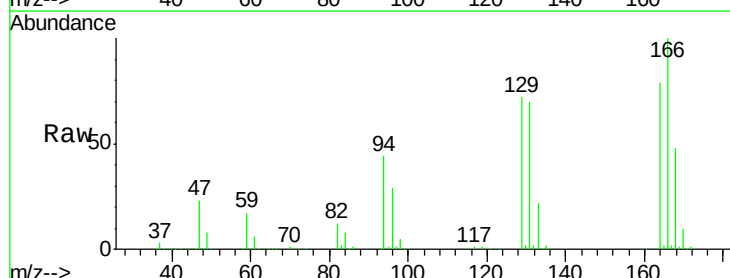

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

