


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV082820\
 Data File : VV018127.D
 Acq On : 28 Aug 2020 09:41
 Operator : SY/MD
 Sample : BFB84
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB84

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis
 Last Update : Sat Aug 29 00:38:30 2020

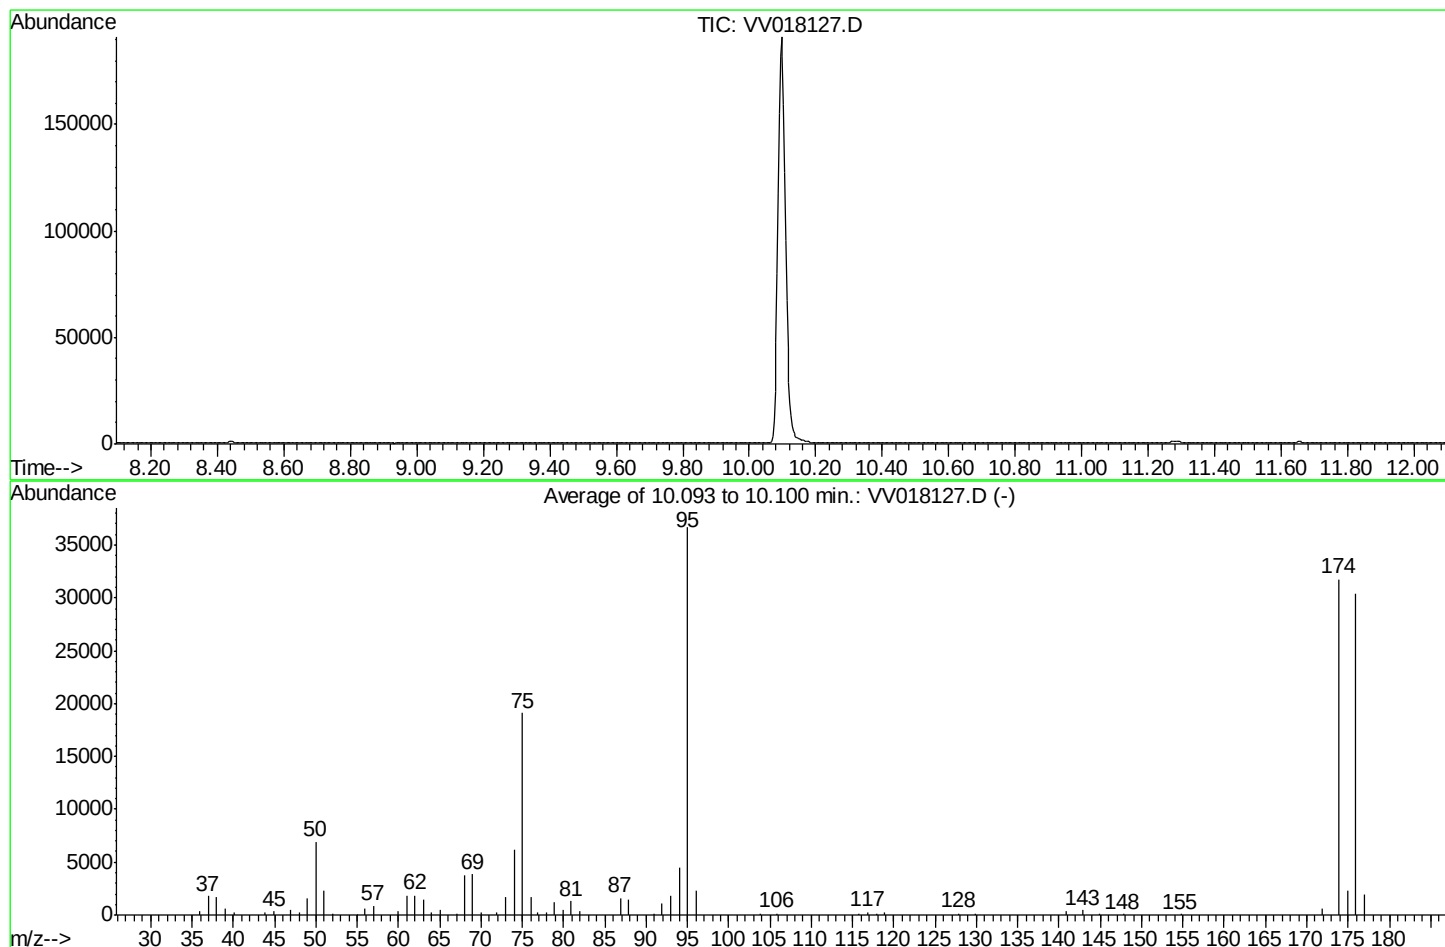

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	6939	PASS
75	95	30	80	52.1	19104	PASS
95	95	100	100	100.0	36674	PASS
96	95	5	9	6.2	2264	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.6	31762	PASS
175	174	5	9	7.2	2298	PASS
176	174	95	101	95.9	30450	PASS
177	176	5	9	6.4	1945	PASS

m/z	Abundance
35.90	371.0
37.00	1777.0
38.00	1810.0
39.10	688.0
40.10	194.0
43.90	563.0
44.90	360.0
46.90	518.0
48.00	270.0
49.00	1620.0
50.00	6809.0
51.00	2308.0
52.00	105.0
56.00	577.0
57.00	846.0
60.00	383.0
61.00	1728.0
62.00	1857.0
63.00	1511.0
63.90	276.0
65.00	504.0
67.00	108.0
68.00	3615.0
69.00	3829.0
69.90	261.0
71.90	237.0
73.00	1793.0
74.00	6002.0
75.00	18840.0
76.00	1703.0
76.90	260.0
78.00	177.0
78.90	1253.0
79.90	438.0
80.90	1289.0
81.90	347.0
86.90	1548.0
87.90	1518.0
91.00	166.0
92.00	1169.0
92.90	1740.0
94.00	4475.0
95.00	36168.0
96.00	2346.0
103.80	172.0
105.90	179.0
115.80	178.0
116.90	269.0
117.80	169.0
118.90	220.0
127.80	139.0
129.90	123.0
140.90	310.0
142.90	486.0
144.90	160.0
154.70	107.0
171.90	626.0
173.90	30496.0
174.90	2308.0
175.90	29552.0
176.90	2090.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
35.00	381.0
37.00	1845.0
38.00	1845.0
39.00	670.0
40.00	225.0
43.90	570.0
45.00	355.0
46.90	504.0
48.00	276.0
49.00	1637.0
50.00	7173.0
51.00	2332.0
52.00	116.0
55.90	573.0
57.00	945.0
59.90	368.0
61.00	1838.0
62.00	1910.0
63.00	1492.0
63.90	303.0
65.00	552.0
67.00	110.0
68.00	3886.0
69.00	3977.0
70.00	257.0
71.80	276.0
73.00	1817.0
74.00	6307.0
75.00	19800.0
76.00	1716.0
76.90	275.0
77.90	206.0
78.90	1278.0
79.90	468.0
80.90	1345.0
81.90	350.0
86.90	1702.0
87.90	1569.0
91.00	186.0
91.90	1197.0
93.00	1839.0
94.00	4536.0
95.00	37760.0
96.00	2296.0
103.80	191.0
105.90	196.0
115.80	176.0
116.90	297.0
117.80	172.0
118.90	257.0
127.80	157.0
129.80	128.0
140.80	337.0
142.90	489.0
144.90	152.0
147.80	116.0
154.80	124.0
171.90	587.0
173.90	32888.0
174.90	2362.0
175.90	31456.0
176.90	1969.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
35.00	328.0
37.00	1722.0
38.00	1588.0
39.00	622.0
40.00	236.0
43.90	546.0
44.90	323.0
46.90	435.0
48.00	232.0
49.00	1458.0
50.00	6836.0
51.00	2128.0
52.00	122.0
55.00	101.0
55.90	513.0
57.00	928.0
59.90	343.0
61.00	1751.0
62.00	1756.0
63.00	1436.0
64.00	286.0
65.00	545.0
68.00	3794.0
69.00	3815.0
70.00	234.0
71.80	286.0
73.00	1651.0
74.00	6058.0
75.00	18672.0
76.00	1551.0
76.90	276.0
77.90	234.0
78.90	1192.0
79.90	443.0
80.90	1245.0
81.90	335.0
86.90	1662.0
87.90	1433.0
91.00	177.0
91.90	1056.0
93.00	1747.0
94.00	4318.0
95.00	36096.0
96.00	2151.0
103.80	181.0
105.90	171.0
115.80	155.0
116.80	276.0
117.90	144.0
118.90	315.0
127.90	151.0
129.80	131.0
140.80	341.0
142.90	463.0
144.90	141.0
147.80	127.0
154.80	122.0
171.90	526.0
173.90	31904.0
174.90	2225.0
175.90	30344.0
176.90	1778.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

Scan 2790 (10.061 min): VV018127.D
BFB84

m/z	Abundance
39.80	151.0
43.90	283.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84