




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031946.D
 Acq On : 28 Aug 2023 16:24
 Operator : SY/MD
 Sample : 04175-05ME
 Misc : 6.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYX0ME

Manual IntegrationsAPPROVED

Quant Time: Aug 29 00:08:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 26 00:50:15 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2023
 Supervised By :Mahesh Dadoda 08/31/2023

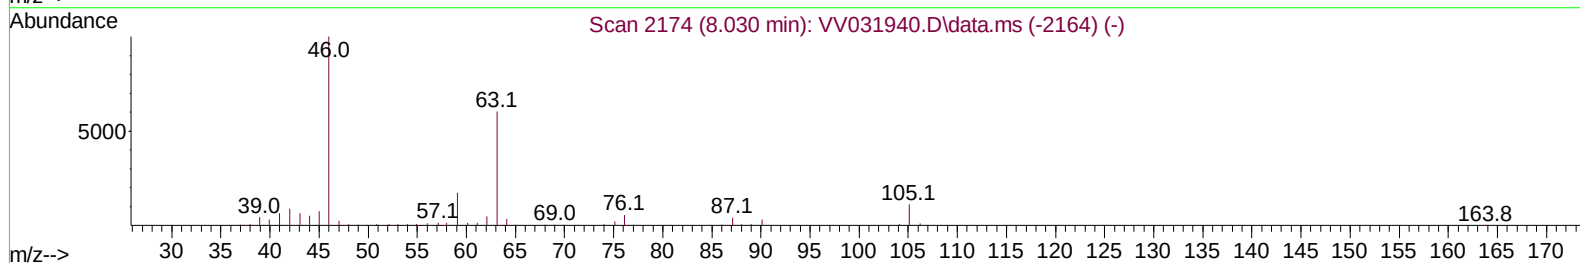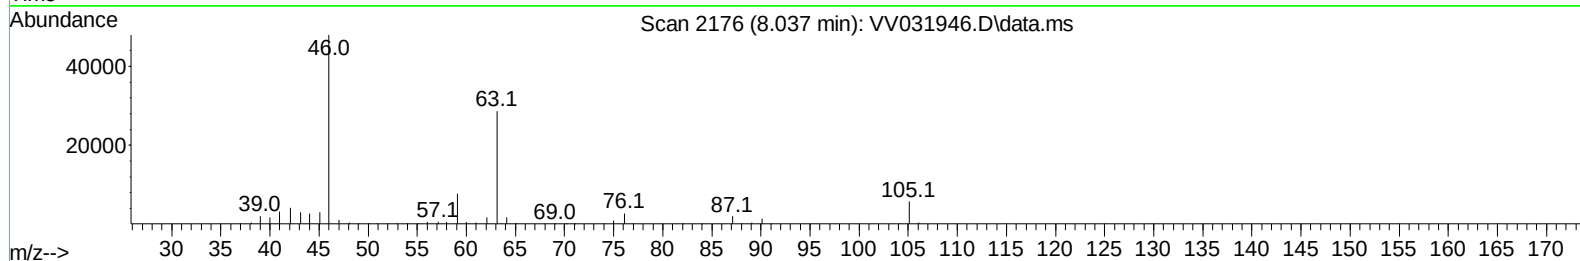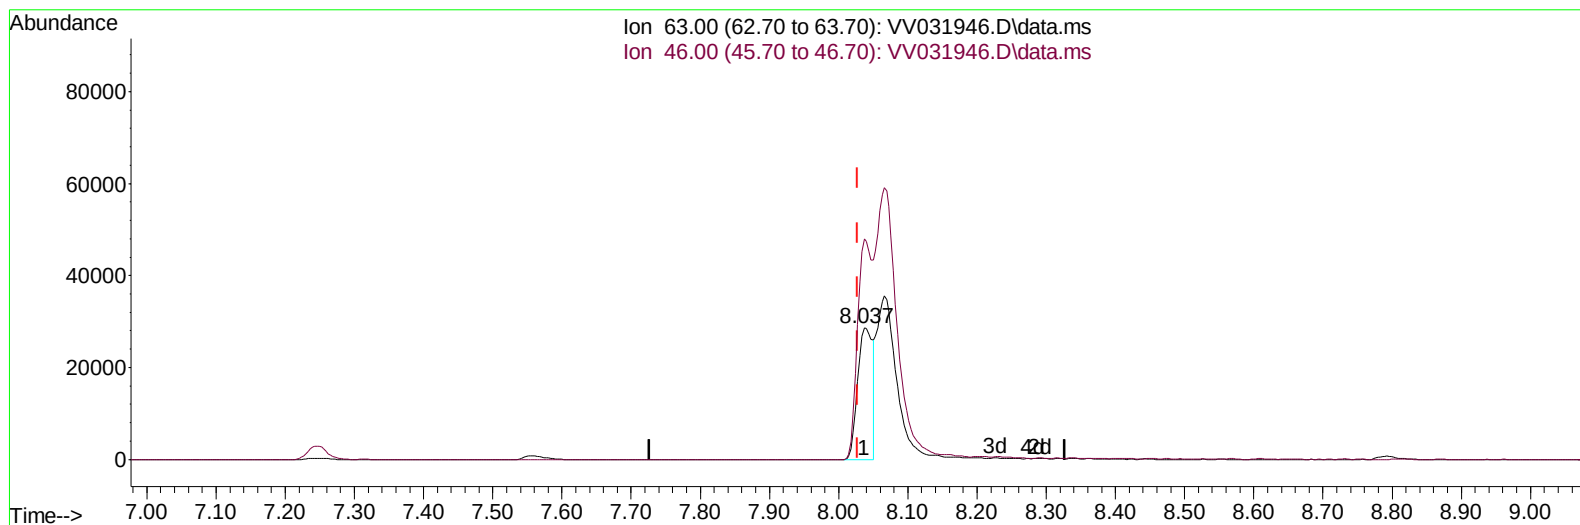

TIC: VV031946.D\data.ms

(47) 2-Hexanone-d5 (S)

8.037min (+ 0.010) 102.63 ug/L

response 42965

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	170.00	168.01
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031946.D
 Acq On : 28 Aug 2023 16:24
 Operator : SY/MD
 Sample : 04175-05ME
 Misc : 6.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYX0ME

Manual IntegrationsAPPROVED

Quant Time: Aug 29 00:08:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 26 00:50:15 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2023
 Supervised By :Mahesh Dadoda 08/31/2023

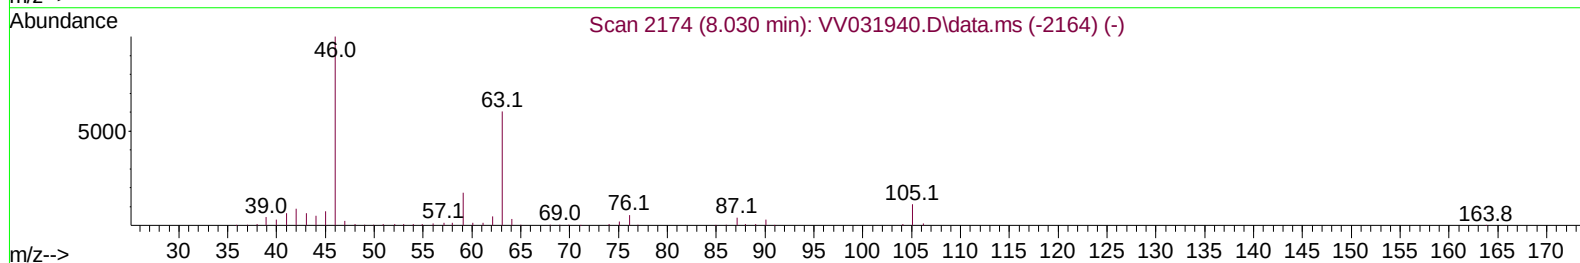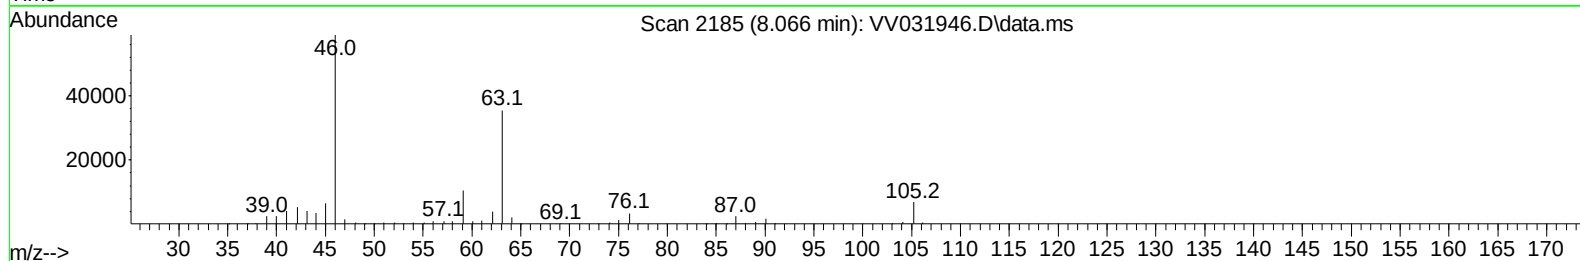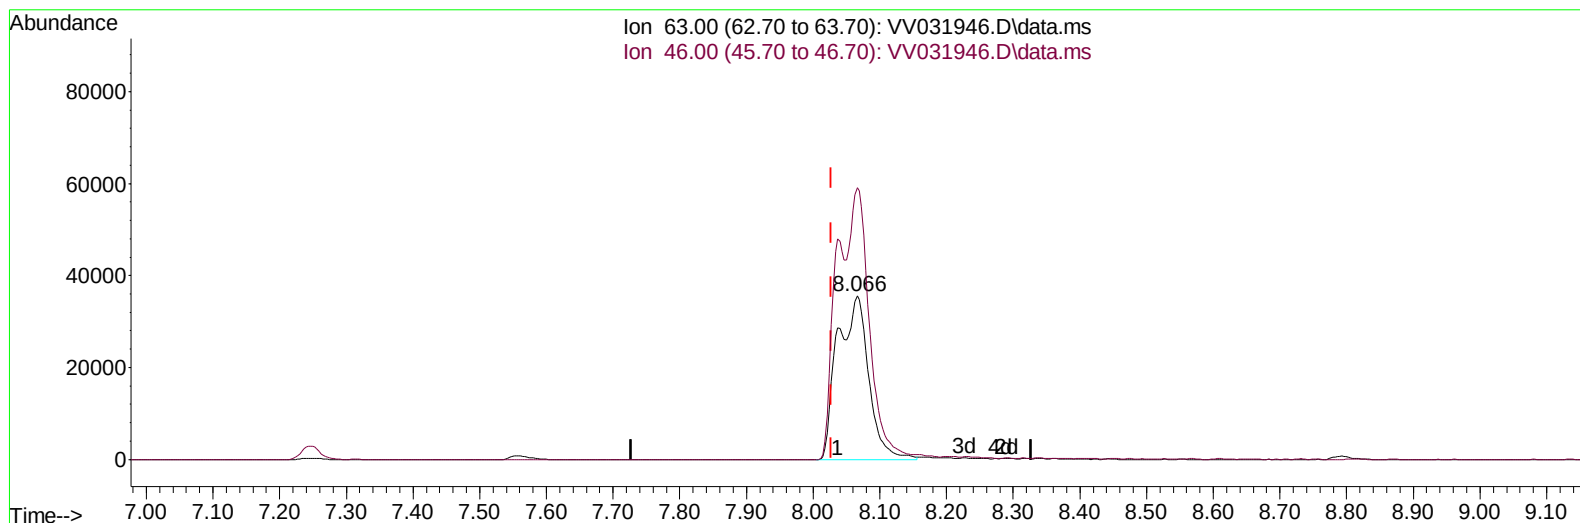

TIC: VV031946.D\data.ms

(47) 2-Hexanone-d5 (S)

8.066min (+ 0.039) 275.27 ug/L m

response 115243

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	170.00	62.64#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031946.D
 Acq On : 28 Aug 2023 16:24
 Operator : SY/MD
 Sample : 04175-05ME
 Misc : 6.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYX0ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2023
 Supervised By :Mahesh Dadoda 08/31/2023

Quant Time: Aug 29 00:08:32 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 26 00:50:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	161385	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	155524	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	79762	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	94937	93.997	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	188.000%#	
7) Chloroethane-d5	1.526	69	57464	64.903	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	129.800%	
11) 1,1-Dichloroethene-d2	2.040	65	46112	97.502	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125	Recovery	=	195.000%#	
21) 2-Butanone-d5	3.809	46	228772	287.993	ug/L	0.01
Spiked Amount 100.000	Range 40	- 130	Recovery	=	287.990%#	
24) Chloroform-d	4.249	84	263825	119.507	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	239.020%#	
26) 1,2-Dichloroethane-d4	4.941	65	178319	121.716	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	243.440%#	
32) Benzene-d6	4.957	84	515448	121.459	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	242.920%#	
36) 1,2-Dichloropropane-d6	5.989	67	183988	134.697	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	269.400%#	
41) Toluene-d8	7.246	98	458578	117.276	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	234.560%#	
43) trans-1,3-Dichloroprop...	7.555	79	91095	128.670	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	257.340%#	
47) 2-Hexanone-d5	8.066	63	115243m	275.270	ug/L	0.04
Spiked Amount 100.000	Range 45	- 130	Recovery	=	275.270%#	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	259640	147.096	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	294.200%#	
66) 1,2-Dichlorobenzene-d4	11.567	152	187998	129.295	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	258.600%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
Data File : VV031946.D
Acq On : 28 Aug 2023 16:24
Operator : SY/MD
Sample : 04175-05ME
Misc : 6.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYX0ME

Manual IntegrationsAPPROVED

Quant Time: Aug 29 00:08:32 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 26 00:50:15 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2023
Supervised By :Mahesh Dadoda 08/31/2023

