




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
Data File : VV031947.D
Acq On : 28 Aug 2023 16:47
Operator : SY/MD
Sample : 04175-06ME
Misc : 4.86g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYX3ME

Manual IntegrationsAPPROVED

Quant Time: Aug 29 00:08:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 26 00:50:15 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2023
Supervised By :Mahesh Dadoda 08/31/2023

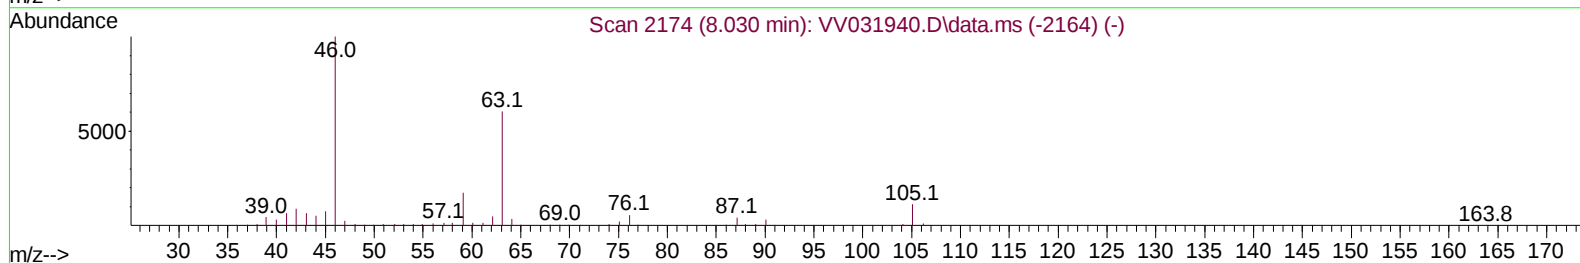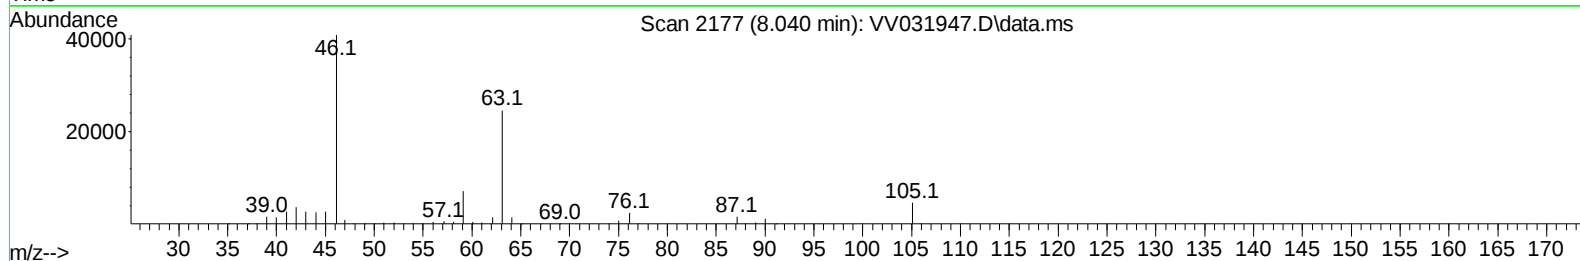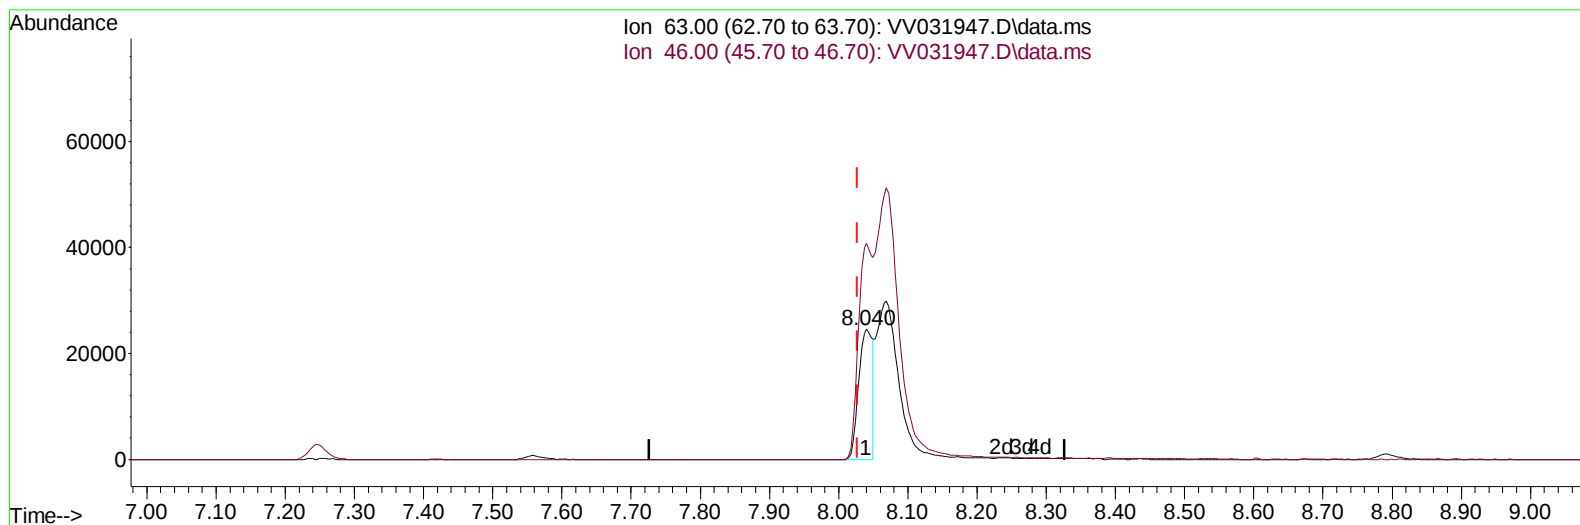

TIC: VV031947.D\data.ms

(47) 2-Hexanone-d5 (S)

8.040min (+ 0.013) 50.10 ug/L

response 34837

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	170.00	169.65
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031947.D
 Acq On : 28 Aug 2023 16:47
 Operator : SY/MD
 Sample : 04175-06ME
 Misc : 4.86g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYX3ME

Manual IntegrationsAPPROVED

Quant Time: Aug 29 00:08:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 26 00:50:15 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 08/31/2023
 Supervised By :Mahesh Dadoda 08/31/2023

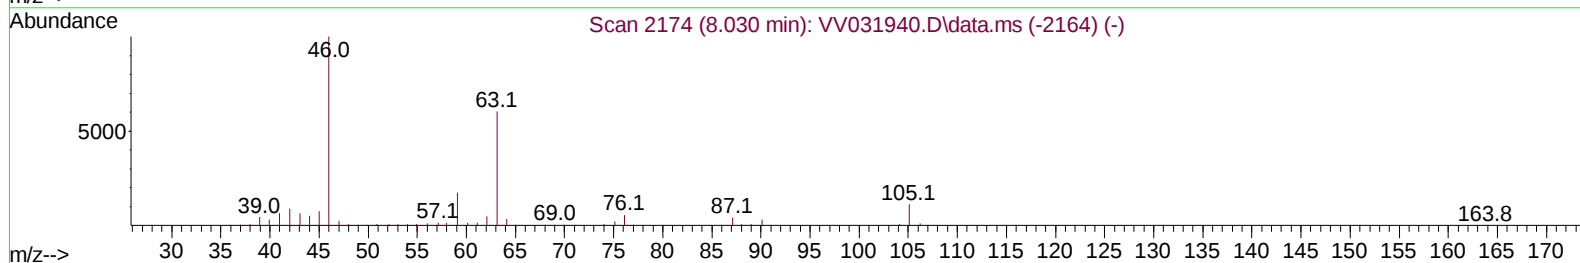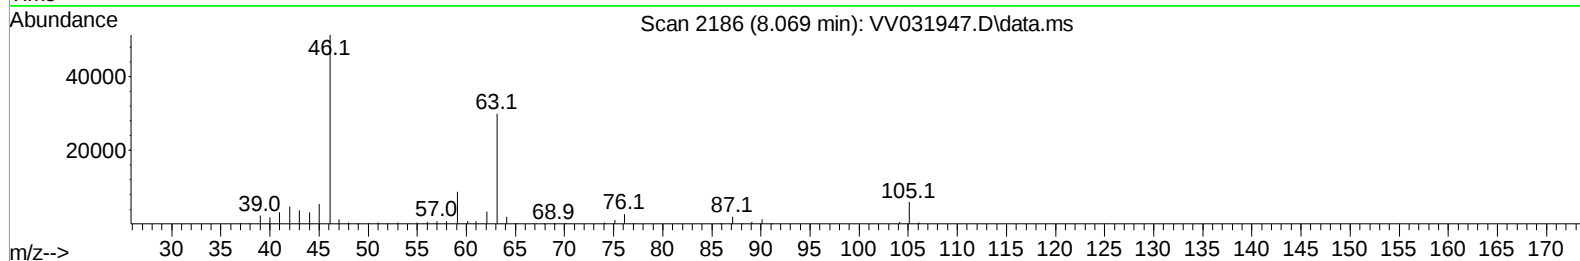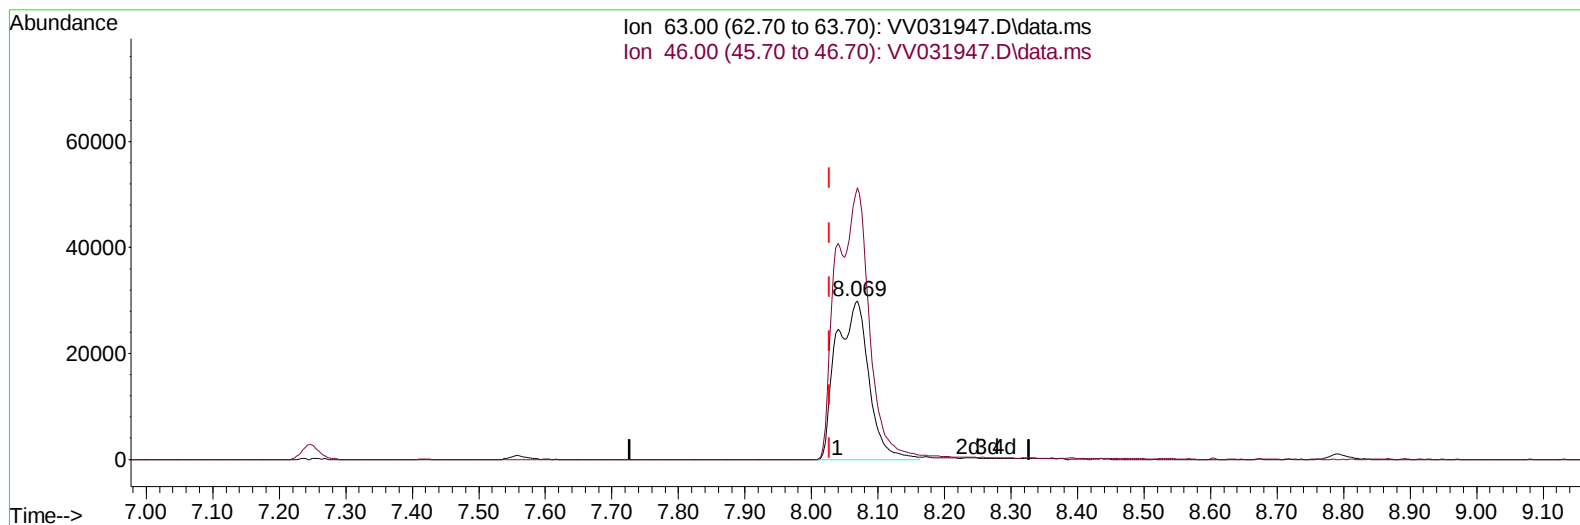

TIC: VV031947.D\data.ms

(47) 2-Hexanone-d5 (S)

8.069min (+ 0.042) 145.84 ug/L m

response 101417

Ion	Exp%	Act%
63.00	100.00	100.00
46.00	170.00	58.27#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031947.D
 Acq On : 28 Aug 2023 16:47
 Operator : SY/MD
 Sample : 04175-06ME
 Misc : 4.86g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYX3ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2023
 Supervised By :Mahesh Dadoda 08/31/2023

Quant Time: Aug 29 00:08:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 26 00:50:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.535	114	267298	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	258328	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	131380	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	84924	50.766	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	101.540%	
7) Chloroethane-d5	1.526	69	51852	35.359	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	70.720%	
11) 1,1-Dichloroethene-d2	2.040	65	40347	51.508	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125	Recovery	=	103.020%	
21) 2-Butanone-d5	3.809	46	201278	152.983	ug/L	0.01
Spiked Amount 100.000	Range 40	- 130	Recovery	=	152.980%#	
24) Chloroform-d	4.252	84	234009	64.000	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	128.000%#	
26) 1,2-Dichloroethane-d4	4.944	65	160562	66.170	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	132.340%#	
32) Benzene-d6	4.957	84	459845	65.235	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	130.480%#	
36) 1,2-Dichloropropane-d6	5.992	67	163535	72.078	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	144.160%#	
41) Toluene-d8	7.246	98	407285	62.708	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	125.420%#	
43) trans-1,3-Dichloroprop...	7.558	79	79125	67.285	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	134.580%#	
47) 2-Hexanone-d5	8.069	63	101417m	145.841	ug/L	0.04
Spiked Amount 100.000	Range 45	- 130	Recovery	=	145.840%#	
56) 1,1,2,2-Tetrachloroeth...	10.165	84	229848	78.396	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	156.800%#	
66) 1,2-Dichlorobenzene-d4	11.570	152	168519	70.363	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	140.720%#	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
Data File : VV031947.D
Acq On : 28 Aug 2023 16:47
Operator : SY/MD
Sample : 04175-06ME
Misc : 4.86g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYX3ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 08/31/2023
Supervised By :Mahesh Dadoda 08/31/2023

Quant Time: Aug 29 00:08:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 26 00:50:15 2023
Response via : Initial Calibration

