

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031952.D
 Acq On : 28 Aug 2023 19:20
 Operator : SY/MD
 Sample : 04175-05ME
 Misc : 6.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZYX0ME

Quant Time: Aug 29 00:09:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Aug 26 00:50:15 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	231938	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	227289	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	120044	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	40126	27.644	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	55.280%#
7) Chloroethane-d5	1.532	69	43090	33.864	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	67.720%#
11) 1,1-Dichloroethene-d2	2.063	65	21104	31.049	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.100%
21) 2-Butanone-d5	3.796	46	119126	104.346	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.350%
24) Chloroform-d	4.253	84	125024	39.406	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	78.820%
26) 1,2-Dichloroethane-d4	4.947	65	90524	42.994	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.980%
32) Benzene-d6	4.963	84	239824	38.669	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	77.340%
36) 1,2-Dichloropropane-d6	5.992	67	88119	44.143	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	88.280%
41) Toluene-d8	7.246	98	209699	36.695	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	73.400%#
43) trans-1,3-Dichloroprop...	7.558	79	40366	39.014	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.020%
47) 2-Hexanone-d5	8.031	63	60195	98.384	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	98.380%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	130535	50.603	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.200%
66) 1,2-Dichlorobenzene-d4	11.564	152	89553	40.923	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.840%
Target Compounds						
16) Methylene chloride	2.452	84	3755	2.404	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
Data File : VV031952.D
Acq On : 28 Aug 2023 19:20
Operator : SY/MD
Sample : 04175-05ME
Misc : 6.08g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZYX0ME

Quant Time: Aug 29 00:09:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Aug 26 00:50:15 2023
Response via : Initial Calibration

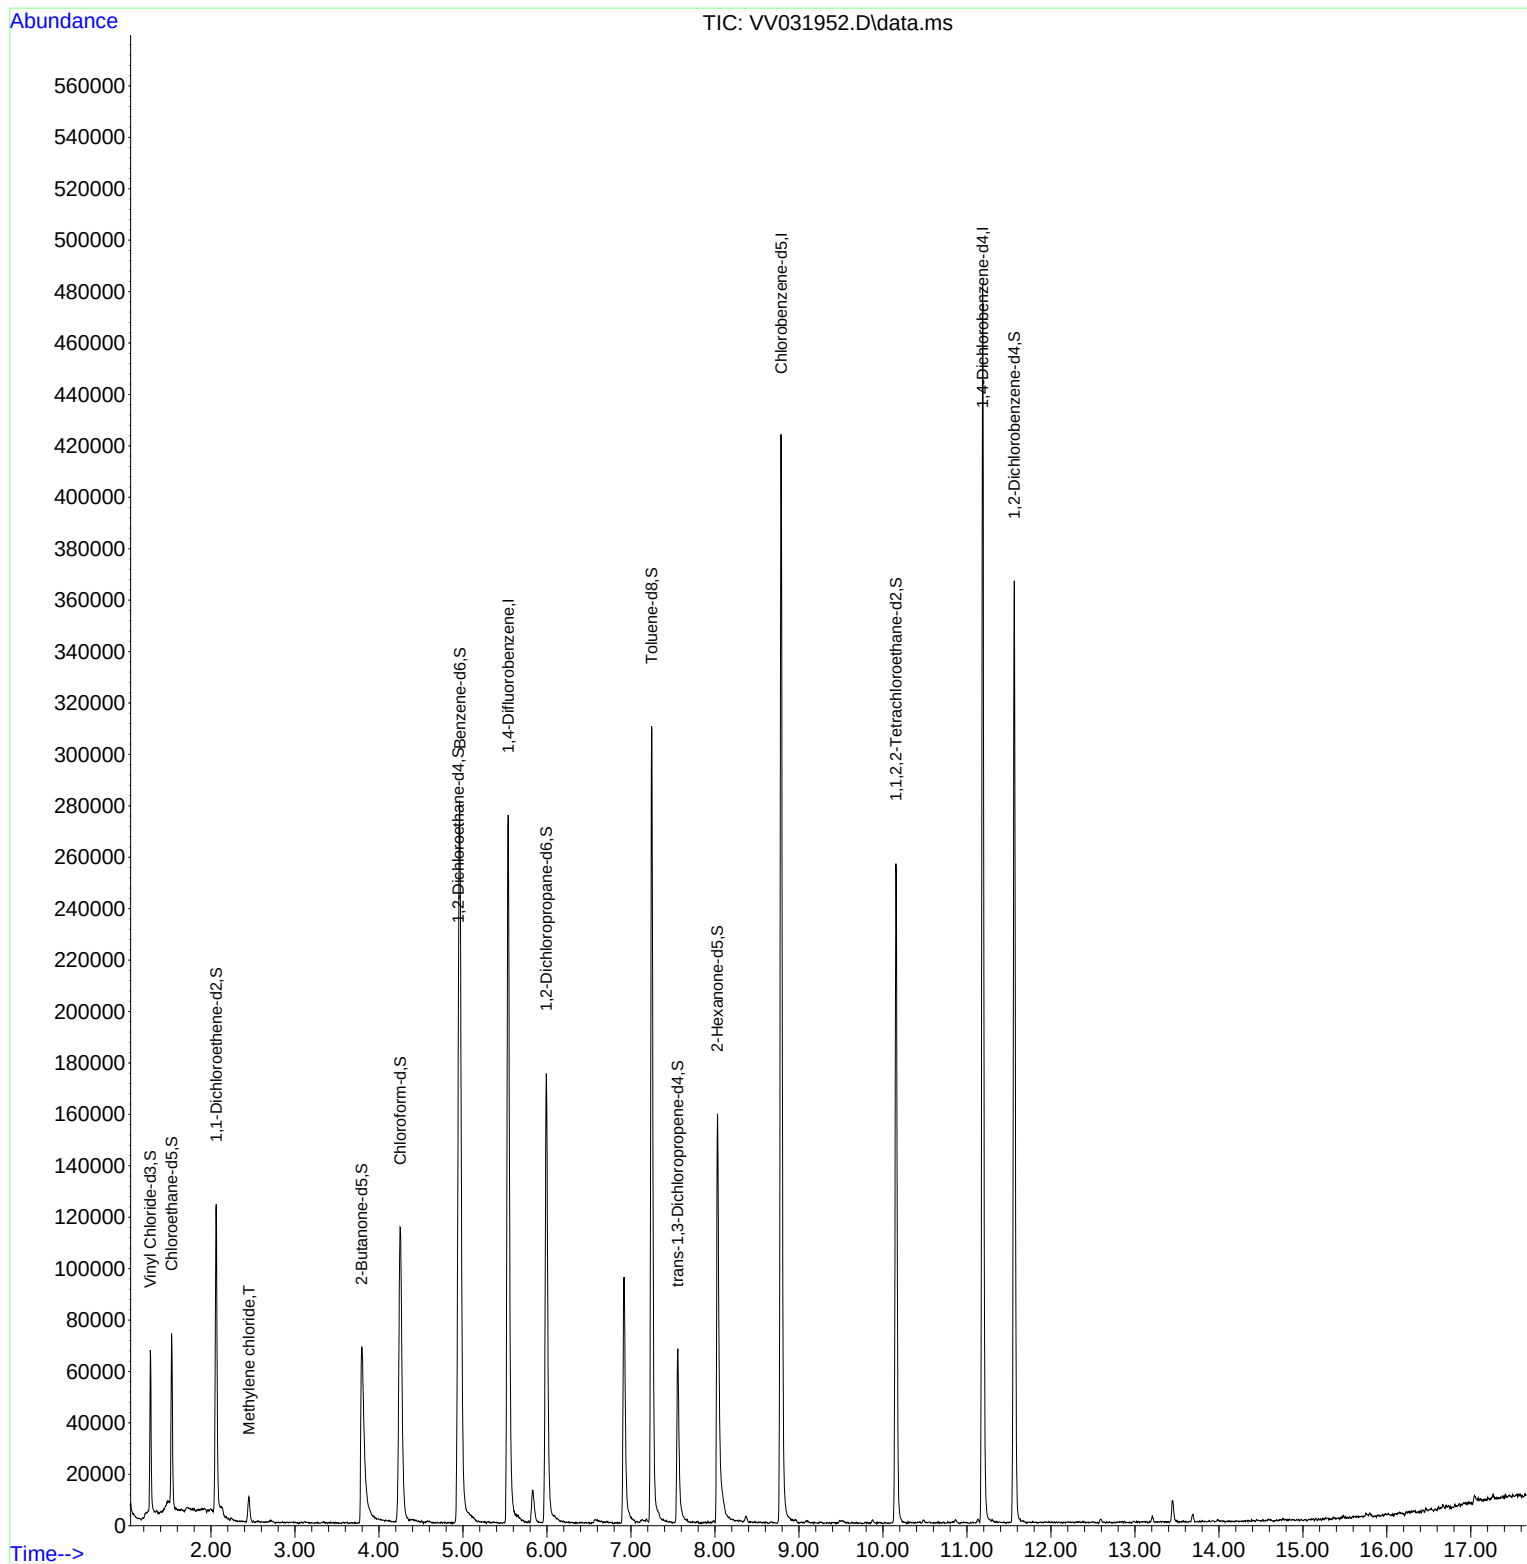

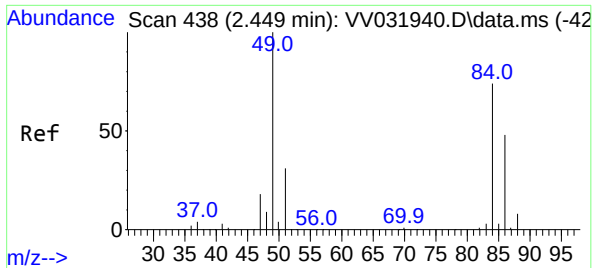

#16
Methylene chloride
Concen: 2.404 ug/L
RT: 2.452 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV031952.D
Acq: 28 Aug 2023 19:20

Instrument :
MSVOA_V
ClientSampleId :
EZYX0ME

Tgt Ion: 84 Resp: 3755
Ion Ratio Lower Upper
84 100
86 66.5 44.6 82.8
49 130.9 91.6 170.2

