

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031941.D
 Acq On : 28 Aug 2023 12:00
 Operator : SY/MD
 Sample : VV0828MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK383

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031941.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	90	rVB	116183	125261	13.25%	1.648%
2	1.532	147	153	169	rVB	102550	120810	12.78%	1.590%
3	2.060	309	317	331	rVB	192860	276757	29.28%	3.642%
4	2.831	553	557	558	rBV3	607	471	0.05%	0.006%
5	2.953	593	595	597	rBV2	433	200	0.02%	0.003%
6	3.037	617	621	624	rBV4	272	274	0.03%	0.004%
7	3.156	655	658	660	rBV2	414	262	0.03%	0.003%
8	3.442	741	747	748	rBV3	500	392	0.04%	0.005%
9	3.574	786	788	790	rBV2	197	85	0.01%	0.001%
10	3.584	790	791	793	rBV	253	113	0.01%	0.001%
11	3.703	822	828	830	rBV3	622	718	0.08%	0.009%
12	3.735	834	838	839	rBV2	394	200	0.02%	0.003%
13	3.757	842	845	849	rVB4	396	304	0.03%	0.004%
14	3.799	849	858	904	rBV	65040	208277	22.03%	2.740%
15	4.249	984	998	1022	rBV	143002	363945	38.50%	4.789%
16	4.741	1146	1151	1154	rVB5	565	440	0.05%	0.006%
17	4.760	1154	1157	1159	rVB2	304	179	0.02%	0.002%
18	4.777	1159	1162	1164	rBV	493	315	0.03%	0.004%
19	4.793	1164	1167	1170	rBV4	364	274	0.03%	0.004%
20	4.844	1178	1183	1187	rBV4	562	582	0.06%	0.008%
21	4.957	1201	1218	1250	rBV2	354606	945234	100.00%	12.437%
22	5.304	1321	1326	1327	rBV	648	531	0.06%	0.007%
23	5.535	1384	1398	1426	rBV	318033	653793	69.17%	8.603%
24	5.825	1479	1488	1508	rVB2	18901	39948	4.23%	0.526%
25	5.989	1527	1539	1575	rBV	206312	441644	46.72%	5.811%
26	6.387	1661	1663	1665	rBV2	562	267	0.03%	0.004%
27	6.477	1688	1691	1692	rBV2	365	221	0.02%	0.003%
28	6.526	1703	1706	1708	rBV3	353	227	0.02%	0.003%
29	6.773	1781	1783	1785	rBV2	218	110	0.01%	0.001%
30	6.805	1792	1793	1795	rBV2	234	73	0.01%	0.001%
31	6.866	1811	1812	1815	rBV2	309	170	0.02%	0.002%
32	6.915	1815	1827	1849	rBV	121010	226904	24.01%	2.986%
33	7.246	1918	1930	1964	rBV	414209	732713	77.52%	9.641%
34	7.555	2015	2026	2052	rBV	83284	154312	16.33%	2.030%
35	7.825	2108	2110	2115	rVB3	890	660	0.07%	0.009%
36	7.850	2115	2118	2119	rBV3	546	354	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031941.D
 Acq On : 28 Aug 2023 12:00
 Operator : SY/MD
 Sample : VV0828MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK383

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	7.876	2124	2126	2134	rVB5	863	973	0.10%	0.013%
38	7.908	2134	2136	2139	rBV4	1055	583	0.06%	0.008%
39	7.963	2151	2153	2155	rBV2	303	195	0.02%	0.003%
40	8.030	2165	2174	2217	rBV	161207	334134	35.35%	4.397%

41	8.407	2289	2291	2294	rBV3	552	400	0.04%	0.005%
42	8.648	2363	2366	2370	rBV3	486	365	0.04%	0.005%
43	8.738	2391	2394	2395	rBV3	364	182	0.02%	0.002%
44	8.786	2398	2409	2432	rBV	479753	801383	84.78%	10.545%
45	9.046	2488	2490	2494	rBV4	461	479	0.05%	0.006%

46	9.153	2521	2523	2526	rBV3	275	178	0.02%	0.002%
47	9.198	2535	2537	2540	rVB3	401	217	0.02%	0.003%
48	9.223	2540	2545	2548	rBV5	593	667	0.07%	0.009%
49	9.265	2550	2558	2563	rBV5	647	945	0.10%	0.012%
50	9.310	2569	2572	2574	rBV2	300	225	0.02%	0.003%

51	9.326	2574	2577	2580	rVV3	542	279	0.03%	0.004%
52	9.339	2580	2581	2583	rVB	355	137	0.01%	0.002%
53	9.374	2588	2592	2593	rBV4	625	380	0.04%	0.005%
54	9.464	2618	2620	2621	rBV	540	250	0.03%	0.003%
55	9.554	2646	2648	2649	rBV	344	147	0.02%	0.002%

56	9.651	2674	2678	2681	rBV3	553	506	0.05%	0.007%
57	9.747	2705	2708	2710	rBV2	435	332	0.04%	0.004%
58	9.783	2717	2719	2723	rBV2	432	276	0.03%	0.004%
59	9.802	2723	2725	2726	rBV	231	80	0.01%	0.001%
60	9.876	2742	2748	2756	rVB5	1915	2680	0.28%	0.035%

61	9.966	2774	2776	2777	rBV2	349	116	0.01%	0.002%
62	10.040	2797	2799	2800	rBV2	330	147	0.02%	0.002%
63	10.108	2816	2820	2821	rBV2	504	345	0.04%	0.005%
64	10.156	2824	2835	2861	rVB	278011	443456	46.91%	5.835%
65	10.307	2880	2882	2884	rBV2	228	81	0.01%	0.001%

66	10.329	2887	2889	2893	rBV4	450	213	0.02%	0.003%
67	10.384	2903	2906	2907	rBV3	350	152	0.02%	0.002%
68	10.484	2929	2937	2944	rBV6	1957	2984	0.32%	0.039%
69	10.577	2962	2966	2967	rBV2	421	285	0.03%	0.004%
70	10.648	2986	2988	2990	rBV	199	102	0.01%	0.001%

71	10.754	3018	3021	3022	rBV	349	198	0.02%	0.003%
72	10.863	3045	3055	3062	rBV5	2500	4013	0.42%	0.053%
73	11.017	3099	3103	3104	rBV3	514	312	0.03%	0.004%
74	11.069	3117	3119	3121	rVB2	359	167	0.02%	0.002%
75	11.085	3121	3124	3125	rBV3	306	206	0.02%	0.003%

76	11.124	3131	3136	3144	rBV6	2839	3920	0.41%	0.052%
----	--------	------	------	------	------	------	------	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031941.D
 Acq On : 28 Aug 2023 12:00
 Operator : SY/MD
 Sample : VV0828MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK383

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	11.188	3145	3156	3180	rVV	566215	873348	92.39%	11.491%
78	11.477	3242	3246	3249	rBV4	589	487	0.05%	0.006%
79	11.564	3258	3273	3296	rBV	455519	721869	76.37%	9.498%
80	11.805	3346	3348	3351	rBV2	585	374	0.04%	0.005%
81	11.873	3367	3369	3372	rBV2	450	317	0.03%	0.004%
82	11.931	3384	3387	3391	rBV3	635	510	0.05%	0.007%
83	12.107	3440	3442	3446	rBV2	404	278	0.03%	0.004%
84	12.165	3458	3460	3461	rBV	169	63	0.01%	0.001%
85	12.265	3487	3491	3492	rBV	570	397	0.04%	0.005%
86	12.371	3519	3524	3530	rBV5	874	1083	0.11%	0.014%
87	12.474	3553	3556	3558	rBV2	385	245	0.03%	0.003%
88	12.490	3559	3561	3566	rBV3	534	409	0.04%	0.005%
89	12.554	3579	3581	3582	rBV	365	142	0.02%	0.002%
90	12.590	3585	3592	3598	rVV4	4243	5809	0.61%	0.076%
91	12.651	3610	3611	3613	rBB	168	44	0.00%	0.001%
92	12.660	3613	3614	3615	rBV	310	116	0.01%	0.002%
93	12.712	3628	3630	3632	rVB	559	189	0.02%	0.002%
94	12.728	3632	3635	3638	rBV4	554	403	0.04%	0.005%
95	13.082	3743	3745	3747	rBV	300	139	0.01%	0.002%
96	13.204	3776	3783	3793	rBV3	8417	12536	1.33%	0.165%
97	13.445	3849	3858	3875	rVB	40100	64257	6.80%	0.845%
98	13.686	3925	3933	3944	rVB4	11624	17271	1.83%	0.227%


Sum of corrected areas: 7599996

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
Data File : VV031941.D
Acq On : 28 Aug 2023 12:00
Operator : SY/MD
Sample : VV0828MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK383

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

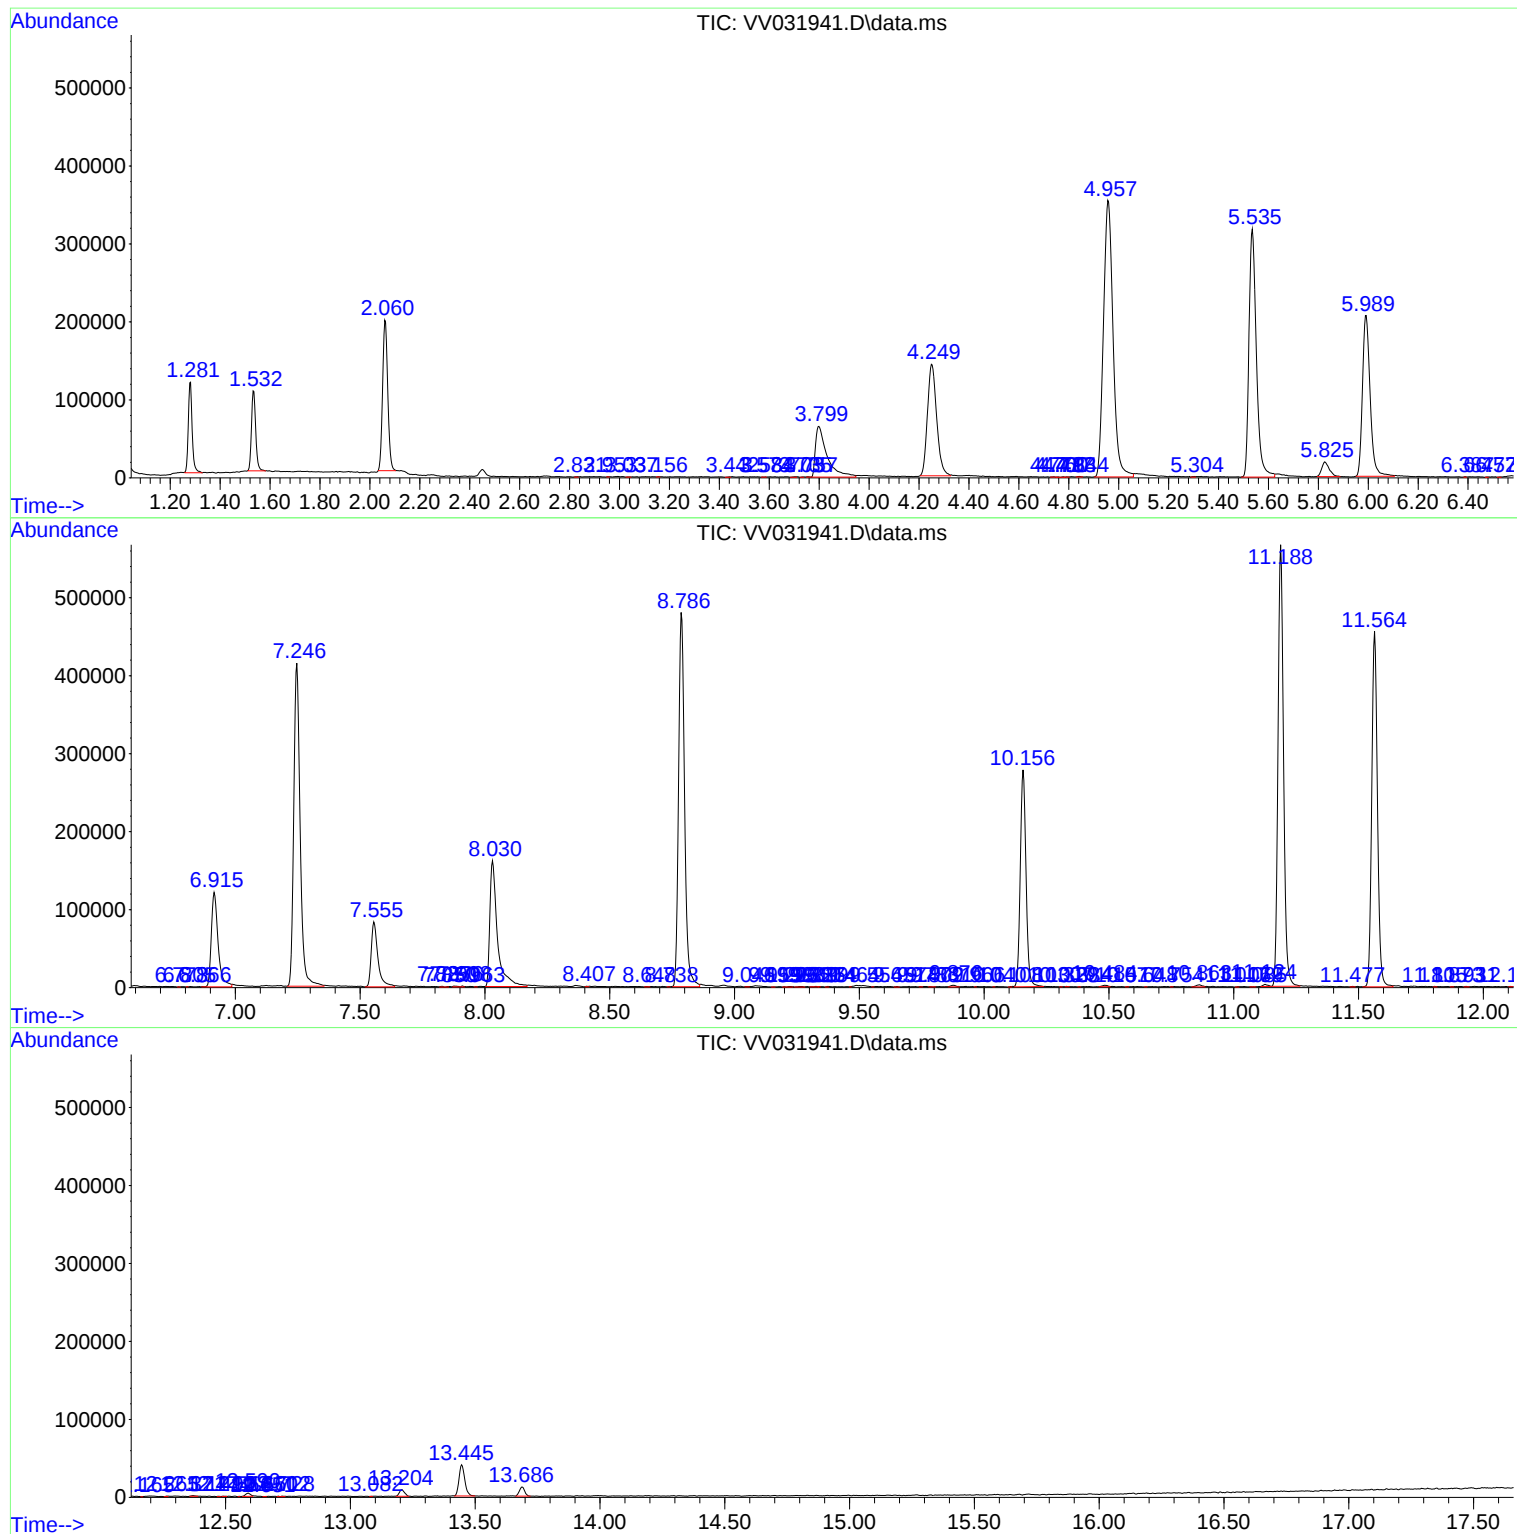

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
Data File : VV031941.D
Acq On : 28 Aug 2023 12:00
Operator : SY/MD
Sample : VV0828MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK383

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
Data File : VV031941.D
Acq On : 28 Aug 2023 12:00
Operator : SY/MD
Sample : VV0828MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK383

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
