

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031943.D
 Acq On : 28 Aug 2023 13:06
 Operator : SY/MD
 Sample : 04172-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCHN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031943.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	69	74	88	rVB	83979	89248	10.06%	1.243%
2	1.532	147	153	167	rVB	86672	101563	11.45%	1.415%
3	2.060	309	317	331	rVB	151086	219488	24.75%	3.058%
4	2.809	548	550	554	rVB3	573	294	0.03%	0.004%
5	3.027	616	618	619	rBV	254	124	0.01%	0.002%
6	3.175	659	664	666	rBV3	592	531	0.06%	0.007%
7	3.204	671	673	677	rVB3	407	294	0.03%	0.004%
8	3.326	706	711	712	rBV2	440	330	0.04%	0.005%
9	3.349	716	718	720	rVB2	303	111	0.01%	0.002%
10	3.362	720	722	723	rBV	407	170	0.02%	0.002%
11	3.404	731	735	740	rBV3	469	472	0.05%	0.007%
12	3.574	786	788	790	rBV2	307	131	0.01%	0.002%
13	3.632	802	806	807	rBV2	417	244	0.03%	0.003%
14	3.670	813	818	822	rBV4	479	506	0.06%	0.007%
15	3.796	847	857	900	rBV	64928	198432	22.37%	2.764%
16	4.249	982	998	1031	rBV	134211	356738	40.22%	4.970%
17	4.680	1130	1132	1136	rBV3	292	151	0.02%	0.002%
18	4.731	1146	1148	1150	rBV2	282	154	0.02%	0.002%
19	4.870	1189	1191	1195	rVB2	528	267	0.03%	0.004%
20	4.957	1200	1218	1249	rBV2	330729	886945	100.00%	12.356%
21	5.310	1327	1328	1331	rBV2	512	223	0.03%	0.003%
22	5.378	1347	1349	1352	rBV2	364	264	0.03%	0.004%
23	5.439	1364	1368	1370	rBV2	505	341	0.04%	0.005%
24	5.455	1370	1373	1376	rBV3	358	283	0.03%	0.004%
25	5.487	1380	1383	1385	rBV3	349	222	0.03%	0.003%
26	5.535	1385	1398	1426	rBV	316280	652760	73.60%	9.094%
27	5.828	1477	1489	1507	rBV2	23733	50491	5.69%	0.703%
28	5.947	1524	1526	1527	rBV	374	112	0.01%	0.002%
29	5.992	1527	1540	1569	rBV	198992	424553	47.87%	5.915%
30	6.227	1609	1613	1615	rBV2	387	252	0.03%	0.004%
31	6.239	1615	1617	1620	rVB3	417	168	0.02%	0.002%
32	6.400	1665	1667	1670	rBV2	446	237	0.03%	0.003%
33	6.439	1675	1679	1681	rBV3	253	208	0.02%	0.003%
34	6.526	1704	1706	1708	rBV2	294	125	0.01%	0.002%
35	6.538	1708	1710	1713	rBV4	423	279	0.03%	0.004%
36	6.677	1750	1753	1754	rBV	487	221	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031943.D
 Acq On : 28 Aug 2023 13:06
 Operator : SY/MD
 Sample : 04172-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCHN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.770	1778	1782	1784	rBV2	504	341	0.04%	0.005%
38	6.850	1804	1807	1810	rBV3	372	214	0.02%	0.003%
39	6.915	1817	1827	1852	rBV2	113798	216260	24.38%	3.013%
40	7.246	1918	1930	1965	rBV	384504	692969	78.13%	9.654%
41	7.554	2016	2026	2054	rBV	79729	148637	16.76%	2.071%
42	7.741	2080	2084	2088	rBV3	662	615	0.07%	0.009%
43	7.763	2089	2091	2095	rBV5	446	301	0.03%	0.004%
44	7.805	2100	2104	2108	rBV5	858	678	0.08%	0.009%
45	7.876	2116	2126	2137	rBV3	5262	9253	1.04%	0.129%
46	8.030	2165	2174	2219	rBV	149806	315525	35.57%	4.396%
47	8.400	2287	2289	2294	rVB3	708	463	0.05%	0.006%
48	8.529	2326	2329	2331	rBV3	440	231	0.03%	0.003%
49	8.542	2331	2333	2336	rBV3	346	227	0.03%	0.003%
50	8.596	2347	2350	2355	rVB5	497	397	0.04%	0.006%
51	8.622	2355	2358	2363	rBV2	505	371	0.04%	0.005%
52	8.677	2370	2375	2377	rBV3	512	355	0.04%	0.005%
53	8.715	2385	2387	2388	rBV2	371	196	0.02%	0.003%
54	8.786	2395	2409	2442	rBV	485633	807822	91.08%	11.254%
55	9.082	2496	2501	2505	rBV4	855	952	0.11%	0.013%
56	9.169	2526	2528	2529	rBV	267	110	0.01%	0.002%
57	9.233	2546	2548	2550	rBV	316	176	0.02%	0.002%
58	9.246	2550	2552	2555	rVB2	510	248	0.03%	0.003%
59	9.262	2555	2557	2562	rBV3	373	214	0.02%	0.003%
60	9.342	2579	2582	2587	rVB5	552	442	0.05%	0.006%
61	9.410	2600	2603	2609	rBV6	576	624	0.07%	0.009%
62	9.529	2636	2640	2642	rBV3	775	573	0.06%	0.008%
63	9.548	2644	2646	2649	rVB2	501	247	0.03%	0.003%
64	9.567	2649	2652	2653	rBV3	377	197	0.02%	0.003%
65	9.587	2656	2658	2661	rBV3	519	350	0.04%	0.005%
66	9.706	2689	2695	2697	rBV4	387	382	0.04%	0.005%
67	9.783	2717	2719	2721	rBV2	470	336	0.04%	0.005%
68	9.815	2726	2729	2736	rVB5	461	534	0.06%	0.007%
69	9.886	2748	2751	2755	rVB3	610	389	0.04%	0.005%
70	9.963	2774	2775	2779	rVB	324	147	0.02%	0.002%
71	9.985	2779	2782	2786	rVB4	490	293	0.03%	0.004%
72	10.005	2786	2788	2789	rBV2	346	107	0.01%	0.001%
73	10.024	2792	2794	2797	rBV4	251	162	0.02%	0.002%
74	10.072	2807	2809	2811	rVB2	336	128	0.01%	0.002%
75	10.088	2812	2814	2820	rVB3	443	294	0.03%	0.004%
76	10.156	2820	2835	2862	rBV	253442	411122	46.35%	5.728%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031943.D
 Acq On : 28 Aug 2023 13:06
 Operator : SY/MD
 Sample : 04172-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DCHN3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	10.252	2862	2865	2866	rBV2	494	293	0.03%	0.004%
78	10.284	2873	2875	2878	rBV3	312	140	0.02%	0.002%
79	10.332	2882	2890	2904	rVB3	8553	13474	1.52%	0.188%
80	10.394	2907	2909	2911	rBV	274	116	0.01%	0.002%
81	10.593	2965	2971	2977	rVB6	495	703	0.08%	0.010%
82	10.619	2977	2979	2981	rBV2	287	151	0.02%	0.002%
83	10.728	3011	3013	3016	rBV3	388	215	0.02%	0.003%
84	10.841	3046	3048	3050	rBV	310	184	0.02%	0.003%
85	10.860	3050	3054	3055	rBV3	559	437	0.05%	0.006%
86	10.902	3065	3067	3069	rVB3	281	102	0.01%	0.001%
87	11.030	3102	3107	3112	rBV3	465	539	0.06%	0.008%
88	11.085	3121	3124	3125	rBV2	375	241	0.03%	0.003%
89	11.188	3145	3156	3178	rBV	567411	870399	98.13%	12.126%
90	11.564	3262	3273	3289	rBV	432629	679391	76.60%	9.465%
91	11.889	3370	3374	3376	rBV2	538	402	0.05%	0.006%
92	11.924	3382	3385	3387	rBV4	479	345	0.04%	0.005%
93	12.021	3413	3415	3416	rBV4	277	145	0.02%	0.002%
94	12.130	3445	3449	3450	rBV2	575	388	0.04%	0.005%
95	12.239	3480	3483	3484	rBV2	365	238	0.03%	0.003%
96	12.297	3496	3501	3515	rBV7	1430	2239	0.25%	0.031%
97	13.107	3751	3753	3759	rVB3	634	413	0.05%	0.006%
98	13.258	3793	3800	3805	rBV3	718	1006	0.11%	0.014%
99	13.451	3854	3860	3868	rVB2	4538	6407	0.72%	0.089%
100	13.930	4006	4009	4010	rBV	371	207	0.02%	0.003%




Sum of corrected areas: 7177989

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
Data File : VV031943.D
Acq On : 28 Aug 2023 13:06
Operator : SY/MD
Sample : 04172-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCHN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

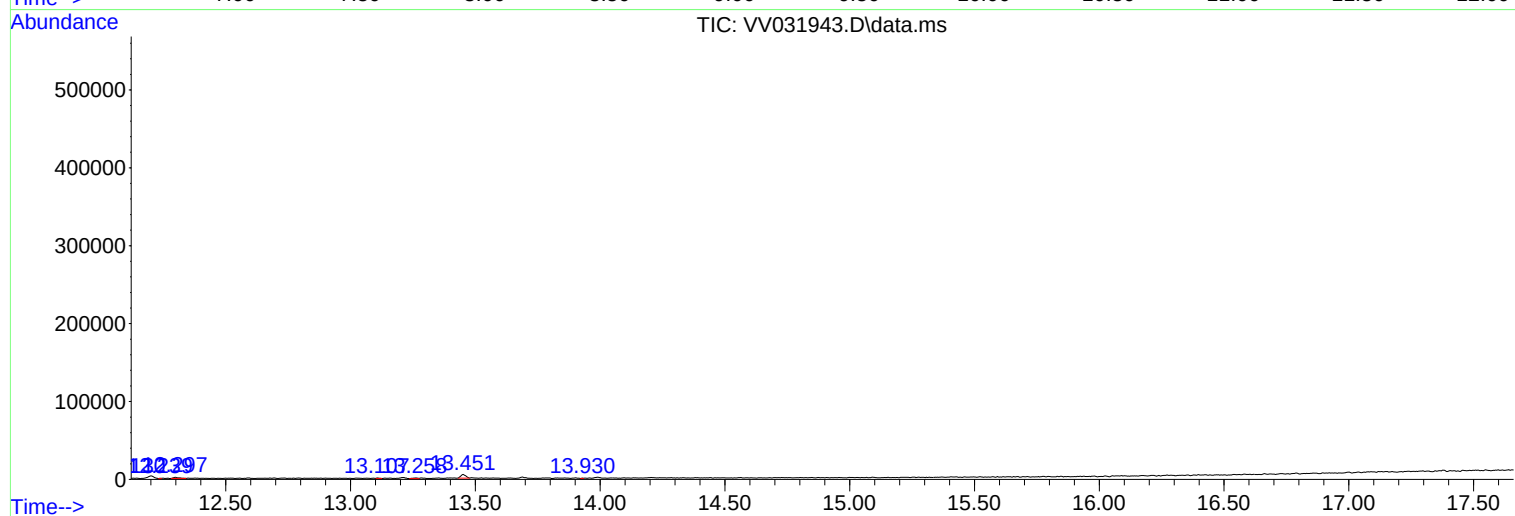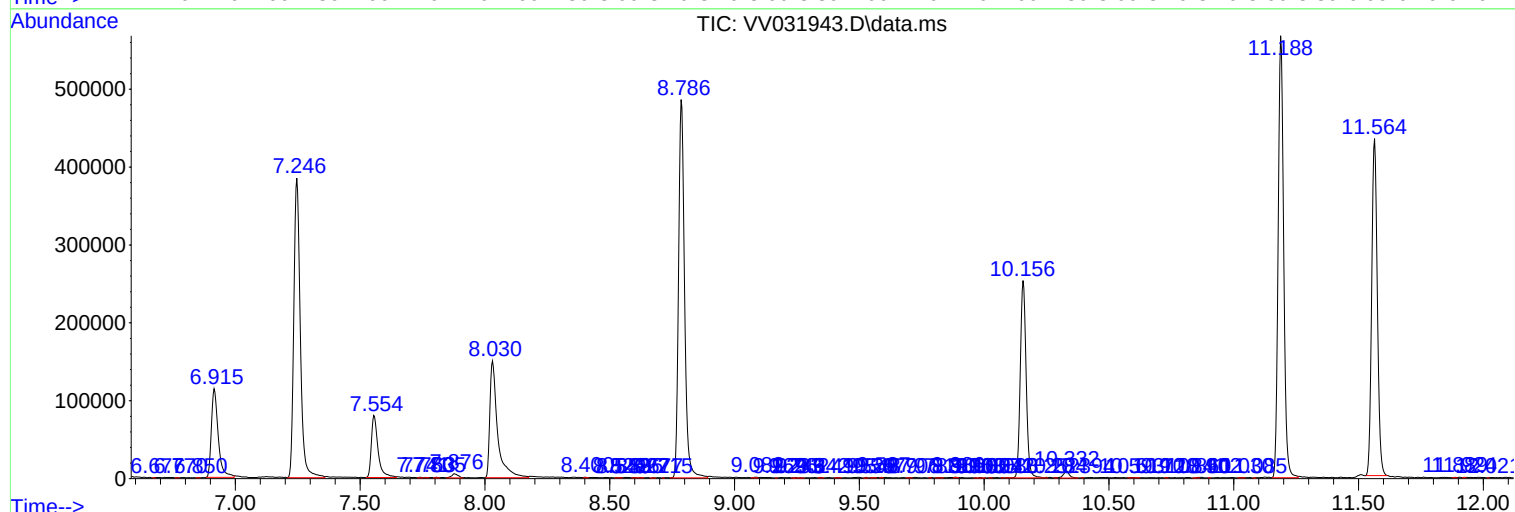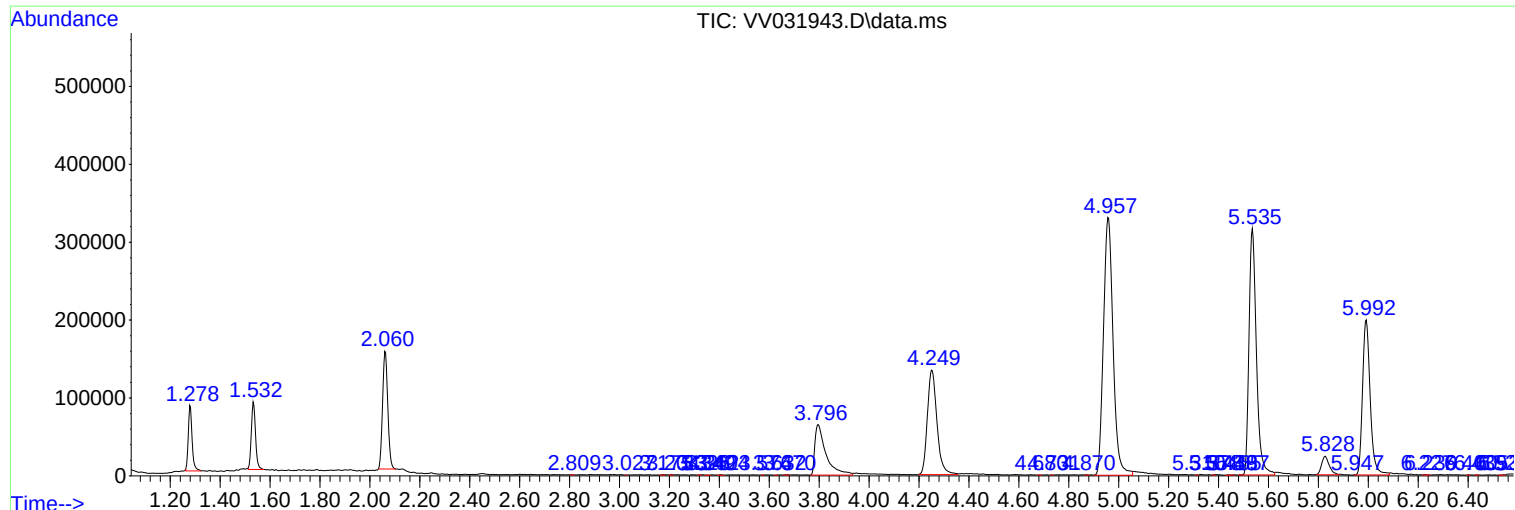

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
Data File : VV031943.D
Acq On : 28 Aug 2023 13:06
Operator : SY/MD
Sample : 04172-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCHN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
Data File : VV031943.D
Acq On : 28 Aug 2023 13:06
Operator : SY/MD
Sample : 04172-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DCHN3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------