

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031950.D
 Acq On : 28 Aug 2023 17:57
 Operator : SY/MD
 Sample : VIBLK227
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

Signal : TIC: VV031950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	86	rBV	76833	81579	9.32%	1.167%
2	1.532	147	153	169	rVB	80731	96662	11.05%	1.382%
3	2.063	309	318	332	rVB	140066	203801	23.29%	2.915%
4	2.452	431	439	451	rVB	9519	14901	1.70%	0.213%
5	2.654	500	502	505	rBV2	417	250	0.03%	0.004%
6	2.860	564	566	568	rBV2	264	72	0.01%	0.001%
7	3.117	641	646	649	rBV3	495	479	0.05%	0.007%
8	3.156	654	658	659	rBV	380	233	0.03%	0.003%
9	3.214	670	676	677	rBV4	606	510	0.06%	0.007%
10	3.253	682	688	692	rBV4	443	548	0.06%	0.008%
11	3.307	703	705	707	rVB2	320	81	0.01%	0.001%
12	3.330	711	712	715	rBV2	272	164	0.02%	0.002%
13	3.384	727	729	730	rBV	335	104	0.01%	0.001%
14	3.497	761	764	765	rBV	342	189	0.02%	0.003%
15	3.574	784	788	791	rBV2	275	229	0.03%	0.003%
16	3.587	791	792	794	rBV3	184	78	0.01%	0.001%
17	3.638	806	808	811	rBV2	535	292	0.03%	0.004%
18	3.725	831	835	839	rBV3	403	361	0.04%	0.005%
19	3.796	848	857	885	rBV	68899	193696	22.14%	2.770%
20	4.256	985	1000	1027	rBV	127476	327423	37.42%	4.682%
21	4.632	1115	1117	1118	rBV2	263	99	0.01%	0.001%
22	4.709	1139	1141	1143	rBV2	247	142	0.02%	0.002%
23	4.847	1181	1184	1185	rBV2	309	167	0.02%	0.002%
24	4.883	1193	1195	1197	rVB2	341	138	0.02%	0.002%
25	4.960	1202	1219	1251	rBV2	314881	843063	96.35%	12.057%
26	5.240	1304	1306	1310	rVB4	773	411	0.05%	0.006%
27	5.259	1310	1312	1313	rBV	401	135	0.02%	0.002%
28	5.384	1349	1351	1353	rVB2	315	126	0.01%	0.002%
29	5.484	1379	1382	1385	rBV2	502	310	0.04%	0.004%
30	5.539	1385	1399	1428	rBV	318600	656483	75.03%	9.388%
31	5.777	1472	1473	1474	rBV	267	80	0.01%	0.001%
32	5.831	1480	1490	1506	rBV3	12124	26988	3.08%	0.386%
33	5.934	1520	1522	1524	rBV	138	55	0.01%	0.001%
34	5.944	1524	1525	1527	rBV	272	78	0.01%	0.001%
35	5.995	1527	1541	1564	rBV	192733	406221	46.42%	5.809%
36	6.278	1627	1629	1632	rBV3	341	243	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031950.D
 Acq On : 28 Aug 2023 17:57
 Operator : SY/MD
 Sample : VIBLK227
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

37	6.355	1649	1653	1657	rBV5	653	519	0.06%	0.007%
38	6.375	1657	1659	1661	rVB	433	162	0.02%	0.002%
39	6.429	1672	1676	1677	rBV	357	207	0.02%	0.003%
40	6.474	1688	1690	1691	rBV	108	40	0.00%	0.001%
41	6.490	1691	1695	1697	rBV3	751	479	0.05%	0.007%
42	6.693	1755	1758	1760	rBV3	518	361	0.04%	0.005%
43	6.748	1771	1775	1778	rBV3	611	585	0.07%	0.008%
44	6.764	1778	1780	1783	rVV2	279	130	0.01%	0.002%
45	6.793	1788	1789	1790	rBV	230	83	0.01%	0.001%
46	6.847	1803	1806	1807	rBV3	261	108	0.01%	0.002%
47	6.918	1817	1828	1856	rBV	106406	205744	23.51%	2.942%
48	7.114	1886	1889	1890	rBV2	755	459	0.05%	0.007%
49	7.249	1919	1931	1959	rBV	358884	649855	74.27%	9.294%
50	7.558	2016	2027	2050	rBV	73566	138587	15.84%	1.982%
51	7.821	2105	2109	2110	rBV2	315	174	0.02%	0.002%
52	7.847	2115	2117	2119	rBV2	346	176	0.02%	0.003%
53	7.950	2147	2149	2153	rVB2	314	178	0.02%	0.003%
54	8.030	2165	2174	2211	rBV	165958	323054	36.92%	4.620%
55	8.455	2303	2306	2310	rBV3	496	479	0.05%	0.007%
56	8.616	2353	2356	2360	rVB4	454	392	0.04%	0.006%
57	8.638	2360	2363	2365	rBV3	310	179	0.02%	0.003%
58	8.667	2369	2372	2374	rBV3	538	350	0.04%	0.005%
59	8.702	2381	2383	2389	rVB2	586	509	0.06%	0.007%
60	8.731	2389	2392	2394	rBV2	559	398	0.05%	0.006%
61	8.789	2398	2410	2433	rBV	483021	813798	93.00%	11.638%
62	9.030	2481	2485	2490	rVB3	622	467	0.05%	0.007%
63	9.120	2512	2513	2521	rVB6	379	390	0.04%	0.006%
64	9.159	2521	2525	2526	rBV2	432	233	0.03%	0.003%
65	9.188	2531	2534	2535	rBV2	529	260	0.03%	0.004%
66	9.223	2543	2545	2548	rVB2	444	184	0.02%	0.003%
67	9.239	2548	2550	2552	rBV	392	244	0.03%	0.003%
68	9.291	2565	2566	2567	rBV	244	80	0.01%	0.001%
69	9.384	2593	2595	2599	rVB3	476	252	0.03%	0.004%
70	9.419	2604	2606	2610	rBV3	426	398	0.05%	0.006%
71	9.461	2616	2619	2621	rVB4	413	185	0.02%	0.003%
72	9.487	2621	2627	2628	rBV3	1001	849	0.10%	0.012%
73	9.619	2666	2668	2671	rBV3	343	179	0.02%	0.003%
74	9.635	2671	2673	2676	rBV3	446	246	0.03%	0.004%
75	9.654	2676	2679	2680	rBV	347	190	0.02%	0.003%
76	9.702	2692	2694	2699	rVB3	422	241	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
 Data File : VV031950.D
 Acq On : 28 Aug 2023 17:57
 Operator : SY/MD
 Sample : VIBLK227
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK227

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
 Title : VOC Analysis

77	9.731	2699	2703	2705	rBV3	598	484	0.06%	0.007%
78	9.792	2718	2722	2725	rBV4	566	458	0.05%	0.007%
79	9.876	2740	2748	2758	rBV6	1382	2001	0.23%	0.029%
80	9.960	2772	2774	2778	rBV4	544	279	0.03%	0.004%
81	10.001	2786	2787	2789	rBV	254	100	0.01%	0.001%
82	10.063	2803	2806	2807	rBV2	420	224	0.03%	0.003%
83	10.156	2823	2835	2860	rBV	272578	443048	50.63%	6.336%
84	10.268	2867	2870	2875	rBV4	775	553	0.06%	0.008%
85	10.313	2880	2884	2888	rBV5	630	672	0.08%	0.010%
86	10.352	2893	2896	2898	rBV2	699	439	0.05%	0.006%
87	10.400	2908	2911	2912	rBV	344	211	0.02%	0.003%
88	10.445	2923	2925	2929	rBV3	515	388	0.04%	0.006%
89	10.609	2972	2976	2980	rBV3	373	353	0.04%	0.005%
90	10.754	3018	3021	3022	rBV2	425	293	0.03%	0.004%
91	10.860	3051	3054	3061	rVB5	1422	1485	0.17%	0.021%
92	11.188	3144	3156	3180	rBV	555061	875009	100.00%	12.513%
93	11.464	3239	3242	3244	rBV4	397	263	0.03%	0.004%
94	11.497	3249	3252	3253	rBV2	450	211	0.02%	0.003%
95	11.564	3261	3273	3292	rBV	417448	668259	76.37%	9.557%




Sum of corrected areas: 6992525

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
Data File : VV031950.D
Acq On : 28 Aug 2023 17:57
Operator : SY/MD
Sample : VIBLK227
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK227

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

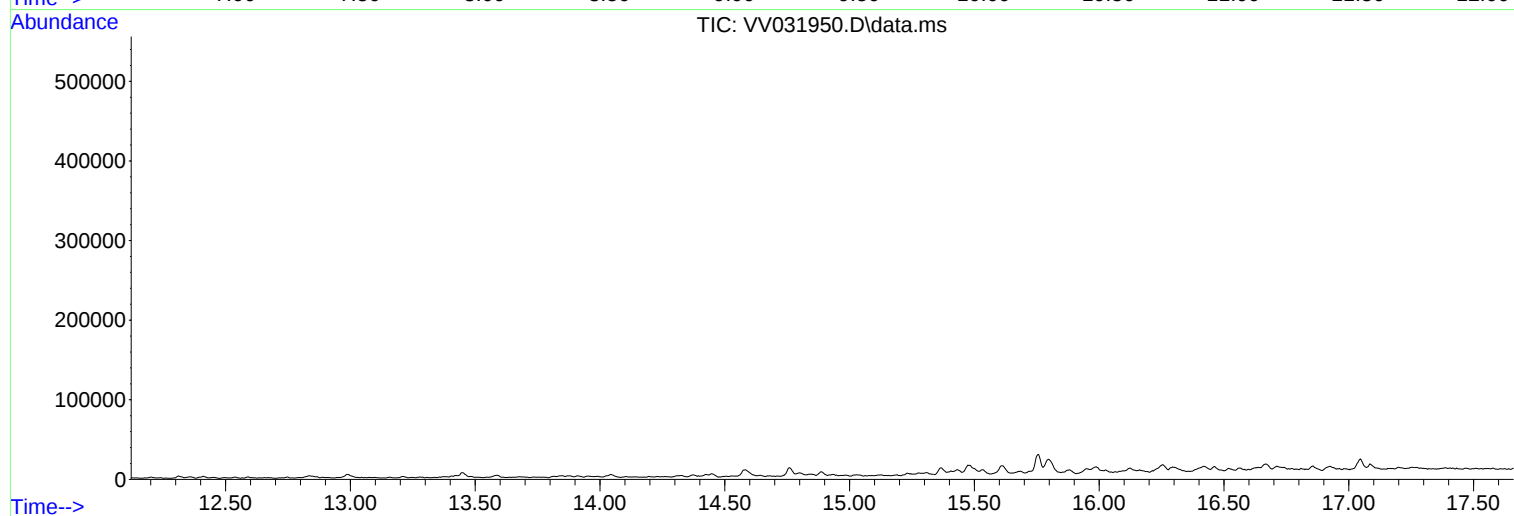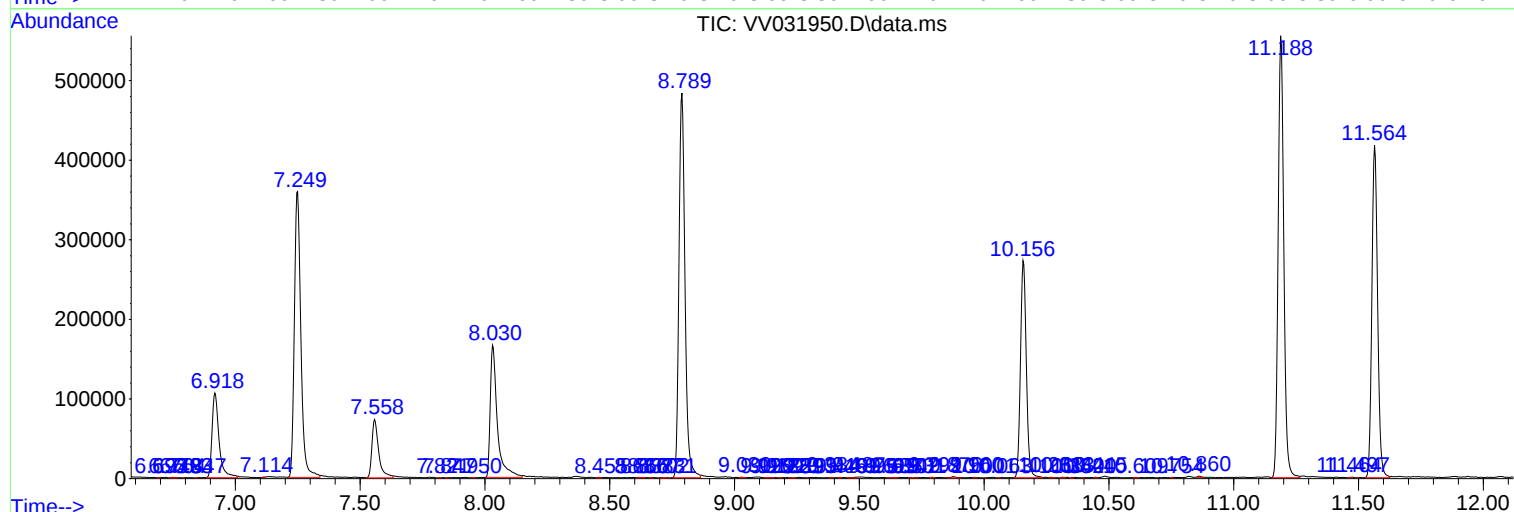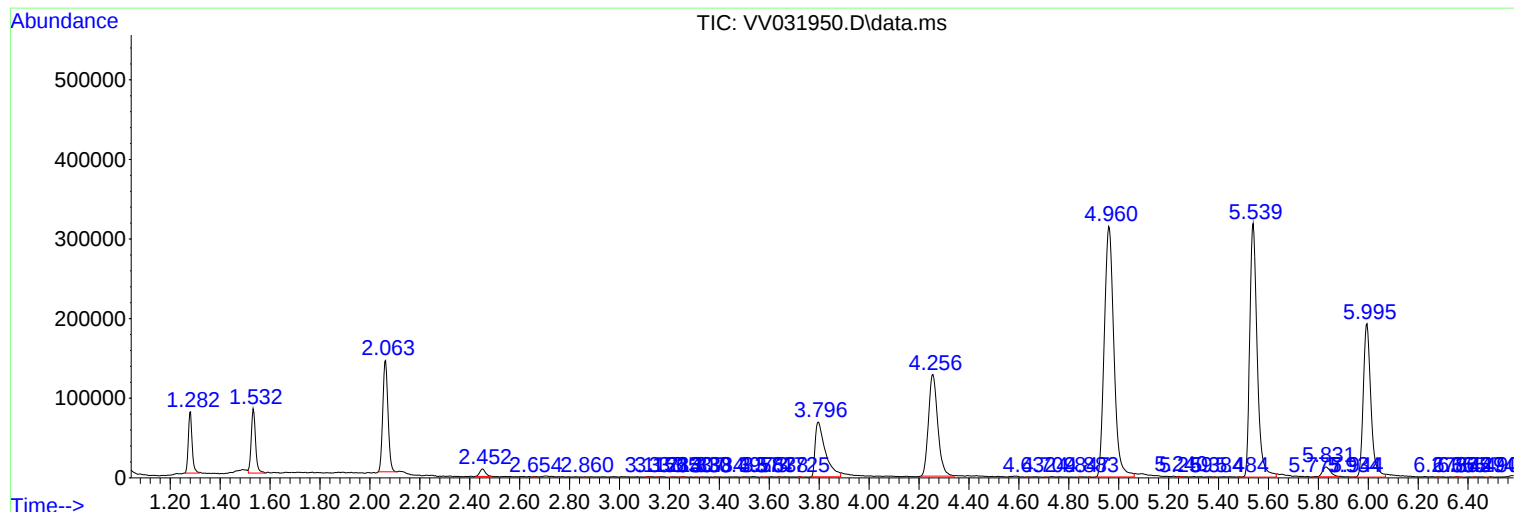

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
Data File : VV031950.D
Acq On : 28 Aug 2023 17:57
Operator : SY/MD
Sample : VIBLK227
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK227

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
Data File : VV031950.D
Acq On : 28 Aug 2023 17:57
Operator : SY/MD
Sample : VIBLK227
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK227

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------