


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082823\
Data File : VV031939.D
Acq On : 28 Aug 2023 10:57
Operator : SY/MD
Sample : BFB207
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB207

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082323WMA.M
Title : VOC Analysis
Last Update : Sat Aug 26 00:50:15 2023

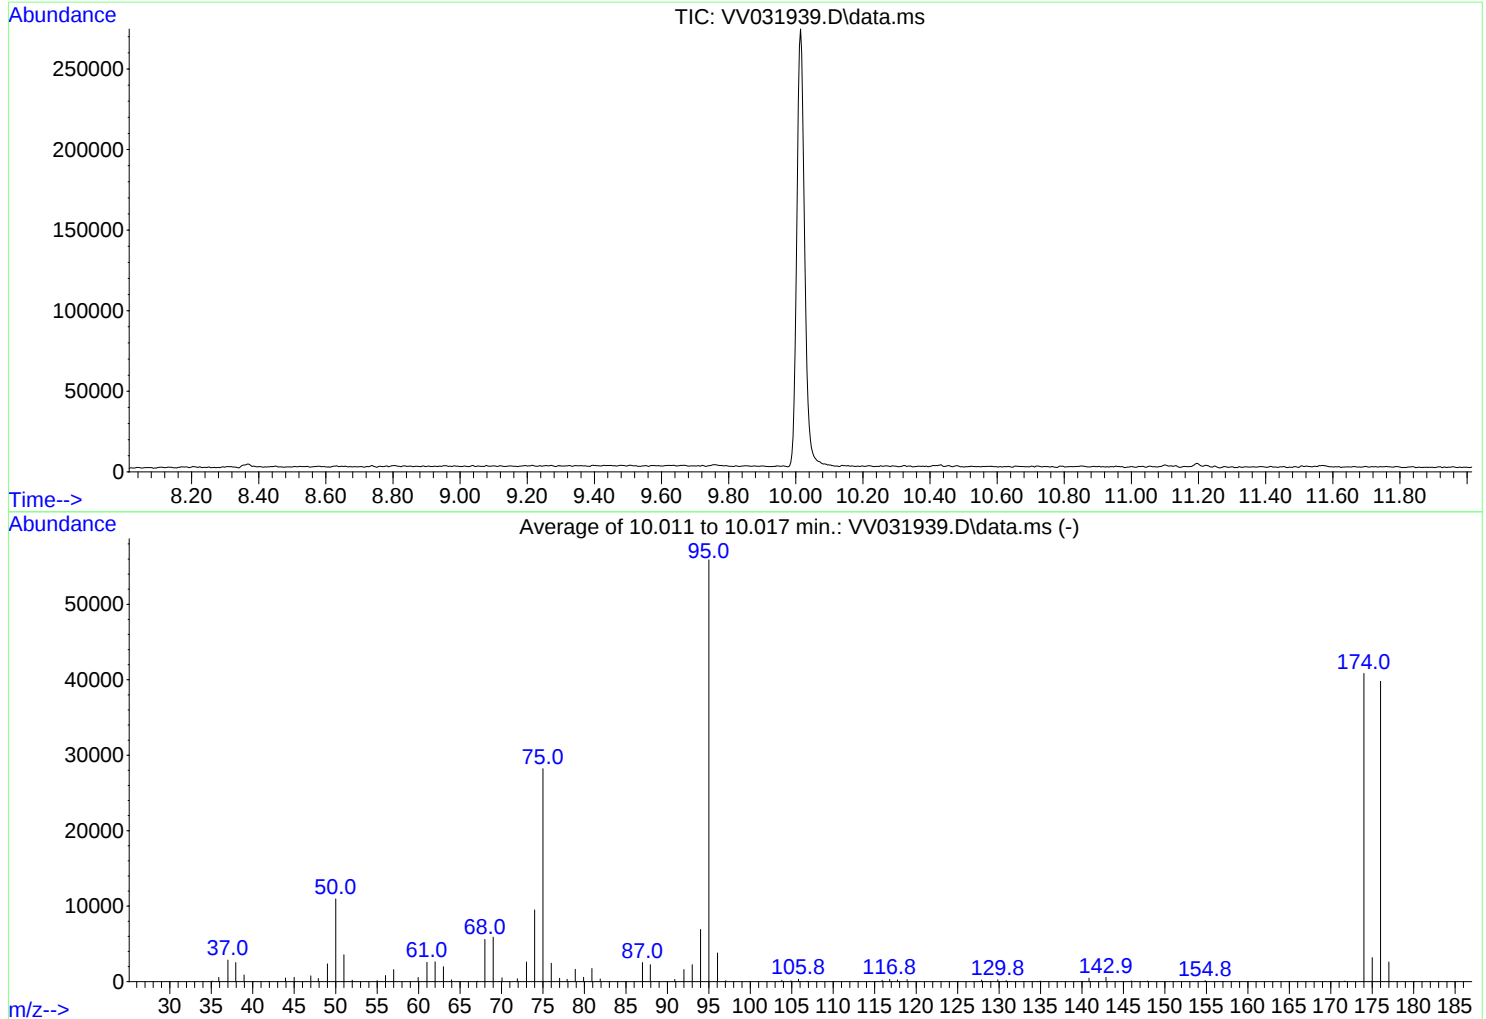

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	10961	PASS
75	95	30	80	50.5	28224	PASS
95	95	100	100	100.0	55891	PASS
96	95	5	9	6.8	3806	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.1	40837	PASS
175	174	5	9	7.8	3182	PASS
176	174	95	105	97.5	39800	PASS
177	176	5	10	6.6	2609	PASS

m/z	Abundance
35.90	1397.0
37.90	475.0
38.80	157.0
39.90	226.0
41.00	168.0
42.00	104.0
43.10	162.0
43.90	388.0
55.00	163.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.00	2005.0
37.00	2816.0
38.00	2944.0
39.00	1094.0
40.00	196.0
40.90	180.0
41.90	143.0
43.00	159.0
44.00	857.0
45.00	542.0
47.00	782.0
47.90	417.0
49.00	2393.0
50.00	10837.0
51.00	3630.0
52.00	181.0
55.00	273.0
56.00	818.0
57.00	1656.0
60.00	530.0
61.00	2565.0
62.00	2713.0
63.00	1842.0
63.90	272.0
67.10	213.0
68.00	5518.0
69.00	6056.0
70.00	497.0
71.90	371.0
73.00	2689.0
74.00	9483.0
75.00	27976.0
76.00	2425.0
77.00	418.0
77.80	307.0
78.90	1587.0
79.90	597.0
80.90	1738.0
81.90	383.0
87.00	2571.0
87.90	2267.0
90.90	316.0
92.00	1524.0
93.00	2199.0
94.00	6882.0
95.00	56024.0
96.00	3764.0
97.00	120.0
103.90	203.0
104.90	116.0
105.80	334.0
106.90	112.0
115.90	202.0
116.80	297.0
117.80	237.0
118.90	304.0
127.90	220.0
129.00	109.0
129.90	274.0
130.90	148.0
134.60	106.0
135.00	111.0
140.90	454.0
142.90	563.0
145.90	107.0
147.90	125.0
154.90	168.0
174.00	39632.0
175.00	3191.0
176.00	38568.0
177.00	2574.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
35.10	258.0
36.00	1971.0
37.00	2946.0
38.00	3071.0
39.00	1069.0
40.00	200.0
41.00	185.0
41.90	129.0
43.00	159.0
44.00	897.0
45.00	581.0
47.00	788.0
47.90	438.0
49.00	2397.0
50.00	11272.0
51.00	3664.0
52.00	200.0
55.00	313.0
56.00	818.0
57.00	1649.0
59.90	538.0
61.00	2639.0
62.00	2728.0
63.00	2039.0
63.90	239.0
68.00	5785.0
69.00	6091.0
70.00	540.0
71.90	390.0
73.00	2727.0
74.00	9770.0
75.00	29096.0
76.00	2485.0
77.00	445.0
77.90	327.0
78.90	1672.0
79.90	586.0
80.90	1819.0
81.90	379.0
87.00	2628.0
87.90	2263.0
90.90	303.0
92.00	1643.0
93.00	2302.0
94.00	7195.0
95.00	57600.0
96.10	3944.0
97.00	121.0
103.80	181.0
104.90	112.0
105.80	325.0
115.90	203.0
116.80	314.0
117.70	242.0
118.90	293.0
127.90	232.0
129.90	272.0
130.90	152.0
134.90	116.0
140.80	488.0
142.90	581.0
145.90	124.0
147.90	117.0
154.90	148.0
156.90	103.0
171.70	130.0
174.00	42192.0
175.00	3308.0
176.00	41168.0
177.00	2693.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207

m/z	Abundance
36.00	1917.0
37.00	2858.0
38.00	2991.0
39.00	965.0
39.90	205.0
41.10	213.0
41.80	112.0
42.90	165.0
44.00	846.0
45.00	593.0
47.00	742.0
47.90	450.0
49.00	2293.0
50.00	10773.0
51.00	3402.0
52.00	191.0
55.00	328.0
56.00	779.0
57.00	1481.0
59.90	563.0
61.00	2503.0
62.00	2477.0
63.00	2035.0
64.00	190.0
68.00	5505.0
69.00	5556.0
70.10	491.0
71.90	365.0
73.00	2417.0
74.00	9237.0
75.00	27600.0
76.00	2383.0
77.00	444.0
78.00	318.0
78.90	1625.0
79.90	524.0
80.90	1647.0
81.90	325.0
87.00	2365.0
88.00	2213.0
90.90	277.0
92.00	1627.0
93.00	2233.0
94.00	6637.0
95.00	54048.0
96.10	3709.0
97.10	117.0
103.70	186.0
104.90	114.0
105.80	293.0
115.90	189.0
116.80	308.0
117.80	222.0
118.90	248.0
127.90	212.0
129.80	236.0
130.80	150.0
140.80	471.0
142.90	557.0
146.00	112.0
154.80	129.0
171.70	135.0
174.00	40688.0
175.00	3047.0
176.00	39664.0
177.00	2561.0

Instrument :
MSVOA_V
ClientSampleId :
BFB207