


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV082918\
Data File : VV007248.D
Acq On : 29 Aug 2018 08:14
Operator : SY/MD
Sample : BFB68
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB68

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082818WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Aug 30 04:42:02 2018

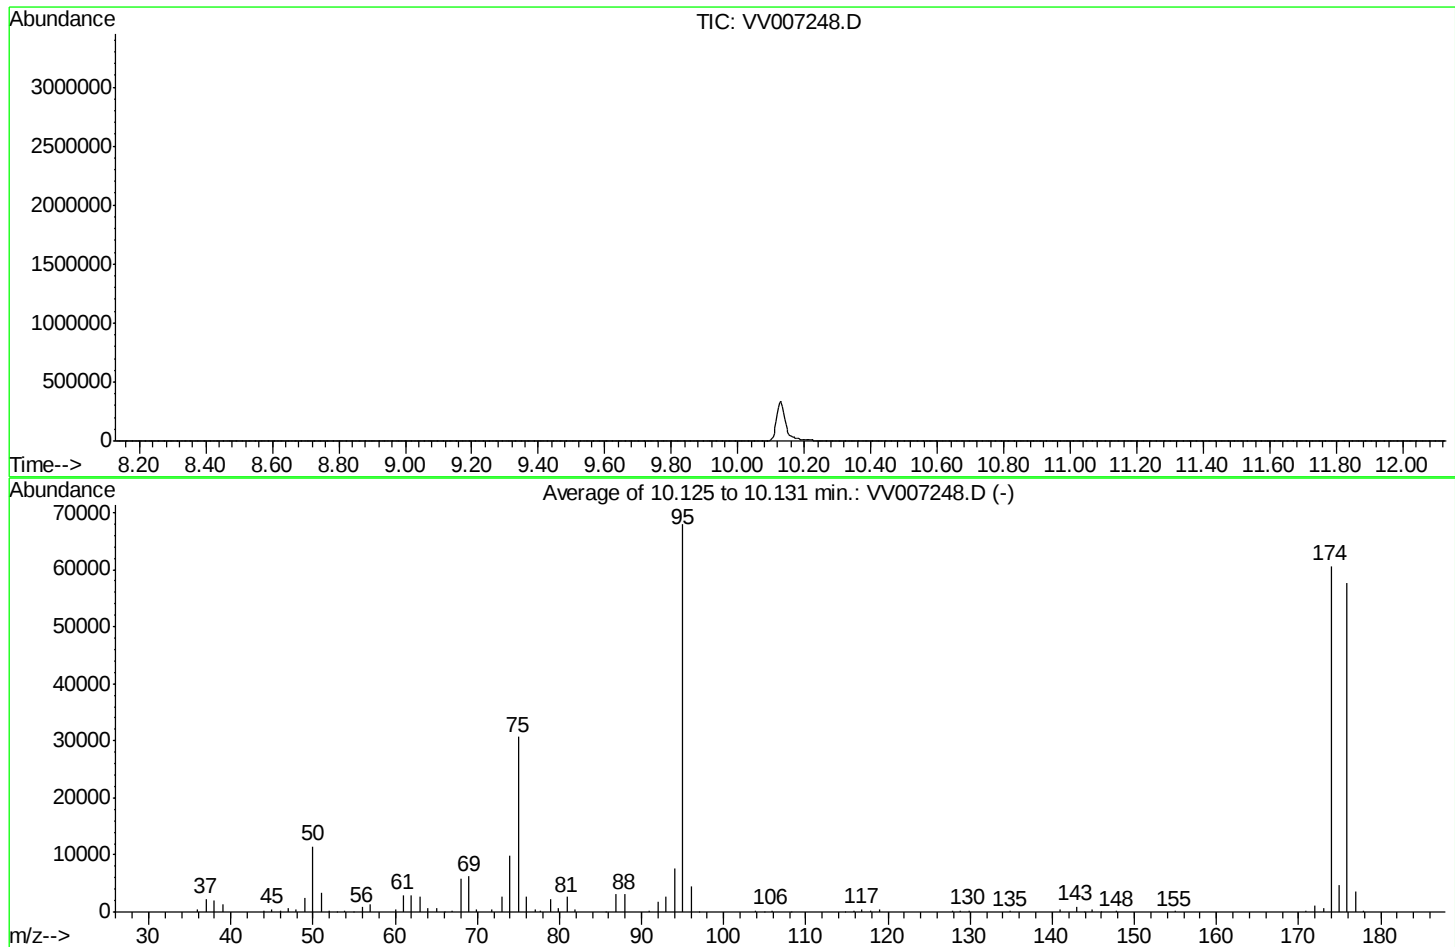

AutoFind: Scans 2872, 2873, 2874; Background Corrected with Scan 2859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	11448	PASS
75	95	30	80	45.2	30706	PASS
95	95	100	100	100.0	67933	PASS
96	95	5	9	6.8	4597	PASS
173	174	0.00	2	1.3	785	PASS
174	95	50	120	89.3	60680	PASS
175	174	5	9	7.7	4700	PASS
176	174	95	101	95.1	57701	PASS
177	176	5	9	6.3	3626	PASS

Scan 2859 (10.083 min): VV007248.D
BFB68

m/z	Abundance
39.90	398.0
43.90	832.0
206.90	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
35.90	524.0
37.00	2383.0
38.00	2193.0
39.10	1230.0
39.80	350.0
44.00	1081.0
45.00	427.0
46.00	133.0
46.90	679.0
48.00	429.0
49.00	2465.0
50.00	11499.0
51.00	3412.0
52.00	230.0
53.90	101.0
54.90	120.0
56.00	899.0
57.00	1348.0
60.00	496.0
61.00	2949.0
62.00	2905.0
63.00	2751.0
64.00	528.0
65.00	766.0
67.00	196.0
68.00	5821.0
69.00	6271.0
69.90	461.0
71.80	553.0
73.00	2620.0
74.00	9692.0
75.00	30872.0
76.00	2577.0
77.00	378.0
77.80	299.0
78.90	2240.0
79.90	792.0
80.90	2598.0
81.90	346.0
86.90	3068.0
87.90	2806.0
90.80	185.0
92.00	1769.0
93.00	2758.0
94.00	7414.0
95.00	67528.0
96.00	4502.0
97.00	147.0
103.80	273.0
104.90	103.0
105.80	261.0
115.90	225.0
116.80	585.0
118.00	259.0
118.90	467.0
127.70	223.0
128.80	180.0
129.80	220.0
134.90	122.0
141.00	475.0
142.90	1101.0
143.90	103.0
144.80	486.0
147.80	110.0
154.90	195.0
170.90	195.0
171.90	1014.0
173.10	766.0
173.90	58160.0
174.90	4593.0
175.90	55536.0
176.90	3608.0
177.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
35.90	536.0
37.00	2372.0
38.00	2180.0
39.00	1271.0
39.90	385.0
44.00	1109.0
45.00	473.0
46.00	143.0
46.90	648.0
48.00	398.0
49.00	2496.0
50.00	11839.0
51.00	3524.0
52.00	237.0
52.90	125.0
53.80	137.0
54.90	115.0
56.00	887.0
57.00	1375.0
60.00	551.0
61.00	3085.0
62.00	3030.0
63.00	2727.0
64.00	612.0
65.00	791.0
66.00	114.0
67.00	241.0
67.90	6021.0
69.00	6376.0
70.00	461.0
71.80	583.0
73.00	2772.0
74.00	10060.0
75.00	31408.0
76.00	2743.0
77.10	393.0
77.80	325.0
78.90	2207.0
79.90	711.0
80.90	2782.0
81.80	408.0
85.70	116.0
86.90	3136.0
87.90	3202.0
90.80	165.0
92.00	1853.0
93.00	2857.0
94.00	7951.0
95.00	70000.0
96.00	4775.0
97.00	122.0
103.80	227.0
105.80	310.0
108.20	115.0
115.90	204.0
116.90	540.0
118.00	262.0
118.90	462.0
127.80	233.0
128.80	174.0
129.90	260.0
134.90	135.0
140.90	569.0
142.90	1025.0
144.80	580.0
145.90	113.0
147.80	118.0
154.90	235.0
170.90	211.0
171.90	1178.0
173.00	812.0
173.90	62696.0
174.90	4839.0
175.90	59224.0
176.90	3706.0
177.80	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68

m/z	Abundance
36.00	508.0
37.00	2310.0
38.00	2006.0
39.00	1295.0
39.90	442.0
44.00	1056.0
45.00	489.0
46.00	120.0
47.00	696.0
47.90	342.0
49.00	2347.0
50.00	11006.0
51.00	3336.0
52.00	184.0
52.90	167.0
53.80	131.0
54.90	112.0
56.00	787.0
56.90	1312.0
60.00	583.0
61.00	2960.0
62.00	2871.0
63.00	2460.0
64.00	635.0
65.00	704.0
66.90	239.0
68.00	5665.0
69.00	5982.0
70.00	419.0
71.80	489.0
73.00	2789.0
74.00	9740.0
75.00	29840.0
76.00	2655.0
76.90	383.0
77.70	286.0
78.90	2146.0
79.90	631.0
80.90	2653.0
81.80	495.0
85.70	141.0
86.90	2941.0
87.90	3187.0
90.90	181.0
92.00	1887.0
93.00	2752.0
94.00	7811.0
95.00	66272.0
96.00	4516.0
103.90	209.0
105.90	298.0
114.70	107.0
115.80	187.0
116.90	482.0
117.90	190.0
118.90	436.0
127.90	259.0
128.80	130.0
129.90	239.0
134.90	125.0
140.90	544.0
142.90	912.0
144.90	617.0
145.90	107.0
147.90	136.0
154.90	241.0
170.90	198.0
171.90	1223.0
173.00	778.0
173.90	61184.0
174.90	4669.0
175.90	58344.0
176.90	3566.0
177.80	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB68