


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV082919\
Data File : VV012437.D
Acq On : 29 Aug 2019 17:19
Operator : SY/MD
Sample : BFB56
Misc : 25mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB56

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082919WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Sep 03 03:10:43 2019

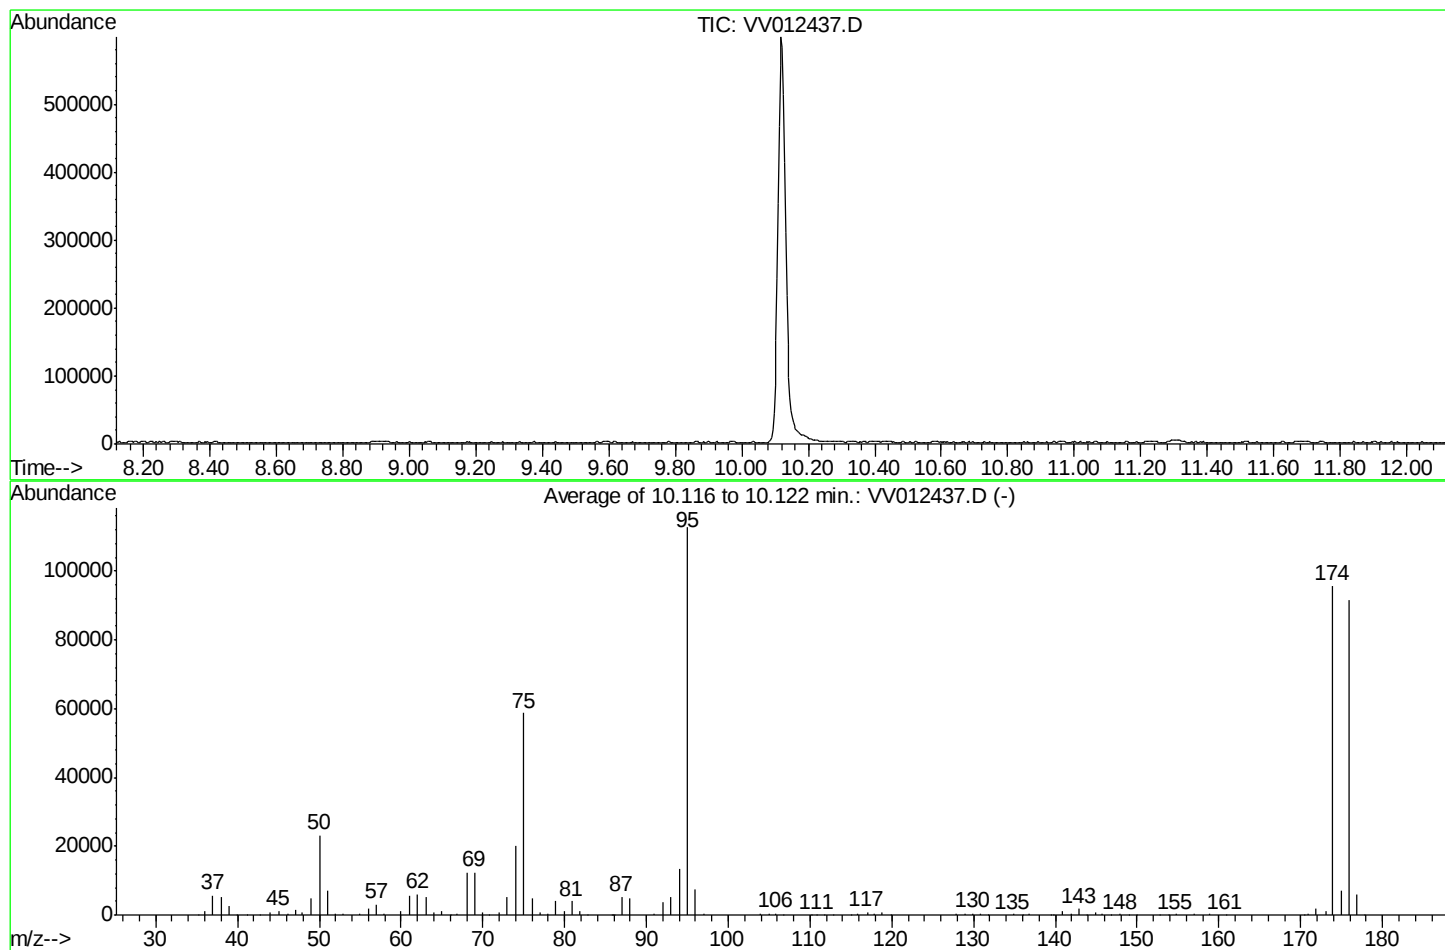

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	23117	PASS
75	95	30	80	52.0	58645	PASS
95	95	100	100	100.0	112690	PASS
96	95	5	9	6.5	7331	PASS
173	174	0.00	2	1.1	1009	PASS
174	95	50	120	85.0	95826	PASS
175	174	5	9	7.5	7208	PASS
176	174	95	101	95.6	91613	PASS
177	176	5	9	6.6	6043	PASS

m/z	Abundance
36.00	1087.0
37.00	5337.0
38.00	5149.0
39.00	2595.0
39.90	1019.0
41.20	121.0
42.90	113.0
43.90	1229.0
45.00	1274.0
46.20	335.0
47.00	1816.0
47.90	590.0
49.00	4633.0
50.00	22960.0
51.00	6683.0
51.90	360.0
52.90	194.0
54.90	347.0
56.00	1841.0
57.00	2948.0
57.90	325.0
60.00	1253.0
61.00	5585.0
62.00	5814.0
63.00	5053.0
64.00	798.0
65.00	1212.0
66.10	154.0
66.90	318.0
68.00	11825.0
69.00	12047.0
70.00	795.0
70.80	105.0
72.00	665.0
73.00	4849.0
74.00	19488.0
75.00	56112.0
76.00	5011.0
77.00	706.0
77.90	456.0
78.90	4075.0
79.90	1115.0
80.90	3999.0
81.90	997.0
82.90	123.0
85.70	205.0
86.10	170.0
86.90	5138.0
87.90	4740.0
90.90	450.0
92.00	3521.0
93.00	5295.0
94.00	12997.0
95.00	108576.0
96.00	7275.0
97.00	284.0
103.90	544.0
105.00	245.0
105.80	435.0
106.70	134.0
110.80	132.0
111.70	138.0
112.70	162.0
115.10	152.0
115.90	464.0
117.00	728.0
117.80	453.0
118.80	654.0
119.80	131.0
127.80	448.0
128.90	255.0
129.90	372.0
130.70	202.0
131.80	113.0
134.80	187.0
136.80	181.0
139.50	175.0
140.90	1137.0
141.90	236.0
142.90	1757.0
143.80	177.0
144.90	632.0
145.70	235.0
146.80	125.0
147.90	241.0
149.00	116.0
150.00	127.0
152.80	132.0
153.90	113.0
154.70	238.0
157.00	211.0
158.80	203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

160.80	175.0
170.90	280.0
171.90	1892.0
173.10	1557.0
173.90	90528.0
174.90	7124.0
175.90	86368.0
176.90	5865.0
177.80	189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
36.00	1262.0
37.00	5863.0
38.00	5382.0
39.00	2584.0
39.90	1031.0
41.30	141.0
42.80	134.0
43.90	1334.0
45.00	1367.0
46.10	302.0
47.00	1686.0
47.90	634.0
49.00	5190.0
50.00	23856.0
51.00	7296.0
51.90	390.0
52.90	227.0
55.00	353.0
56.00	2004.0
57.00	3200.0
57.90	292.0
60.00	1172.0
61.00	5810.0
62.00	6235.0
63.00	5483.0
64.00	857.0
65.00	1250.0
66.00	114.0
66.90	391.0
68.00	12576.0
69.00	12831.0
70.00	905.0
72.00	709.0
73.00	5357.0
74.00	20824.0
75.00	60504.0
76.00	4991.0
77.00	757.0
77.90	496.0
78.90	4176.0
79.90	1257.0
80.90	4127.0
81.90	1011.0
82.90	123.0
85.80	236.0
86.90	5539.0
87.90	5026.0
90.90	473.0
92.00	3676.0
93.00	5509.0
94.00	14010.0
95.00	116688.0
96.00	7582.0
97.00	254.0
103.80	556.0
104.90	275.0
105.90	547.0
110.20	105.0
110.80	182.0
111.70	166.0
112.80	167.0
115.10	168.0
115.90	515.0
117.00	800.0
117.80	444.0
118.90	720.0
119.80	118.0
127.80	418.0
128.90	275.0
129.90	435.0
130.80	210.0
134.90	243.0
135.90	109.0
136.80	223.0
139.40	179.0
140.90	1277.0
141.90	251.0
143.00	1871.0
143.80	176.0
144.90	636.0
145.80	225.0
146.90	119.0
147.90	300.0
149.00	123.0
149.90	130.0
152.80	161.0
153.80	150.0
154.70	282.0
156.90	247.0
158.80	225.0
160.80	160.0
170.50	171.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

170.90	251.0
171.90	2038.0
173.90	99144.0
174.90	7453.0
175.90	94768.0
176.90	6249.0
177.80	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

m/z	Abundance
35.20	108.0
36.00	1349.0
37.00	5732.0
38.00	5133.0
39.00	2372.0
39.90	1002.0
41.10	128.0
42.70	148.0
44.00	1334.0
45.00	1177.0
46.10	214.0
47.10	1468.0
47.90	705.0
49.00	5079.0
50.00	22536.0
51.00	7212.0
52.00	352.0
53.00	218.0
55.00	342.0
56.00	1989.0
57.00	3082.0
57.90	220.0
60.00	1028.0
61.00	5602.0
62.00	5892.0
63.00	5190.0
64.00	830.0
65.00	1277.0
66.00	130.0
66.90	404.0
68.00	12219.0
69.00	12060.0
70.00	982.0
72.00	702.0
73.00	5242.0
74.00	20048.0
75.00	59320.0
76.00	4543.0
77.00	740.0
77.90	532.0
78.90	3844.0
79.90	1257.0
80.90	3885.0
81.90	989.0
82.80	132.0
85.90	228.0
87.00	5090.0
87.90	4925.0
91.00	518.0
92.00	3450.0
93.00	5175.0
94.00	13552.0
95.00	112808.0
96.00	7138.0
97.00	185.0
103.90	454.0
104.90	246.0
105.90	589.0
110.90	210.0
111.80	176.0
112.90	143.0
115.10	166.0
115.80	481.0
117.00	774.0
117.90	469.0
118.90	811.0
127.80	359.0
128.90	253.0
129.90	481.0
130.90	235.0
134.90	245.0
136.00	130.0
136.90	259.0
139.40	153.0
139.80	146.0
140.90	1272.0
142.00	228.0
143.00	1723.0
143.80	149.0
144.80	608.0
145.80	221.0
146.90	122.0
147.90	301.0
148.90	114.0
149.90	132.0
152.70	153.0
153.80	173.0
154.80	297.0
156.90	301.0
158.80	204.0
160.90	149.0
170.90	243.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

171.90	1993.0
173.00	1472.0
173.90	97808.0
174.90	7049.0
175.90	93704.0
176.90	6015.0
177.80	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56

Scan 2794 (10.074 min): VV012437.D
BFB56

m/z	Abundance
35.90	183.0
36.50	121.0
39.90	843.0
40.80	102.0
43.90	669.0

Instrument :
MSVOA_V
ClientSampleId :
BFB56