

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082922\
 Data File : VV027569.D
 Acq On : 29 Aug 2022 17:59
 Operator : SY/MD
 Sample : N4366-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F43

Quant Time: Aug 30 04:19:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Aug 27 03:12:26 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	123009	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	119488	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	52529	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	43802	5.003	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 100.000%		
7) Chloroethane-d5	1.565	69	35926	5.607	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 112.200%		
11) 1,1-Dichloroethene-d2	2.105	63	66606	3.263	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 65.200%		
20) 2-Butanone-d5	3.899	46	66202	60.763	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 121.520%		
24) Chloroform-d	4.346	84	82906	4.736	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 94.800%		
26) 1,2-Dichloroethane-d4	5.031	65	36645	4.839	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 96.800%		
32) Benzene-d6	5.047	84	134131	4.053	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 81.000%		
36) 1,2-Dichloropropane-d6	6.069	67	39475	4.102	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 82.000%		
41) Toluene-d8	7.317	98	118780	3.975	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 79.400%		
43) trans-1,3-Dichloroprop...	7.632	79	8367	2.540	ug/L	0.01
Spiked Amount	5.000	Range 55 - 130	Recovery	= 50.800%#		
46) 2-Hexanone-d5	8.092	63	41232	38.019	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 76.040%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	24586	4.012	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 80.200%		
66) 1,2-Dichlorobenzene-d4	11.622	152	36084	4.634	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 92.600%		
Target Compounds						
14) Carbon disulfide	2.291	76	1937	0.076	ug/L #	Qvalue 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082922\
Data File : VV027569.D
Acq On : 29 Aug 2022 17:59
Operator : SY/MD
Sample : N4366-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F43

Quant Time: Aug 30 04:19:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Aug 27 03:12:26 2022
Response via : Initial Calibration

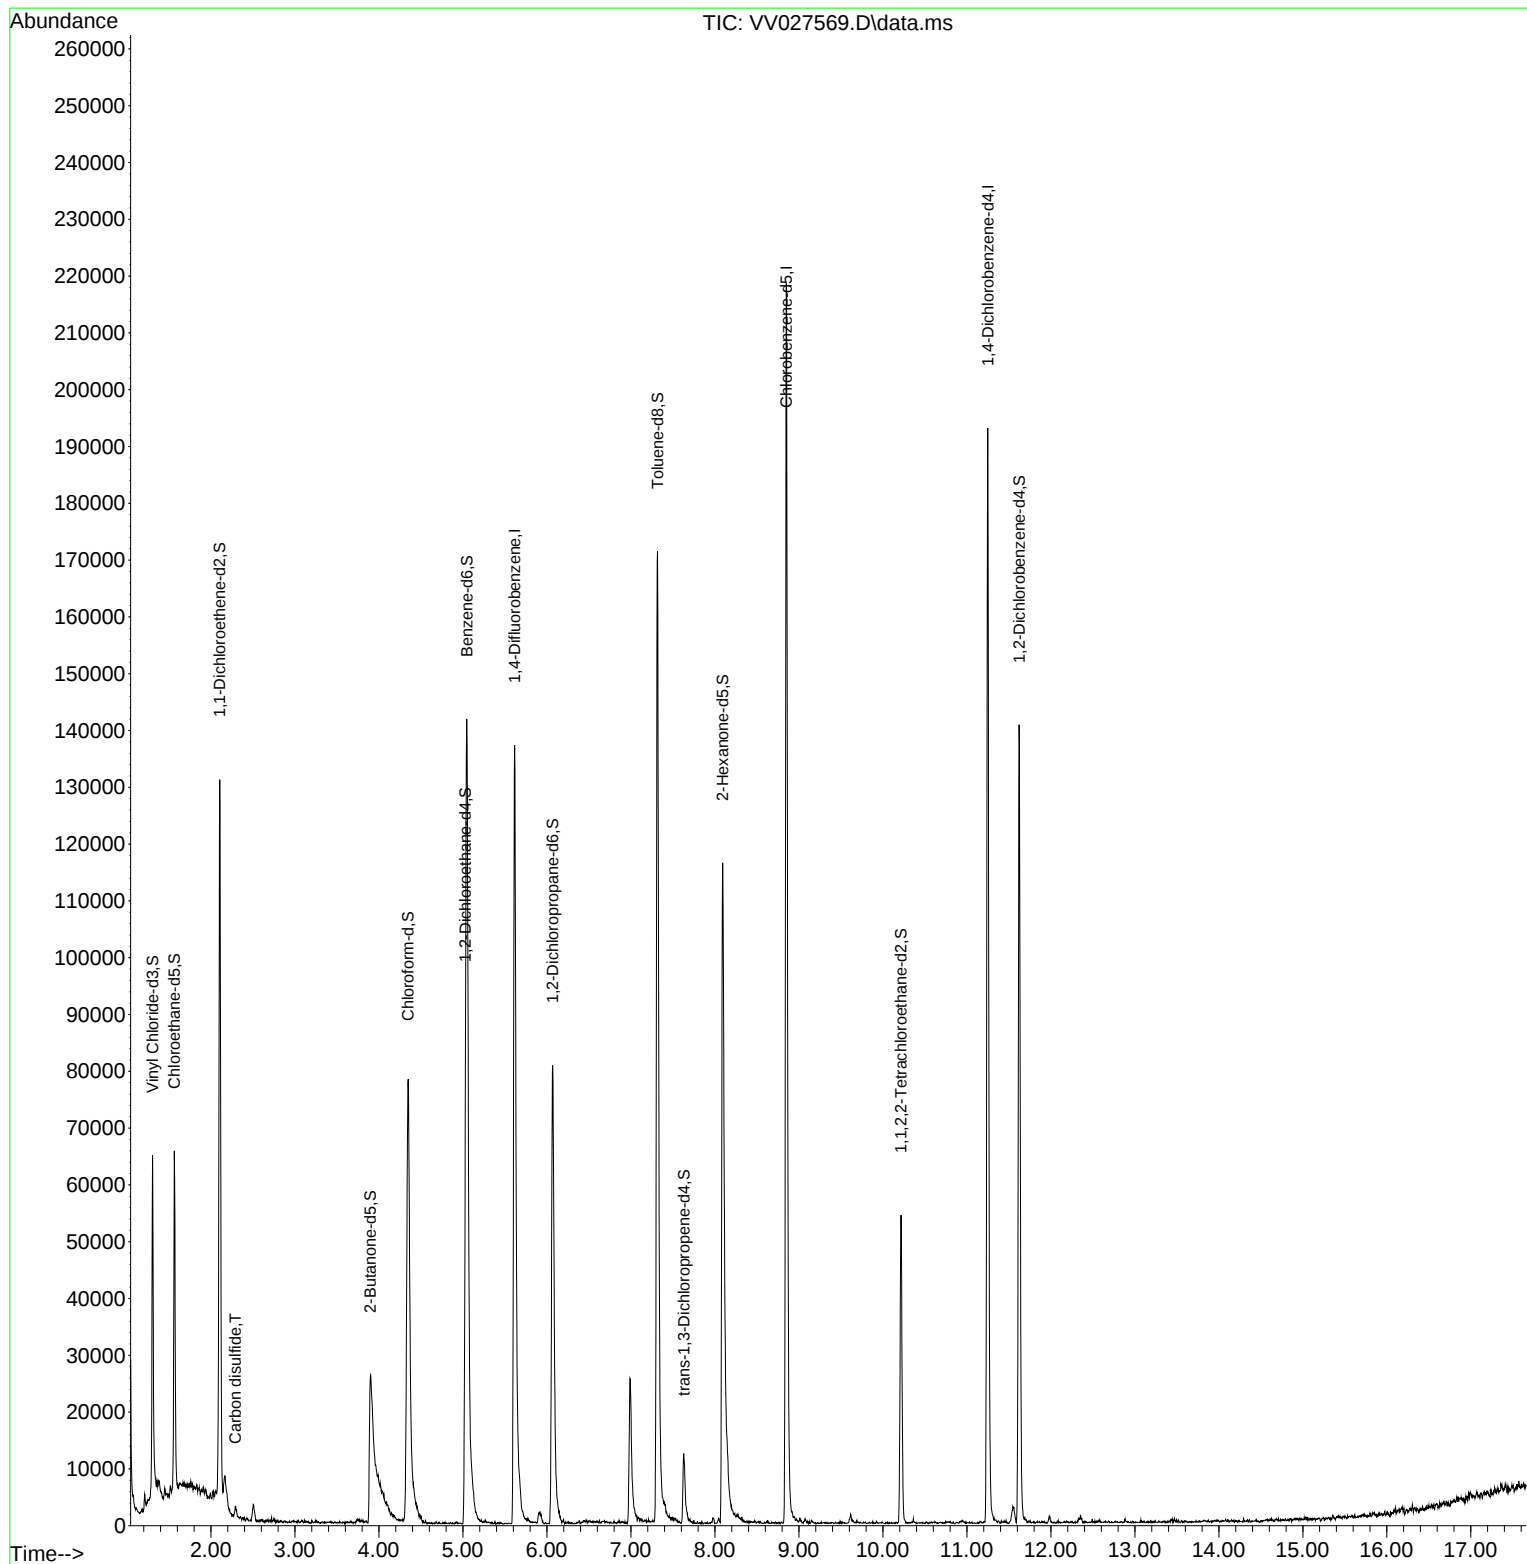

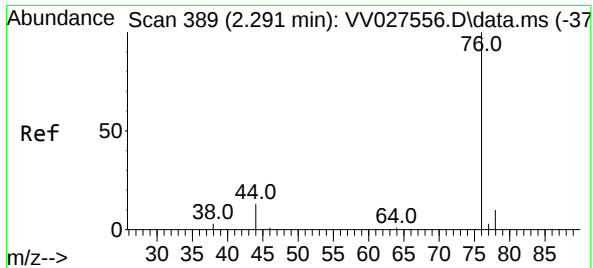

#14
Carbon disulfide
Concen: 0.076 ug/L
RT: 2.291 min Scan# 31
Delta R.T. 0.003 min
Lab File: VV027569.D
Acq: 29 Aug 2022 17:59

Instrument :
MSVOA_V
ClientSampleId :
F5F43

Tgt Ion: 76 Resp: 1937
Ion Ratio Lower Upper
76 100
78 12.1 7.3 10.9#

