

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082922\
 Data File : VV027563.D
 Acq On : 29 Aug 2022 15:31
 Operator : SY/MD
 Sample : N4366-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F09

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027563.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	91	rBV	47159	49158	12.74%	1.480%
2	1.564	152	163	175	rBV	64488	79984	20.73%	2.409%
3	2.108	321	332	343	rBV	121824	174976	45.35%	5.269%
4	2.510	447	457	464	rBV4	2749	4078	1.06%	0.123%
5	3.889	877	886	921	rBV	35111	112081	29.05%	3.375%
6	4.349	1013	1029	1061	rBV2	71224	208696	54.09%	6.285%
7	5.047	1232	1246	1274	rBV3	144254	378499	98.10%	11.398%
8	5.616	1409	1423	1465	rBV	138625	309144	80.12%	9.309%
9	5.924	1506	1519	1535	rBV	4990	11666	3.02%	0.351%
10	6.069	1551	1564	1590	rBV2	85995	189735	49.17%	5.714%
11	6.522	1692	1705	1716	rBV5	3659	7424	1.92%	0.224%
12	6.992	1839	1851	1867	rBV2	22298	46379	12.02%	1.397%
13	7.317	1941	1952	1975	rBV	148864	278312	72.13%	8.381%
14	7.632	2041	2050	2067	rBV2	13320	27121	7.03%	0.817%
15	7.976	2146	2157	2171	rBV2	38100	67458	17.48%	2.031%
16	8.091	2184	2193	2232	rBV2	137786	314053	81.39%	9.457%
17	8.854	2419	2430	2447	rBV	228120	385841	100.00%	11.619%
18	10.217	2840	2854	2868	rBV	74015	113604	29.44%	3.421%
19	11.249	3164	3175	3197	rBV	207152	329611	85.43%	9.926%
20	11.625	3280	3292	3314	rBV	142844	232959	60.38%	7.015%




Sum of corrected areas: 3320779

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082922\
Data File : VV027563.D
Acq On : 29 Aug 2022 15:31
Operator : SY/MD
Sample : N4366-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

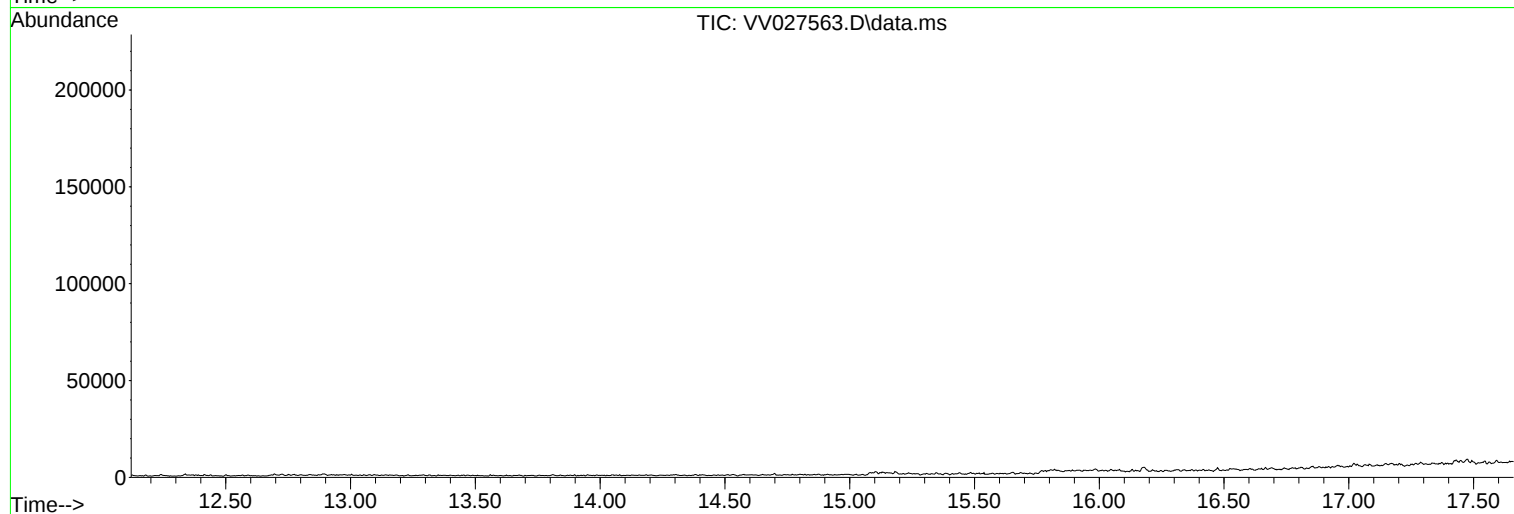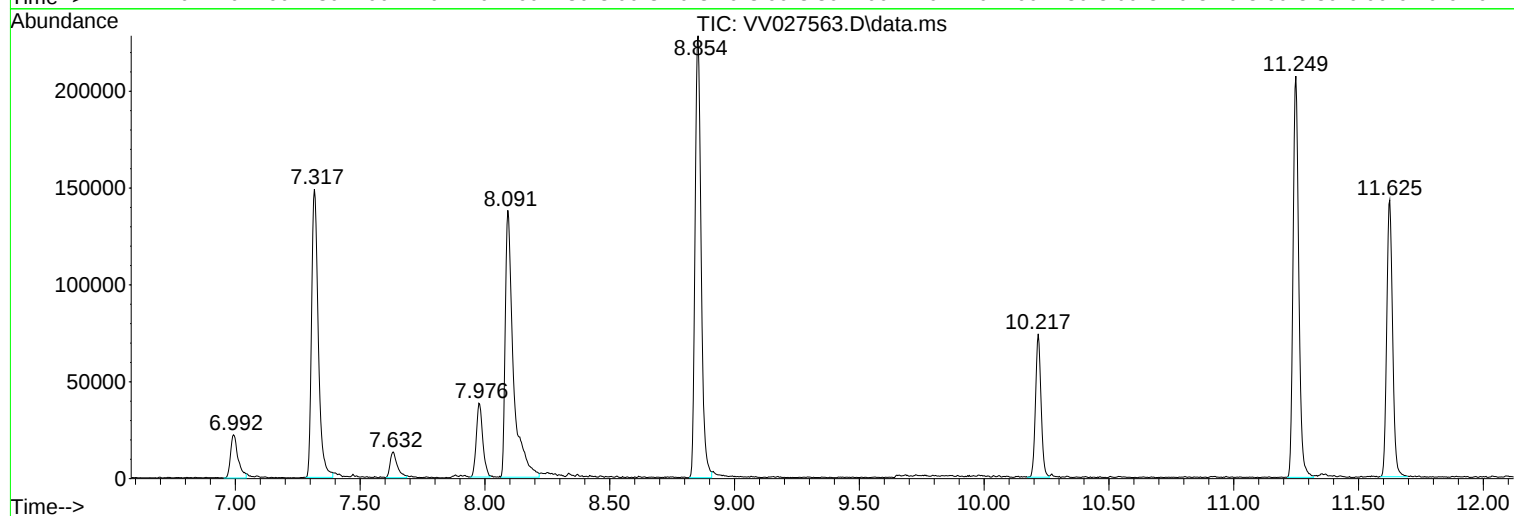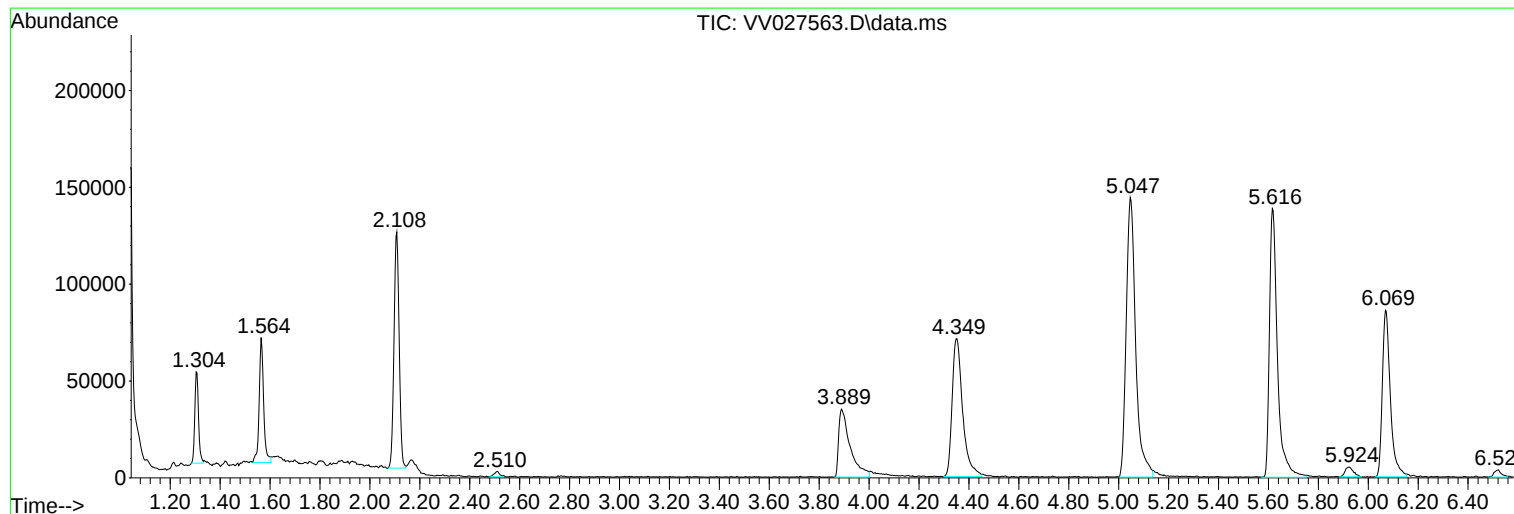

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082922\
Data File : VV027563.D
Acq On : 29 Aug 2022 15:31
Operator : SY/MD
Sample : N4366-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082922\
Data File : VV027563.D
Acq On : 29 Aug 2022 15:31
Operator : SY/MD
Sample : N4366-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F09

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc