

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082922\
 Data File : VV027570.D
 Acq On : 29 Aug 2022 18:24
 Operator : SY/MD
 Sample : N4402-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVA8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	72	82	94	rBV	52433	61789	13.25%	1.572%
2	1.565	153	163	174	rBV	67566	80946	17.36%	2.059%
3	2.105	321	331	347	rVB	129496	188299	40.39%	4.789%
4	2.770	523	538	554	rBV2	18168	41484	8.90%	1.055%
5	3.896	879	888	910	rBV2	27945	96133	20.62%	2.445%
6	4.346	1012	1028	1056	rBV2	85345	245852	52.73%	6.253%
7	5.047	1226	1246	1284	rBV2	173063	466209	100.00%	11.858%
8	5.616	1412	1423	1462	rBV	153847	339601	72.84%	8.638%
9	5.918	1504	1517	1533	rBV8	9766	22977	4.93%	0.584%
10	6.069	1551	1564	1586	rBV2	104557	228144	48.94%	5.803%
11	6.989	1841	1850	1875	rBV2	25984	52944	11.36%	1.347%
12	7.317	1941	1952	1980	rBV	174176	332253	71.27%	8.451%
13	7.629	2041	2049	2066	rBV3	14431	29610	6.35%	0.753%
14	7.973	2142	2156	2180	rBV	141382	255665	54.84%	6.503%
15	8.092	2183	2193	2225	rBV2	137020	345016	74.00%	8.776%
16	8.850	2419	2429	2454	rBV	242397	410653	88.08%	10.445%
17	10.217	2841	2854	2871	rBV2	70093	112261	24.08%	2.855%
18	11.249	3164	3175	3204	rBV	207391	328742	70.51%	8.362%
19	11.535	3252	3264	3281	rBV3	16307	31556	6.77%	0.803%
20	11.622	3281	3291	3311	rVB	161683	261424	56.07%	6.649%




Sum of corrected areas: 3931558

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082922\
Data File : VV027570.D
Acq On : 29 Aug 2022 18:24
Operator : SY/MD
Sample : N4402-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

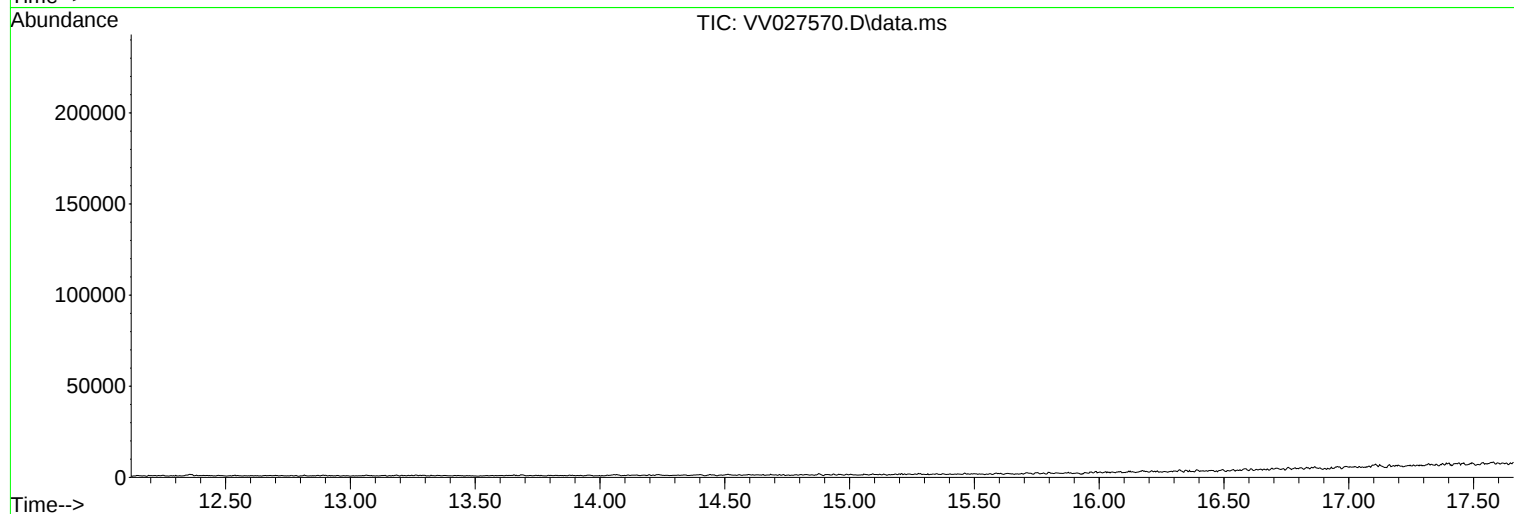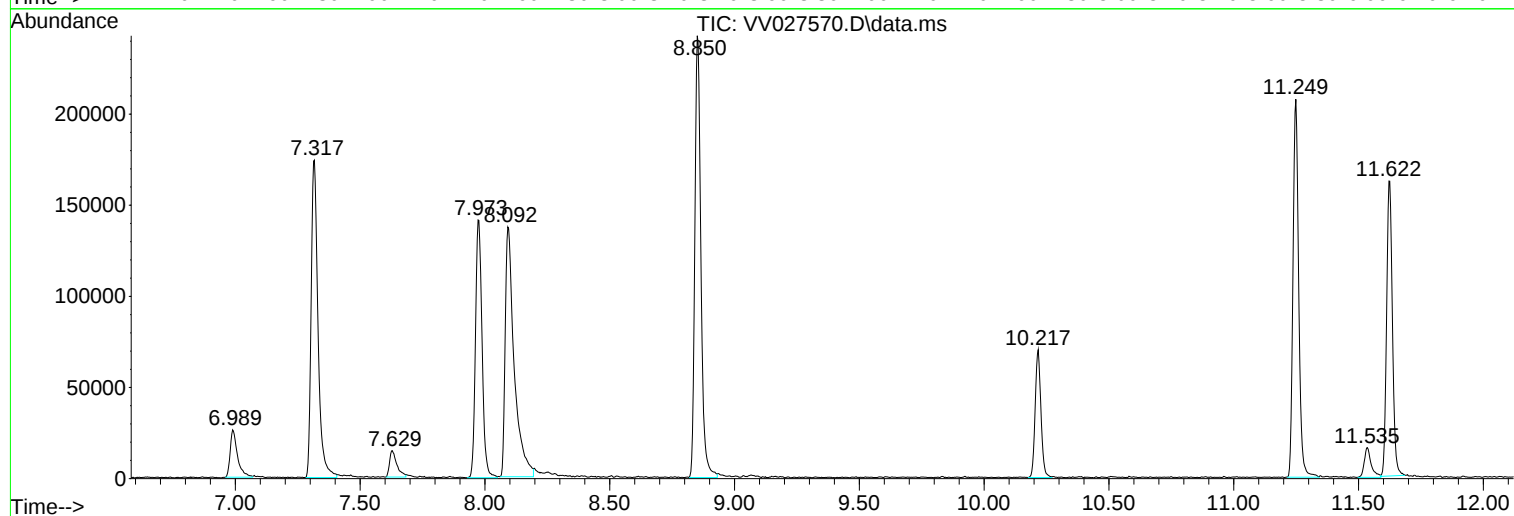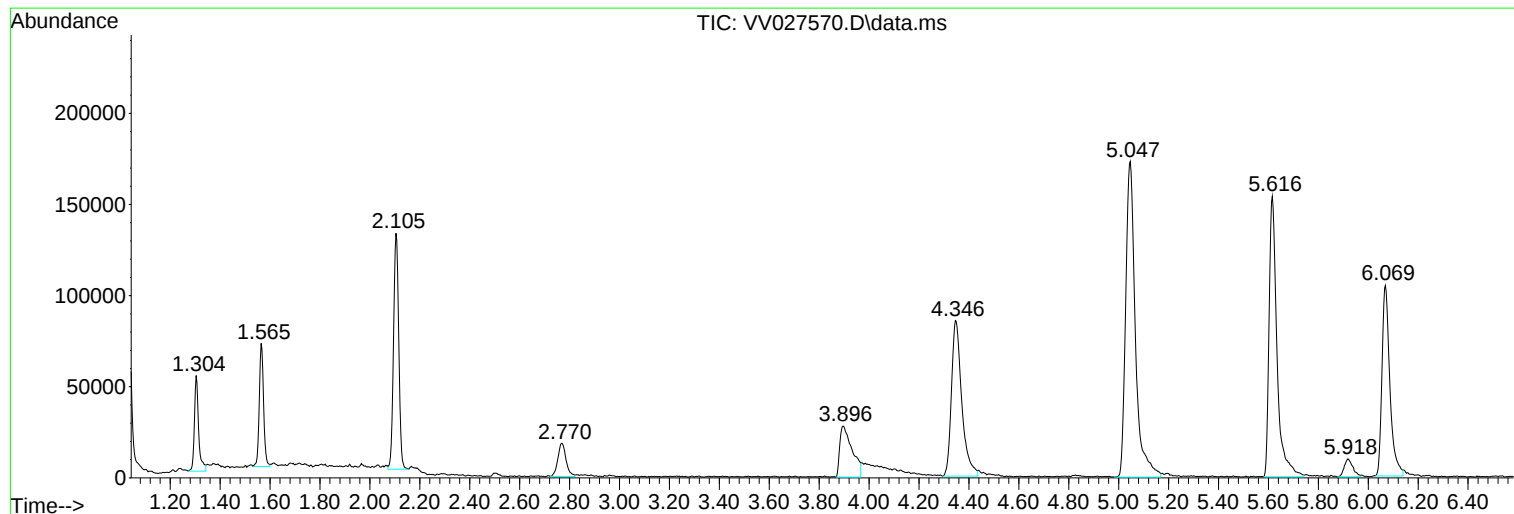

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082922\
Data File : VV027570.D
Acq On : 29 Aug 2022 18:24
Operator : SY/MD
Sample : N4402-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082922\
Data File : VV027570.D
Acq On : 29 Aug 2022 18:24
Operator : SY/MD
Sample : N4402-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
