
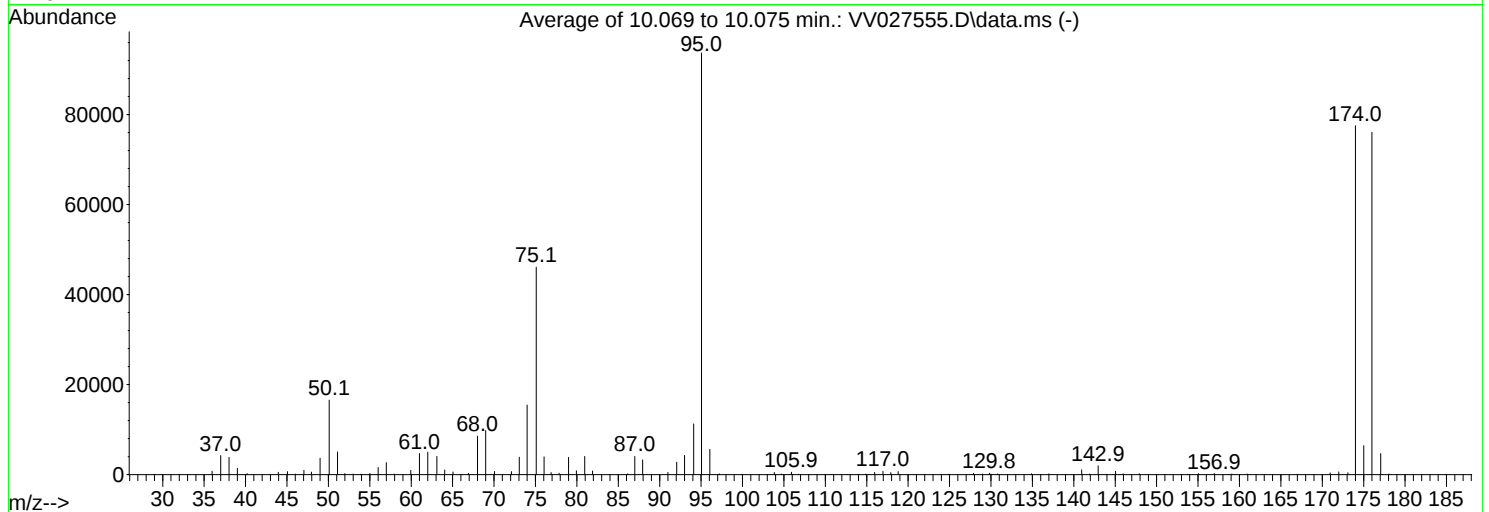


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV082922\
Data File : VV027555.D
Acq On : 29 Aug 2022 09:42
Operator : SY/MD
Sample : BFB362
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB362

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Sep 01 02:33:10 2022

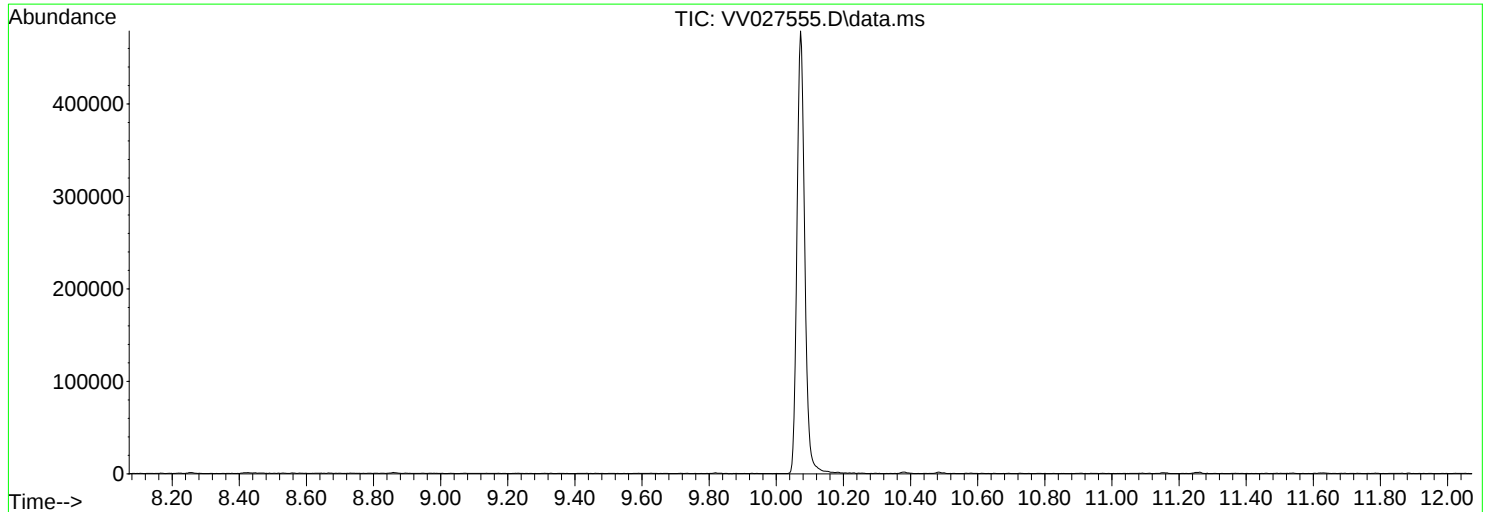

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	16560	PASS
75	95	30	80	49.2	46101	PASS
95	95	100	100	100.0	93717	PASS
96	95	5	9	6.0	5617	PASS
173	174	0.00	2	0.6	431	PASS
174	95	50	120	82.7	77520	PASS
175	174	5	9	8.3	6432	PASS
176	174	95	105	98.1	76061	PASS
177	176	5	10	6.2	4688	PASS

m/z	Abundance
39.80	166.0
43.80	181.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362

m/z	Abundance
35.90	797.0
37.00	4005.0
38.00	3739.0
39.00	1424.0
40.20	234.0
44.00	684.0
45.10	733.0
46.10	151.0
47.10	984.0
48.00	546.0
49.00	3668.0
50.10	16335.0
51.10	5035.0
52.00	228.0
53.00	135.0
54.90	206.0
56.00	1535.0
57.00	2562.0
58.00	120.0
59.90	929.0
61.00	4652.0
62.00	5150.0
63.10	3999.0
64.00	1034.0
65.10	647.0
66.80	271.0
68.00	8307.0
69.00	9456.0
70.00	741.0
72.10	629.0
73.00	3652.0
74.00	15046.0
75.10	45608.0
76.00	3841.0
76.90	500.0
77.80	324.0
79.00	3614.0
79.90	778.0
81.00	3977.0
81.90	740.0
86.20	181.0
87.00	4135.0
87.90	3177.0
91.00	498.0
92.10	2937.0
93.00	4097.0
94.10	10877.0
95.00	91064.0
96.00	5868.0
97.10	211.0
103.80	496.0
104.70	119.0
105.90	515.0
106.70	107.0
110.70	103.0
115.00	161.0
116.00	463.0
117.00	777.0
117.90	412.0
118.80	628.0
124.80	102.0
127.90	332.0
129.00	168.0
129.80	327.0
130.00	331.0
130.80	177.0
134.90	188.0
137.00	204.0
140.90	1031.0
141.90	123.0
143.00	1854.0
143.90	120.0
145.10	662.0
146.00	170.0
147.90	237.0
153.80	103.0
155.00	244.0
157.00	305.0
158.70	128.0
159.10	124.0
160.90	151.0
171.00	336.0
172.00	557.0
174.00	74016.0
175.00	6128.0
176.00	72376.0
177.10	4631.0
178.10	158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362

m/z	Abundance
35.90	813.0
37.00	4400.0
38.00	3952.0
39.00	1473.0
40.20	212.0
44.00	716.0
45.10	680.0
46.10	157.0
47.10	985.0
47.90	570.0
49.00	3835.0
50.10	17088.0
51.10	5253.0
52.00	251.0
53.00	148.0
53.90	125.0
55.00	264.0
56.00	1652.0
57.00	2783.0
58.00	160.0
60.00	1024.0
61.00	4959.0
62.00	5127.0
63.10	4182.0
64.00	1079.0
65.00	622.0
66.10	101.0
66.90	262.0
68.00	8710.0
69.00	10162.0
70.00	749.0
72.10	729.0
73.00	4051.0
74.00	15968.0
75.10	47560.0
76.10	4067.0
76.90	492.0
77.90	341.0
79.00	4005.0
80.00	865.0
80.90	4199.0
81.90	861.0
82.90	119.0
86.10	183.0
87.00	4231.0
88.00	3383.0
91.00	507.0
92.10	2806.0
93.00	4415.0
94.10	11660.0
95.10	97272.0
96.00	5725.0
97.20	187.0
103.90	504.0
104.70	139.0
105.90	565.0
106.70	107.0
111.90	110.0
114.90	134.0
115.90	508.0
117.00	756.0
117.90	492.0
118.80	705.0
124.90	101.0
127.90	327.0
129.00	139.0
129.80	326.0
130.80	182.0
134.90	221.0
137.00	210.0
140.90	1099.0
141.90	143.0
143.00	2031.0
143.90	130.0
145.10	780.0
145.90	170.0
147.90	223.0
153.70	104.0
155.10	231.0
157.00	249.0
159.10	176.0
161.00	164.0
170.90	404.0
172.00	606.0
174.00	80368.0
175.00	6744.0
176.00	78712.0
177.10	4755.0
178.00	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362

m/z	Abundance
36.00	799.0
37.00	4243.0
38.00	3877.0
39.00	1395.0
40.20	184.0
40.90	111.0
44.00	726.0
44.90	615.0
46.00	128.0
47.00	874.0
47.90	576.0
49.00	3545.0
50.10	16258.0
51.10	4824.0
52.00	287.0
53.00	158.0
53.90	127.0
55.10	293.0
56.00	1599.0
57.00	2611.0
57.90	191.0
60.00	957.0
61.00	4513.0
62.00	4619.0
63.10	3955.0
64.10	936.0
65.00	559.0
66.20	115.0
67.00	321.0
68.00	8683.0
69.00	9828.0
70.10	669.0
72.10	675.0
73.10	3944.0
74.00	15431.0
75.10	45136.0
76.10	3956.0
76.90	417.0
77.90	345.0
79.00	3915.0
80.00	929.0
80.90	4001.0
81.90	863.0
83.00	120.0
86.10	130.0
87.00	3821.0
88.00	3227.0
91.00	487.0
92.00	2611.0
93.00	4313.0
94.10	11320.0
95.10	92816.0
96.10	5259.0
97.30	138.0
103.90	453.0
104.70	134.0
105.90	512.0
106.80	102.0
111.90	108.0
112.70	110.0
114.80	132.0
116.00	486.0
116.80	743.0
117.90	449.0
118.80	692.0
127.90	313.0
129.00	123.0
129.80	337.0
130.80	156.0
134.90	210.0
137.00	170.0
141.00	1131.0
141.90	162.0
142.90	1999.0
143.90	115.0
145.00	824.0
145.90	158.0
147.90	190.0
153.70	106.0
155.00	205.0
156.90	205.0
159.10	188.0
161.00	174.0
171.00	417.0
172.00	664.0
173.10	1293.0
174.00	78176.0
175.00	6425.0
176.00	77096.0
177.00	4679.0
178.00	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB362