

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083018\
 Data File : VV007274.D
 Acq On : 30 Aug 2018 21:13
 Operator : SY/MD
 Sample : J4633-04
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB3J8

Quant Time: Aug 31 02:46:51 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR083018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 31 02:32:21 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	273333	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	269383	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	110504	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	80138	3.35	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.00%
7) Chloroethane-d5	1.58	69	74931	4.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.60%
11) 1,1-Dichloroethene-d2	2.13	63	108595	2.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	54.40%#
20) 2-Butanone-d5	3.97	46	224299	48.08	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.16%
24) Chloroform-d	4.41	84	185869	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.40%
26) 1,2-Dichloroethane-d4	5.09	65	91503	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.00%
32) Benzene-d6	5.10	84	347935	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.40%
36) 1,2-Dichloropropane-d6	6.12	67	119507	4.52	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.40%
41) Toluene-d8	7.37	98	263949	3.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	70.40%
43) trans-1,3-Dichloropropene-	7.67	79	35699	3.88	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.60%
46) 2-Hexanone-d5	8.15	63	140485	44.61	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.22%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	90602	4.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	102968	4.66	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	17963	6.99 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV083018\
Data File : VV007274.D
Acq On : 30 Aug 2018 21:13
Operator : SY/MD
Sample : J4633-04
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB3J8

Quant Time: Aug 31 02:46:51 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR083018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 31 02:32:21 2018
Response via : Initial Calibration

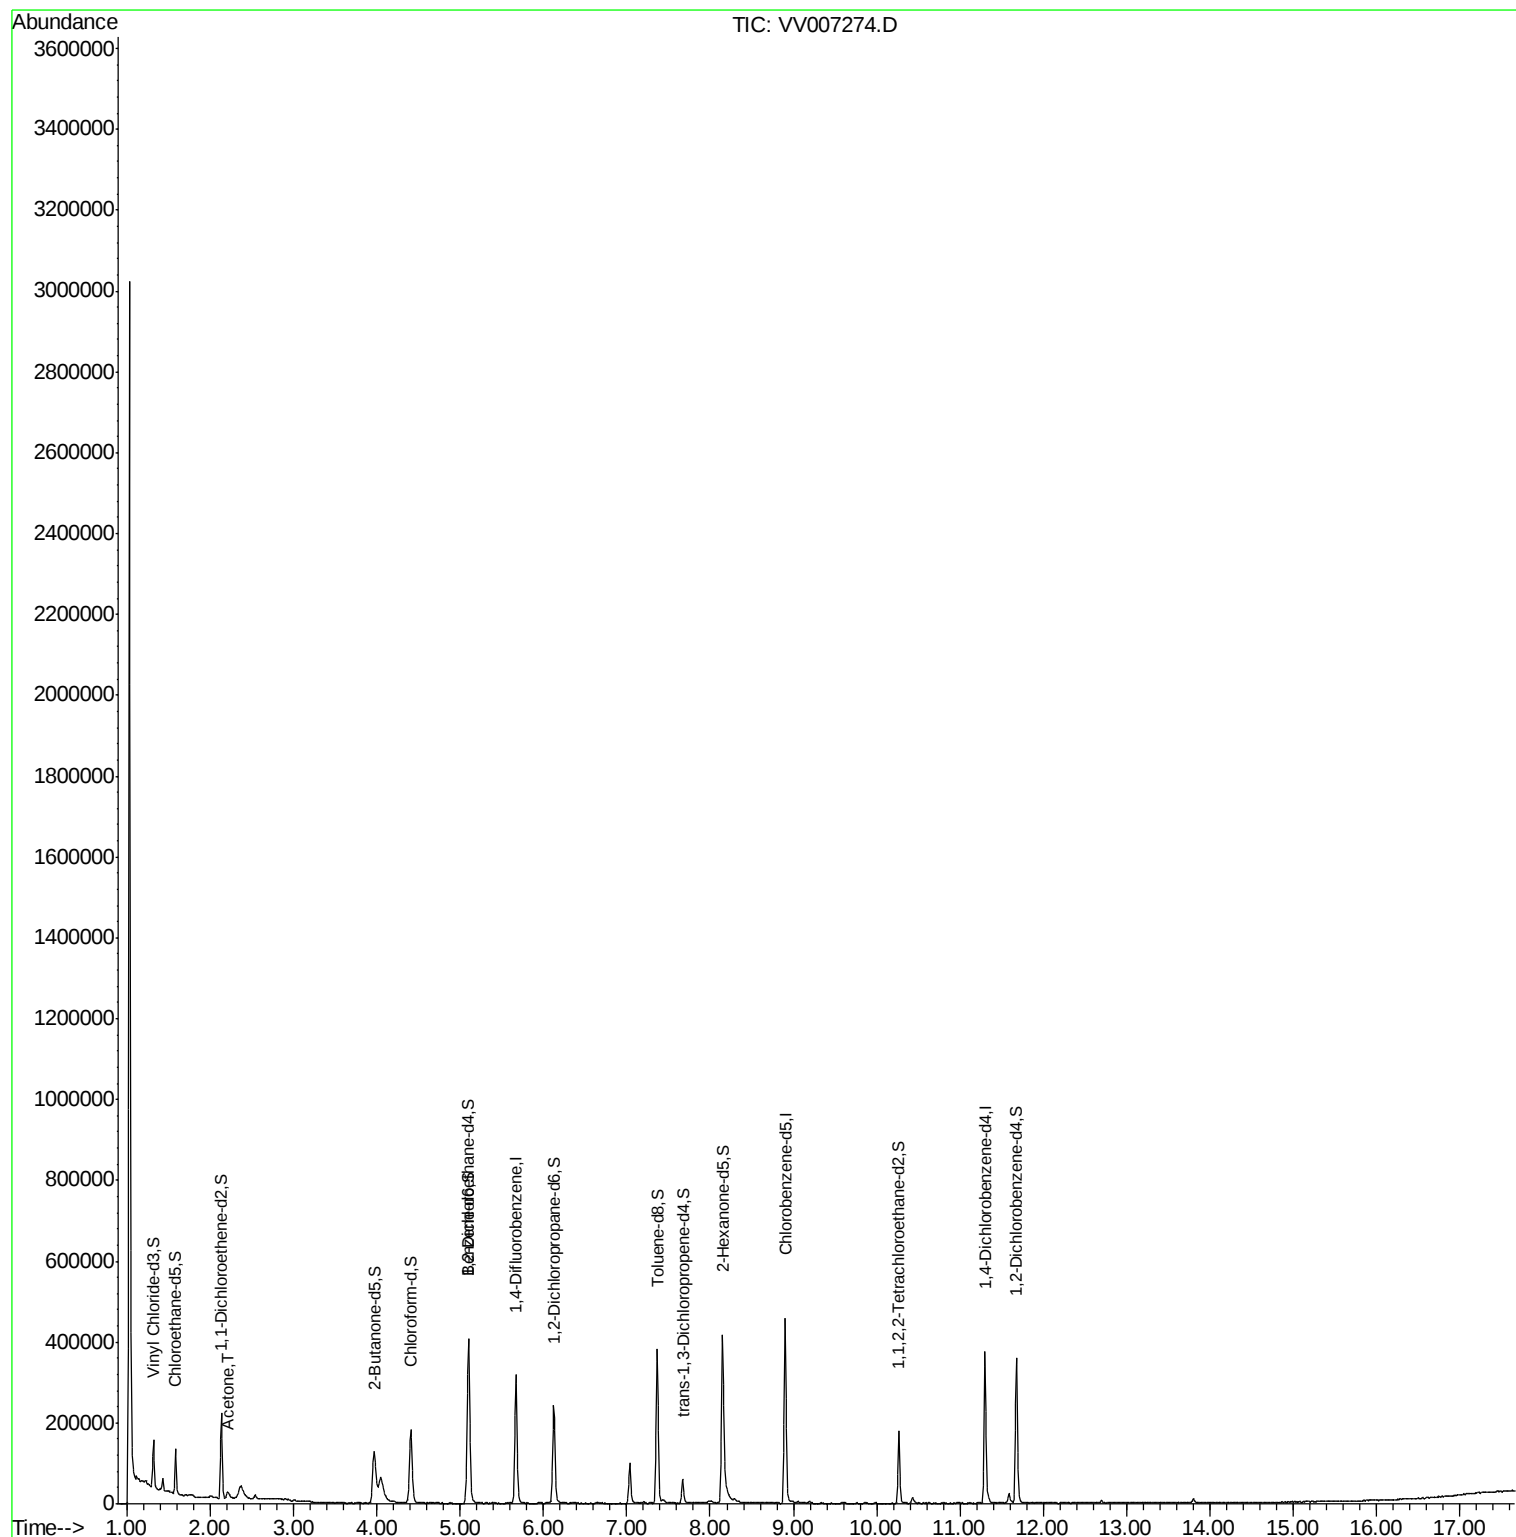

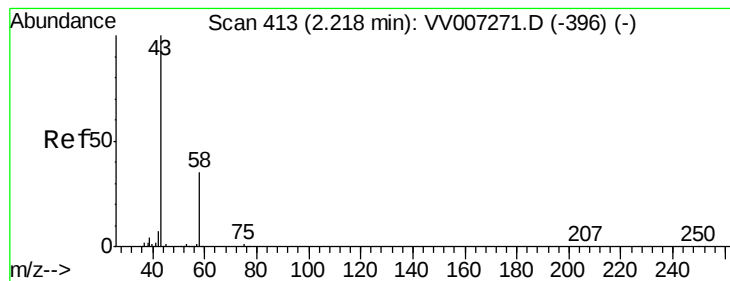

#13

Acetone

Concen: 6.99 ug/L

RT: 2.21 min Scan# 410

Delta R.T. -0.01 min

Lab File: VV007274.D

Acq: 30 Aug 2018 21:13

Instrument :
MSVOA_V
ClientSampleId :
DB3J8

Tot Ion: 43 Resp: 17963

Ion Ratio Lower Upper

43 100

58 39.7 0.0 71.8

