

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083018\
 Data File : VV007285.D
 Acq On : 31 Aug 2018 02:10
 Operator : SY/MD
 Sample : J4649-10
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GAB93

Quant Time: Aug 31 03:08:56 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR083018WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Aug 31 02:32:21 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	287077	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	293530	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	112420	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	119534	4.75	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.00%
7) Chloroethane-d5	1.58	69	98784	5.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.20%
11) 1,1-Dichloroethene-d2	2.13	63	155221	3.70	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.00%
20) 2-Butanone-d5	3.97	46	266225	54.33	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	108.66%
24) Chloroform-d	4.41	84	219950	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
26) 1,2-Dichloroethane-d4	5.09	65	108525	5.25	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.00%
32) Benzene-d6	5.10	84	437360	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.00%
36) 1,2-Dichloropropane-d6	6.12	67	140615	4.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.60%
41) Toluene-d8	7.37	98	336908	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.40%
43) trans-1,3-Dichloropropene-	7.67	79	43800	4.36	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.20%
46) 2-Hexanone-d5	8.14	63	146523	42.70	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.40%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	106688	5.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	116112	5.17	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	15004	5.56 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083018\
Data File : VV007285.D
Acq On : 31 Aug 2018 02:10
Operator : SY/MD
Sample : J4649-10
Misc : 25.0 mL/MSVOA V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GAB93

Quant Time: Aug 31 03:08:56 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR083018WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Aug 31 02:32:21 2018
Response via : Initial Calibration

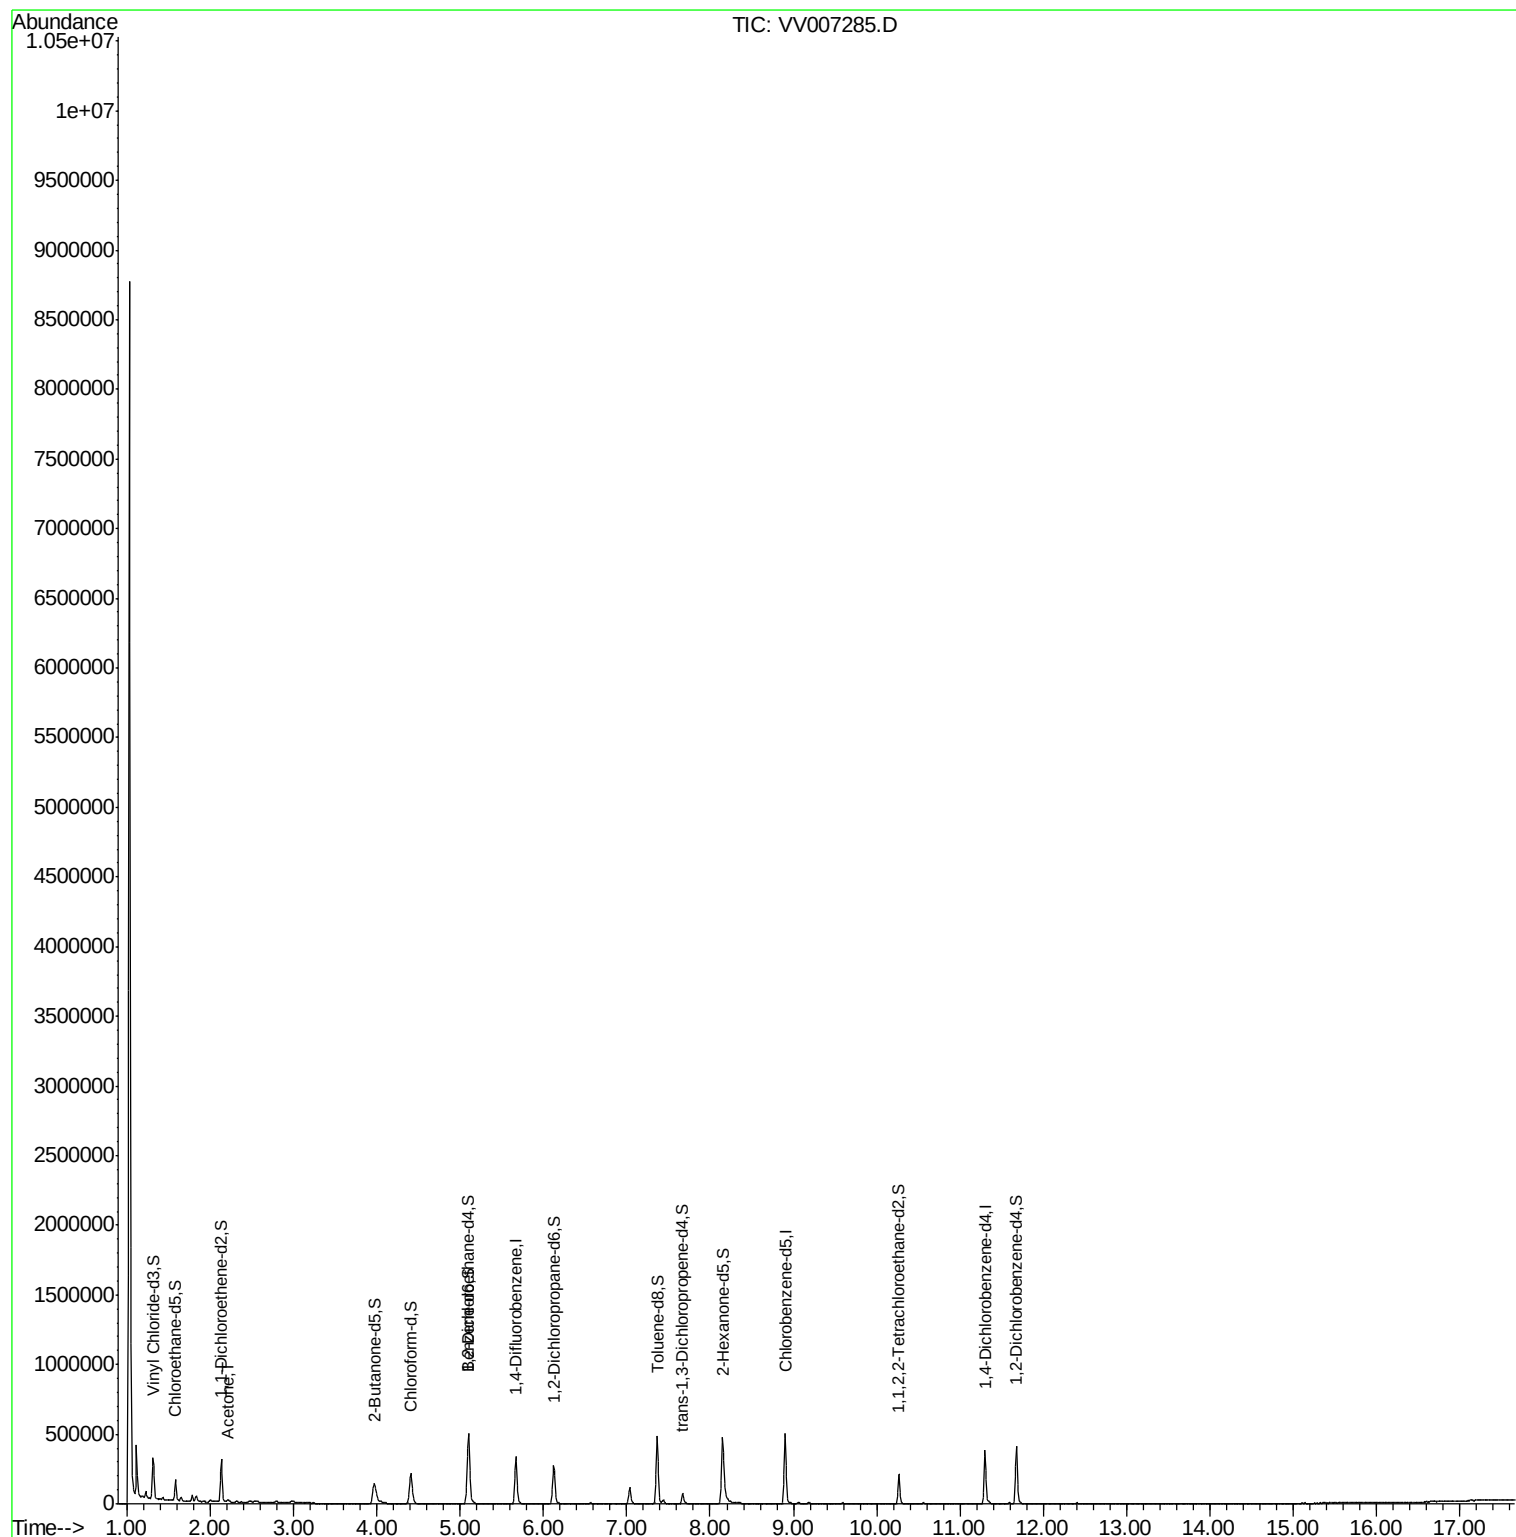

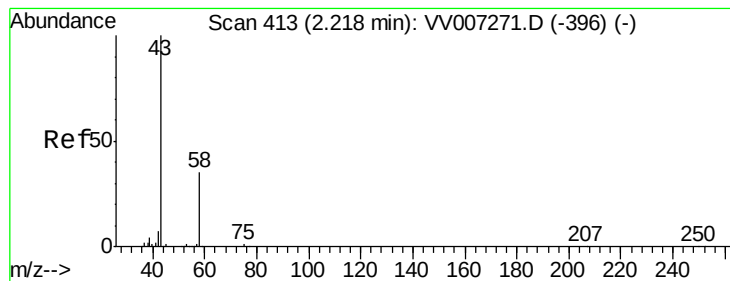

#13
 Acetone
 Concen: 5.56 ug/L
 RT: 2.21 min Scan# 411
 Delta R.T. -0.01 min
 Lab File: VV007285.D
 Acq: 31 Aug 2018 02:10

Instrument :
 MSVOA_V
 ClientSampleId :
 GAB93

Tot Ion: 43 Resp: 15004
 Ion Ratio Lower Upper
 43 100
 58 42.7 0.0 71.8

