


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV083018\
 Data File : VV007262.D
 Acq On : 30 Aug 2018 14:35
 Operator : SY/MD
 Sample : BFB69
 Misc : 25.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB69

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR083018WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Aug 31 02:32:21 2018

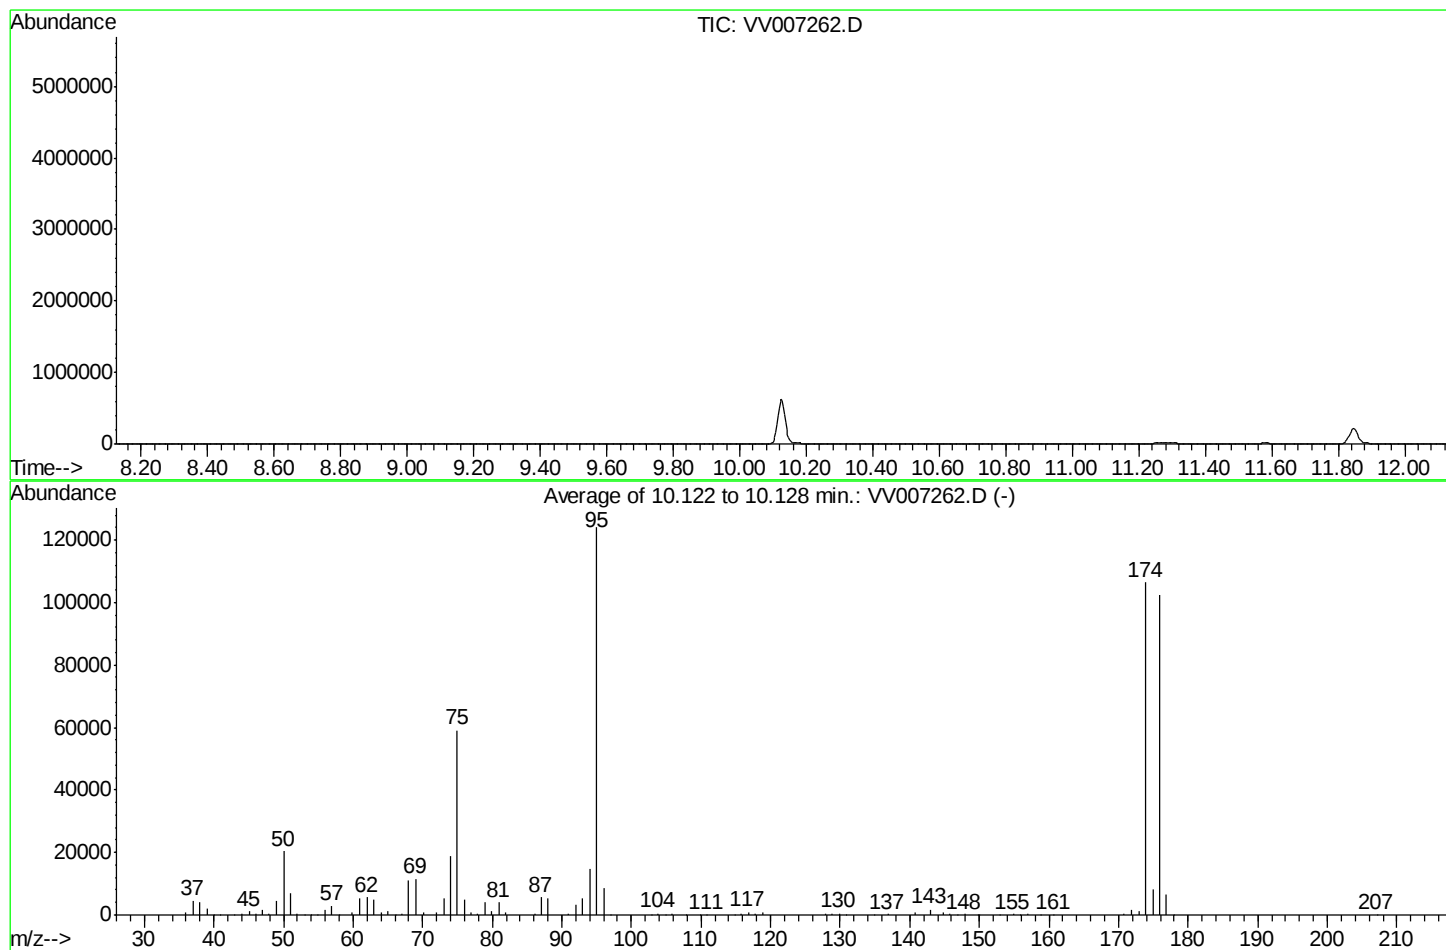

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2857

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	20429	PASS
75	95	30	80	47.6	59072	PASS
95	95	100	100	100.0	124050	PASS
96	95	5	9	6.9	8580	PASS
173	174	0.00	2	1.3	1355	PASS
174	95	50	120	85.7	106328	PASS
175	174	5	9	7.9	8399	PASS
176	174	95	101	96.5	102616	PASS
177	176	5	9	6.3	6422	PASS

Scan 2857 (10.077 min): VV007262.D
BFB69

m/z	Abundance
40.00	330.0
43.90	996.0
55.00	194.0
56.90	102.0
76.80	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.00	869.0
37.00	4636.0
38.00	4231.0
39.00	2189.0
40.00	337.0
40.90	180.0
43.00	123.0
44.00	1371.0
45.00	1075.0
46.00	255.0
47.00	1635.0
47.90	514.0
49.00	4544.0
50.00	20168.0
51.00	7000.0
52.00	303.0
53.00	162.0
54.90	432.0
56.00	1564.0
57.00	2986.0
58.00	194.0
59.90	942.0
61.00	5307.0
62.00	5538.0
63.00	4697.0
64.00	998.0
65.00	1367.0
66.20	162.0
67.00	356.0
68.00	10780.0
69.00	11139.0
70.10	797.0
72.00	768.0
73.00	5004.0
74.00	18624.0
75.00	59000.0
76.00	4790.0
77.00	1073.0
77.90	626.0
78.90	3875.0
79.90	1014.0
80.90	4002.0
81.90	817.0
86.10	302.0
87.00	5884.0
87.90	5385.0
90.90	352.0
92.00	3113.0
93.00	5279.0
94.00	14362.0
95.00	121944.0
96.00	8493.0
96.90	233.0
102.80	105.0
103.90	437.0
104.90	179.0
105.90	407.0
107.80	115.0
114.90	145.0
115.80	371.0
116.90	957.0
117.80	396.0
118.80	876.0
127.80	443.0
128.80	219.0
129.90	395.0
130.90	156.0
134.90	125.0
136.90	212.0
140.80	828.0
143.00	1753.0
144.90	755.0
145.80	182.0
146.90	120.0
147.90	330.0
149.80	183.0
154.90	377.0
155.80	101.0
157.00	346.0
160.70	125.0
170.80	328.0
171.90	1723.0
173.00	1225.0
173.90	101944.0
174.90	7918.0
175.90	97632.0
176.90	6289.0
177.90	134.0
207.10	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.00	903.0
37.00	4877.0
38.00	4472.0
39.00	2336.0
40.10	394.0
40.90	158.0
42.90	128.0
44.00	1356.0
45.10	1145.0
46.00	260.0
47.00	1711.0
47.90	504.0
49.00	4659.0
50.00	21000.0
51.00	7349.0
51.90	288.0
53.10	158.0
55.00	445.0
56.00	1642.0
57.00	3169.0
58.00	210.0
59.90	1002.0
61.00	5401.0
62.00	5839.0
63.00	5118.0
64.00	1017.0
65.00	1369.0
66.10	194.0
67.00	356.0
68.00	11274.0
69.00	12119.0
70.10	809.0
72.00	834.0
73.00	5342.0
74.00	19472.0
75.00	60808.0
76.00	4968.0
76.90	1026.0
77.90	615.0
78.90	4016.0
79.90	1100.0
80.90	4173.0
81.90	895.0
86.10	362.0
87.00	5917.0
87.90	5673.0
90.90	405.0
92.00	3311.0
93.00	5672.0
94.00	15217.0
95.00	128224.0
96.00	8845.0
96.90	227.0
103.80	511.0
104.90	170.0
105.90	436.0
107.80	127.0
109.80	101.0
110.80	119.0
114.90	178.0
115.80	411.0
116.80	973.0
117.80	470.0
118.80	758.0
127.80	401.0
128.90	223.0
129.90	440.0
130.80	197.0
134.90	185.0
136.90	234.0
140.80	859.0
142.90	1741.0
144.90	804.0
145.80	255.0
146.90	104.0
147.90	408.0
149.80	159.0
154.90	387.0
156.90	301.0
158.70	115.0
160.70	136.0
170.80	316.0
171.90	1904.0
173.00	1378.0
173.90	109696.0
174.90	8754.0
175.90	106168.0
176.90	6591.0
177.80	119.0
207.10	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.00	826.0
37.00	4620.0
38.00	4215.0
39.00	2219.0
40.00	415.0
40.90	168.0
42.80	126.0
44.00	1351.0
45.00	1044.0
46.00	264.0
47.00	1600.0
47.90	494.0
49.00	4281.0
50.00	20120.0
51.00	6654.0
51.90	259.0
53.10	187.0
54.00	104.0
55.00	345.0
55.90	1540.0
57.00	3053.0
57.90	221.0
59.90	976.0
61.00	5068.0
62.00	5505.0
63.00	4942.0
64.00	914.0
65.00	1228.0
66.10	161.0
67.00	354.0
68.00	10784.0
69.00	11469.0
70.00	774.0
71.90	799.0
73.00	5314.0
74.00	18664.0
75.00	57408.0
76.00	4656.0
76.90	912.0
77.90	479.0
78.90	3890.0
79.90	1040.0
80.90	3924.0
81.90	936.0
86.10	297.0
87.00	5298.0
87.90	5374.0
90.90	430.0
92.00	3178.0
93.00	5438.0
94.00	14589.0
95.00	121984.0
96.00	8404.0
96.90	190.0
103.80	494.0
104.90	161.0
105.90	470.0
107.80	127.0
109.80	118.0
110.80	115.0
114.90	202.0
115.80	388.0
116.80	943.0
117.80	502.0
118.80	592.0
127.80	326.0
128.90	258.0
129.90	444.0
130.80	229.0
134.90	221.0
136.90	245.0
140.90	916.0
142.90	1631.0
144.90	690.0
145.70	313.0
147.90	372.0
150.00	130.0
152.90	113.0
154.90	381.0
156.80	231.0
158.70	132.0
160.70	115.0
170.80	255.0
171.90	1903.0
173.00	1463.0
173.90	107344.0
174.90	8526.0
175.90	104048.0
176.90	6388.0
177.80	126.0
207.10	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69