

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV083019\
 Data File : VV012459.D
 Acq On : 30 Aug 2019 17:13
 Operator : SY/MD
 Sample : K4501-08DL 20X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GANM3DL

Quant Time: Aug 31 01:49:14 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082919WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Aug 31 01:38:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	213525	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	215220	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	79207	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	65201	3.42	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.40%
7) Chloroethane-d5	1.58	69	52634	3.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.40%
11) 1,1-Dichloroethene-d2	2.13	63	81326	2.60	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	52.00%#
20) 2-Butanone-d5	3.97	46	165091	42.56	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.12%
24) Chloroform-d	4.40	84	133009	4.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.40%
26) 1,2-Dichloroethane-d4	5.08	65	66953	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.20%
32) Benzene-d6	5.09	84	247926	3.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	77.20%
36) 1,2-Dichloropropane-d6	6.12	67	84298	4.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.60%
41) Toluene-d8	7.36	98	197957	3.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.40%#
43) trans-1,3-Dichloropropene-	7.66	79	27441	3.81	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.20%
46) 2-Hexanone-d5	8.14	63	115408	40.73	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.46%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	58739	4.06	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	70355	4.57	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.40%


Target Compounds					Qvalue
47) Tetrachloroethene	8.02	164	40223	2.213 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV083019\
Data File : VV012459.D
Acq On : 30 Aug 2019 17:13
Operator : SY/MD
Sample : K4501-08DL 20X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GANM3DL

Quant Time: Aug 31 01:49:14 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082919WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Aug 31 01:38:02 2019
Response via : Initial Calibration

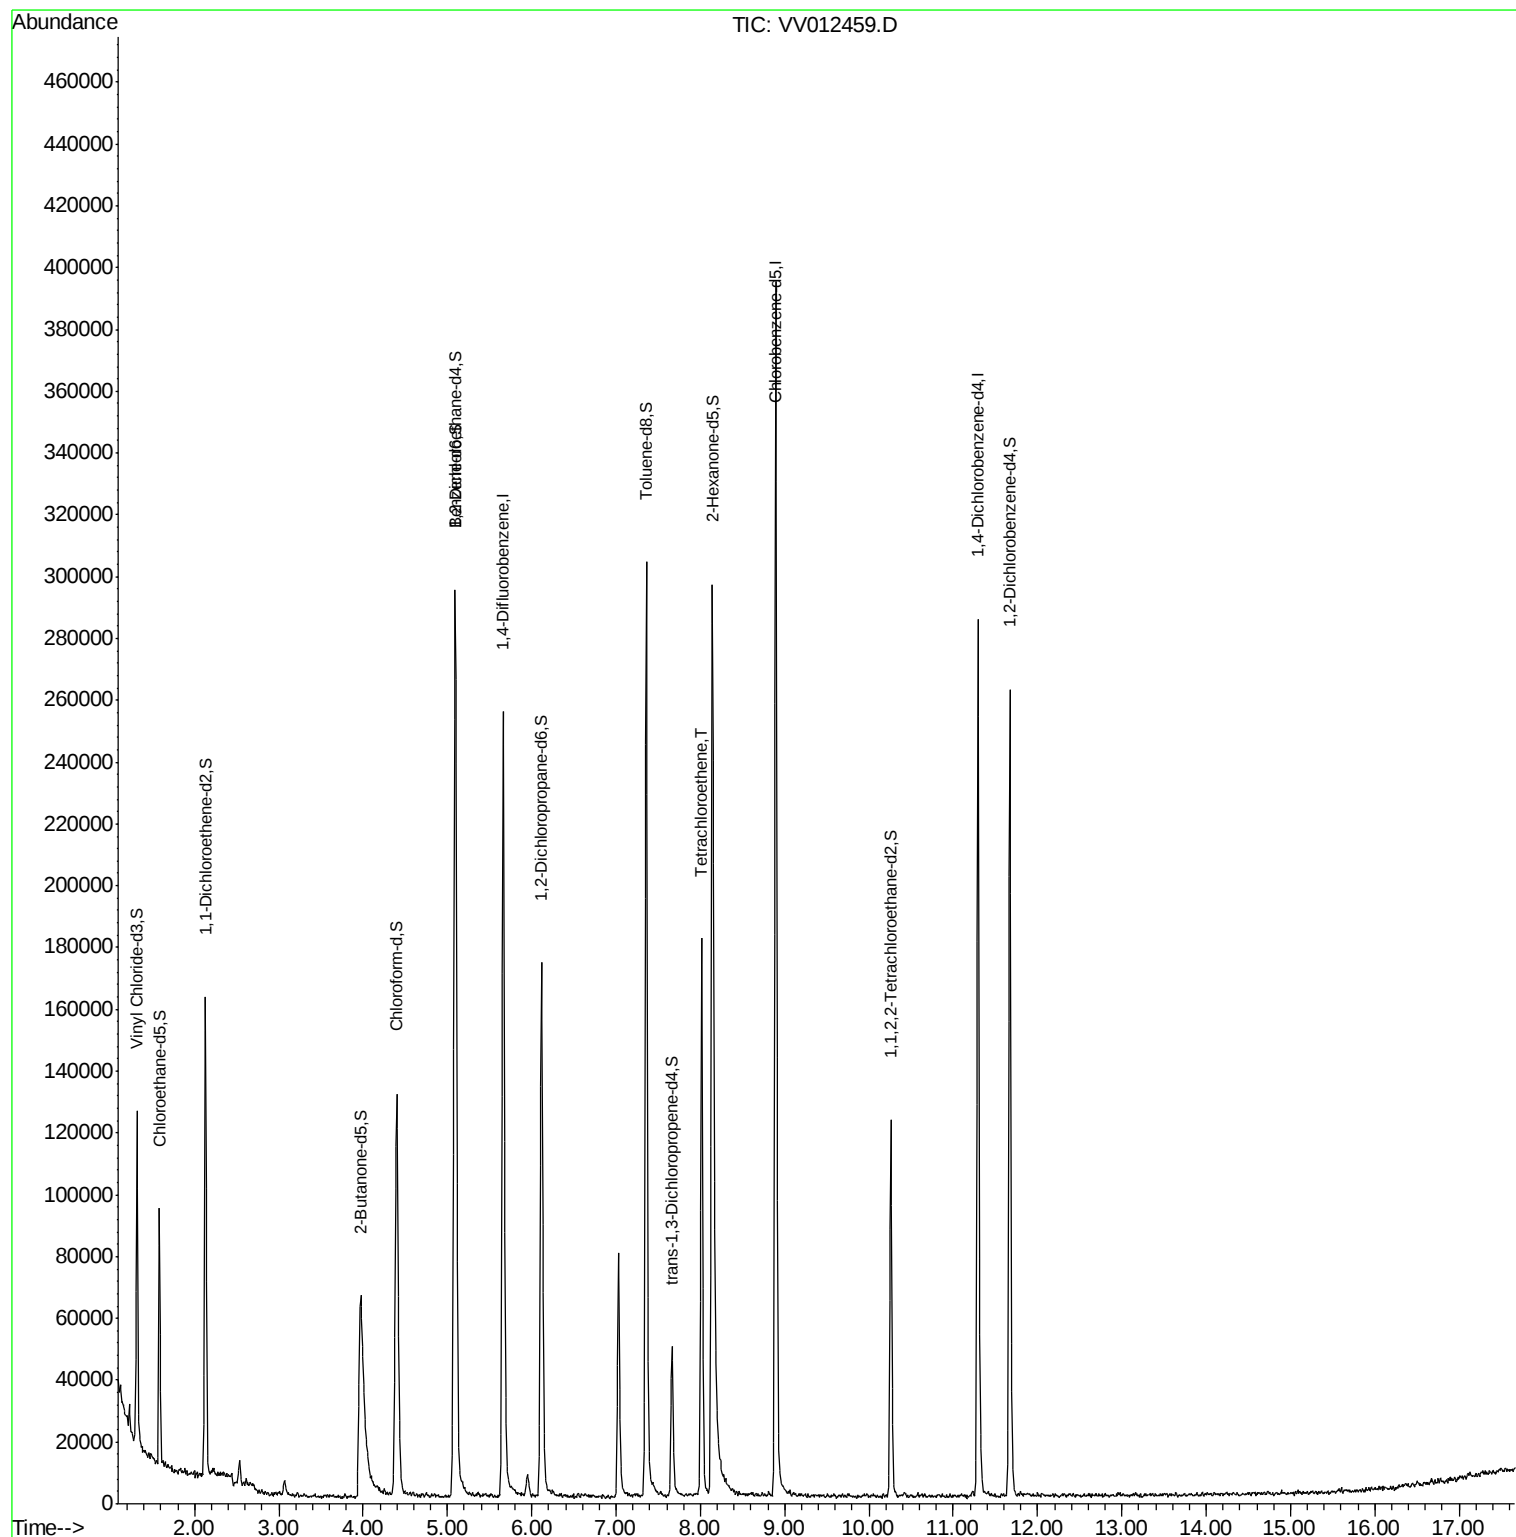

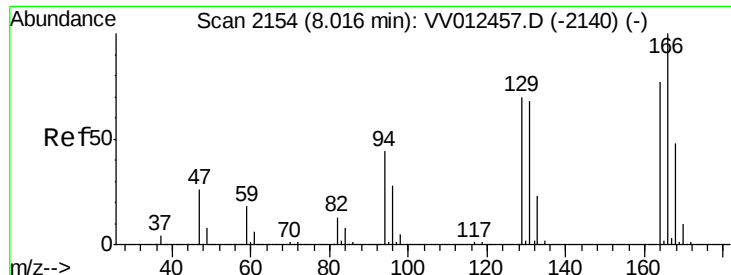

#47

Tetrachloroethene

Concen: 2.213 ug/L

RT: 8.02 min Scan# 2154

Delta R.T. 0.00 min

Lab File: VV012459.D


Acq: 30 Aug 2019 17:13

Instrument :

MSVOA_V

ClientSampleId :

GANM3DL

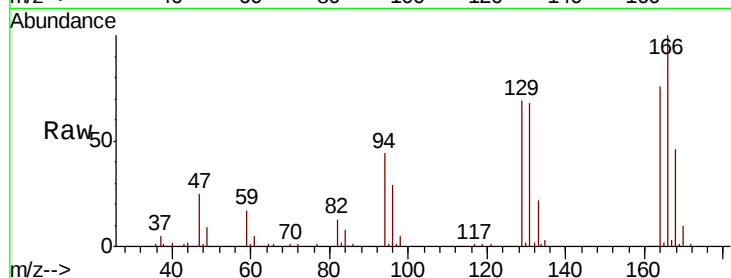

Tgt Ion:164 Resp: 40223


Ion Ratio Lower Upper

164 100

129 90.7 65.6 121.8

131 89.0 63.3 117.5

166 131.0 89.4 166.0

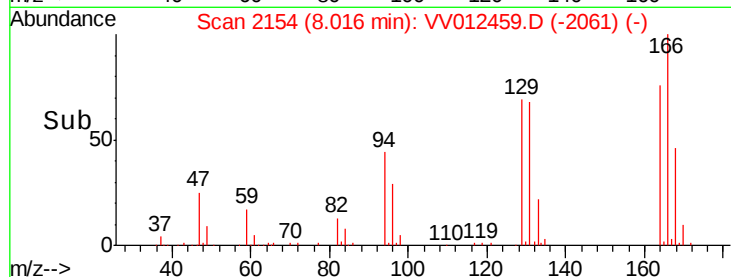

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

