


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV083019\
Data File : VV012444.D
Acq On : 30 Aug 2019 08:32
Operator : SY/MD
Sample : BFB57
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB57

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR082919WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Sep 03 03:10:43 2019

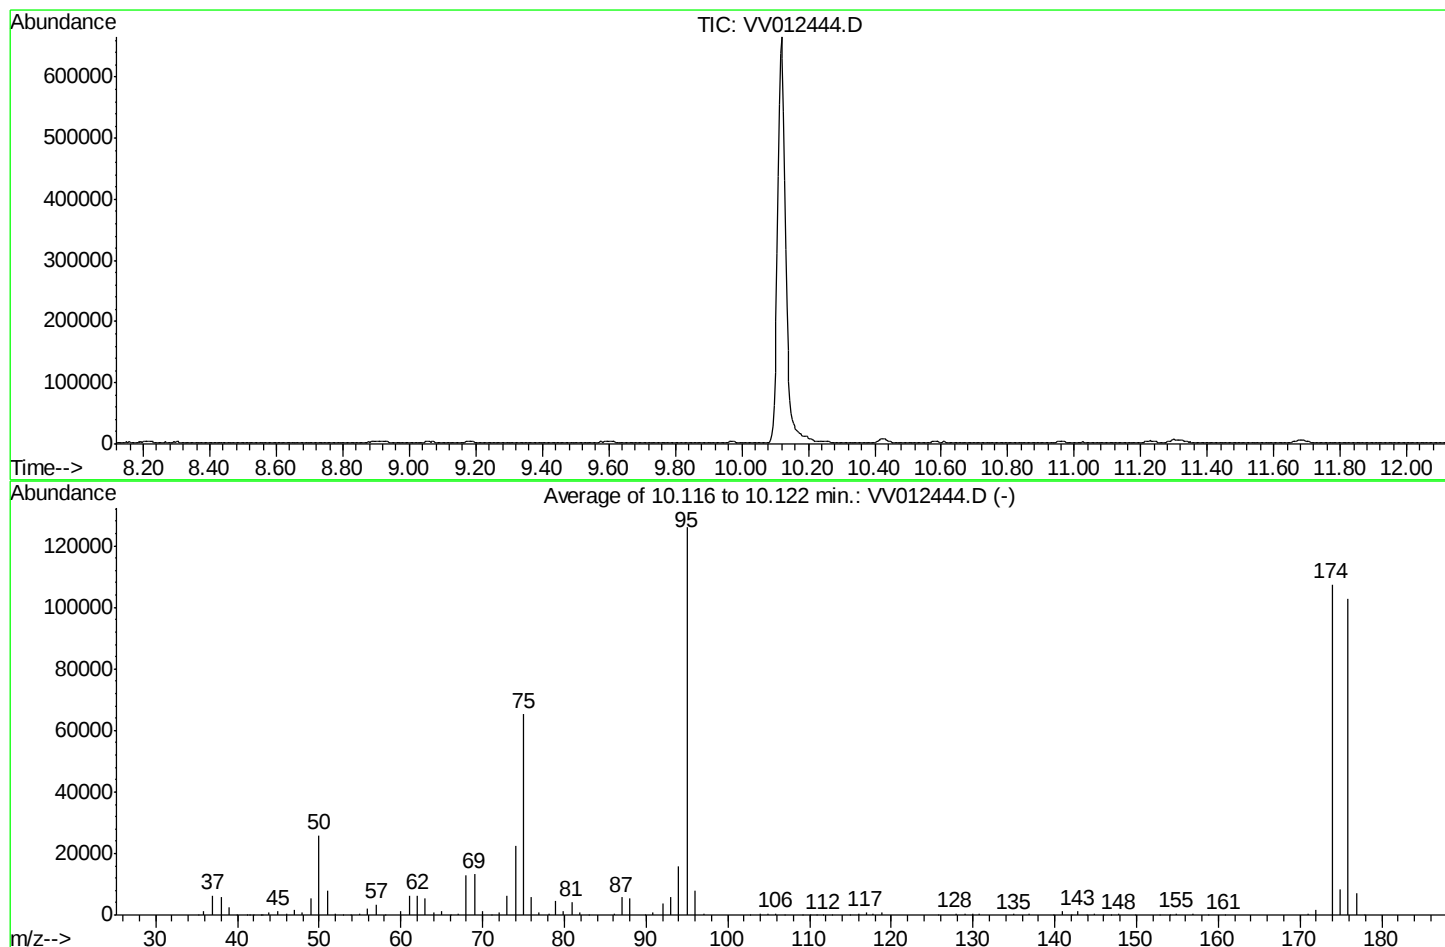

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	25997	PASS
75	95	30	80	51.8	65341	PASS
95	95	100	100	100.0	126026	PASS
96	95	5	9	6.4	8099	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.2	107429	PASS
175	174	5	9	7.8	8428	PASS
176	174	95	101	95.8	102880	PASS
177	176	5	9	6.8	7046	PASS

m/z	Abundance
38.50	139.0
39.90	695.0
41.00	142.0
43.90	705.0
54.10	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

m/z	Abundance
35.90	1154.0
37.00	6386.0
38.00	6320.0
39.00	2919.0
40.00	904.0
41.20	143.0
42.80	146.0
43.90	1430.0
45.00	1272.0
46.00	312.0
46.90	1692.0
47.90	766.0
49.00	4982.0
50.00	26232.0
51.00	7917.0
51.90	532.0
52.90	198.0
53.80	151.0
54.90	481.0
56.00	1889.0
57.00	3527.0
58.10	190.0
60.00	1220.0
61.00	6219.0
62.00	6563.0
63.00	5337.0
64.00	757.0
65.00	1381.0
66.10	213.0
67.00	446.0
68.00	13262.0
69.00	13525.0
70.00	1113.0
71.00	124.0
71.90	716.0
73.00	6324.0
74.00	22264.0
75.00	64928.0
76.00	5745.0
76.90	713.0
78.00	638.0
78.90	4827.0
79.90	1258.0
80.90	4366.0
81.90	950.0
83.00	112.0
86.10	291.0
87.00	6133.0
88.00	5601.0
89.90	152.0
90.80	660.0
92.00	3674.0
93.00	5686.0
94.00	15513.0
95.00	125752.0
96.00	8414.0
97.10	277.0
102.70	108.0
103.90	504.0
104.90	275.0
105.90	584.0
107.00	175.0
109.10	119.0
111.00	114.0
111.60	174.0
112.80	149.0
114.90	173.0
115.90	642.0
116.90	862.0
117.80	498.0
118.90	845.0
125.80	115.0
127.90	534.0
128.90	281.0
129.90	456.0
130.80	318.0
135.00	308.0
136.90	213.0
139.90	145.0
140.90	1286.0
142.80	1502.0
143.90	169.0
144.90	468.0
145.90	185.0
146.80	131.0
147.80	284.0
152.80	141.0
154.90	448.0
156.90	256.0
158.80	189.0
160.80	186.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

170.90	330.0
171.90	1486.0
173.90	104072.0
174.90	8361.0
175.90	99376.0
176.90	6992.0
177.90	226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

m/z	Abundance
35.90	1197.0
37.00	6423.0
38.00	6144.0
39.00	2767.0
40.00	902.0
40.80	127.0
41.50	113.0
42.00	109.0
42.90	137.0
43.90	1401.0
45.00	1348.0
46.10	345.0
46.90	1731.0
48.00	806.0
49.00	5435.0
50.00	26976.0
51.00	8186.0
51.90	493.0
52.90	225.0
54.90	519.0
56.00	2008.0
57.00	3450.0
58.10	172.0
60.00	1313.0
61.00	6315.0
62.00	6460.0
63.00	5616.0
64.00	779.0
65.00	1430.0
66.00	208.0
66.90	454.0
68.00	13347.0
69.00	13876.0
70.00	1172.0
71.00	120.0
72.00	727.0
73.00	6516.0
74.00	23056.0
75.00	67528.0
76.00	5935.0
76.90	856.0
78.00	596.0
78.90	4900.0
79.90	1320.0
80.90	4520.0
81.90	972.0
82.90	157.0
86.10	253.0
87.00	6016.0
88.00	5478.0
89.90	119.0
90.90	701.0
92.00	3937.0
93.00	5885.0
94.00	16286.0
95.00	130064.0
96.00	8370.0
97.00	249.0
103.90	494.0
104.90	280.0
105.90	537.0
106.90	195.0
109.10	125.0
110.90	107.0
111.70	197.0
112.80	105.0
114.90	210.0
116.00	643.0
116.90	1061.0
117.80	500.0
118.90	863.0
125.80	100.0
127.80	488.0
128.90	330.0
129.90	500.0
130.80	276.0
135.00	318.0
136.90	233.0
139.80	151.0
140.90	1383.0
142.10	200.0
142.90	1479.0
143.80	166.0
144.90	484.0
145.90	200.0
146.80	128.0
147.90	281.0
149.80	103.0
152.80	130.0
154.00	150.0
154.90	487.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

156.90	288.0
158.80	175.0
160.70	213.0
170.90	314.0
171.90	1625.0
173.90	111208.0
174.90	8695.0
175.90	106208.0
176.90	7279.0
177.90	220.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

m/z	Abundance
35.20	129.0
35.90	1153.0
37.00	5985.0
38.00	5392.0
39.00	2386.0
40.00	936.0
40.80	135.0
41.60	145.0
43.10	173.0
43.90	1303.0
45.00	1273.0
46.00	325.0
47.00	1621.0
48.00	821.0
49.00	5343.0
50.00	24784.0
51.00	7639.0
51.90	448.0
52.80	236.0
54.90	502.0
55.90	1925.0
57.00	3240.0
58.00	170.0
60.00	1226.0
61.00	5849.0
62.00	5887.0
63.00	5283.0
64.00	832.0
65.00	1300.0
65.90	212.0
66.90	400.0
68.00	12156.0
69.00	12958.0
70.00	1107.0
71.00	111.0
72.10	700.0
73.00	6149.0
74.00	21680.0
75.00	63568.0
76.00	5524.0
76.90	895.0
78.10	541.0
78.90	4453.0
79.90	1283.0
80.90	4251.0
81.90	951.0
83.00	203.0
86.10	196.0
87.00	5322.0
88.00	5061.0
90.90	630.0
92.00	3774.0
93.00	5589.0
94.00	15311.0
95.00	122264.0
96.00	7514.0
96.90	206.0
103.90	450.0
105.00	274.0
105.90	458.0
106.90	179.0
110.00	106.0
110.80	108.0
111.70	177.0
114.90	214.0
115.90	569.0
116.90	1086.0
117.80	464.0
118.90	788.0
125.80	121.0
127.80	464.0
129.00	327.0
129.90	496.0
130.80	172.0
135.00	255.0
136.90	252.0
139.80	159.0
140.90	1410.0
142.00	190.0
142.90	1341.0
143.80	135.0
144.90	452.0
145.90	268.0
146.80	105.0
147.90	267.0
149.80	141.0
152.90	104.0
154.00	165.0
154.90	452.0
156.90	311.0
158.80	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57

160.70	210.0
171.00	220.0
171.90	1592.0
173.90	107008.0
174.90	8229.0
175.90	103056.0
176.90	6869.0
177.90	210.0

Instrument :
MSVOA_V
ClientSampleId :
BFB57