

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022012.D
 Acq On : 30 Aug 2021 18:40
 Operator : SY/MD
 Sample : M3566-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKH2

Quant Time: Aug 31 02:40:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 31 02:34:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	368066	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	348903	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	178189	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	95483	37.460	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	74.920%		
7) Chloroethane-d5	1.565	69	85776	43.093	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.180%		
11) 1,1-Dichloroethene-d2	2.105	63	132783	31.499	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	63.000%		
21) 2-Butanone-d5	3.876	46	158162	90.477	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	90.480%		
24) Chloroform-d	4.349	84	194871	41.929	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	83.860%		
26) 1,2-Dichloroethane-d4	5.034	65	130180	47.553	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.100%		
32) Benzene-d6	5.050	84	441820	46.687	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.380%		
36) 1,2-Dichloropropane-d6	6.072	67	140532	47.220	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	94.440%		
41) Toluene-d8	7.317	98	403733	45.194	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.380%		
43) trans-1,3-Dichloroprop...	7.625	79	59323	41.880	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.760%		
47) 2-Hexanone-d5	8.088	63	109559	95.942	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	95.940%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	188573	49.474	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.940%		
66) 1,2-Dichlorobenzene-d4	11.625	152	164279	46.897	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.800%		
Target Compounds					Qvalue	
25) Chloroform	4.378	83	16891	3.490	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022012.D
Acq On : 30 Aug 2021 18:40
Operator : SY/MD
Sample : M3566-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKH2

Quant Time: Aug 31 02:40:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 31 02:34:28 2021
Response via : Initial Calibration

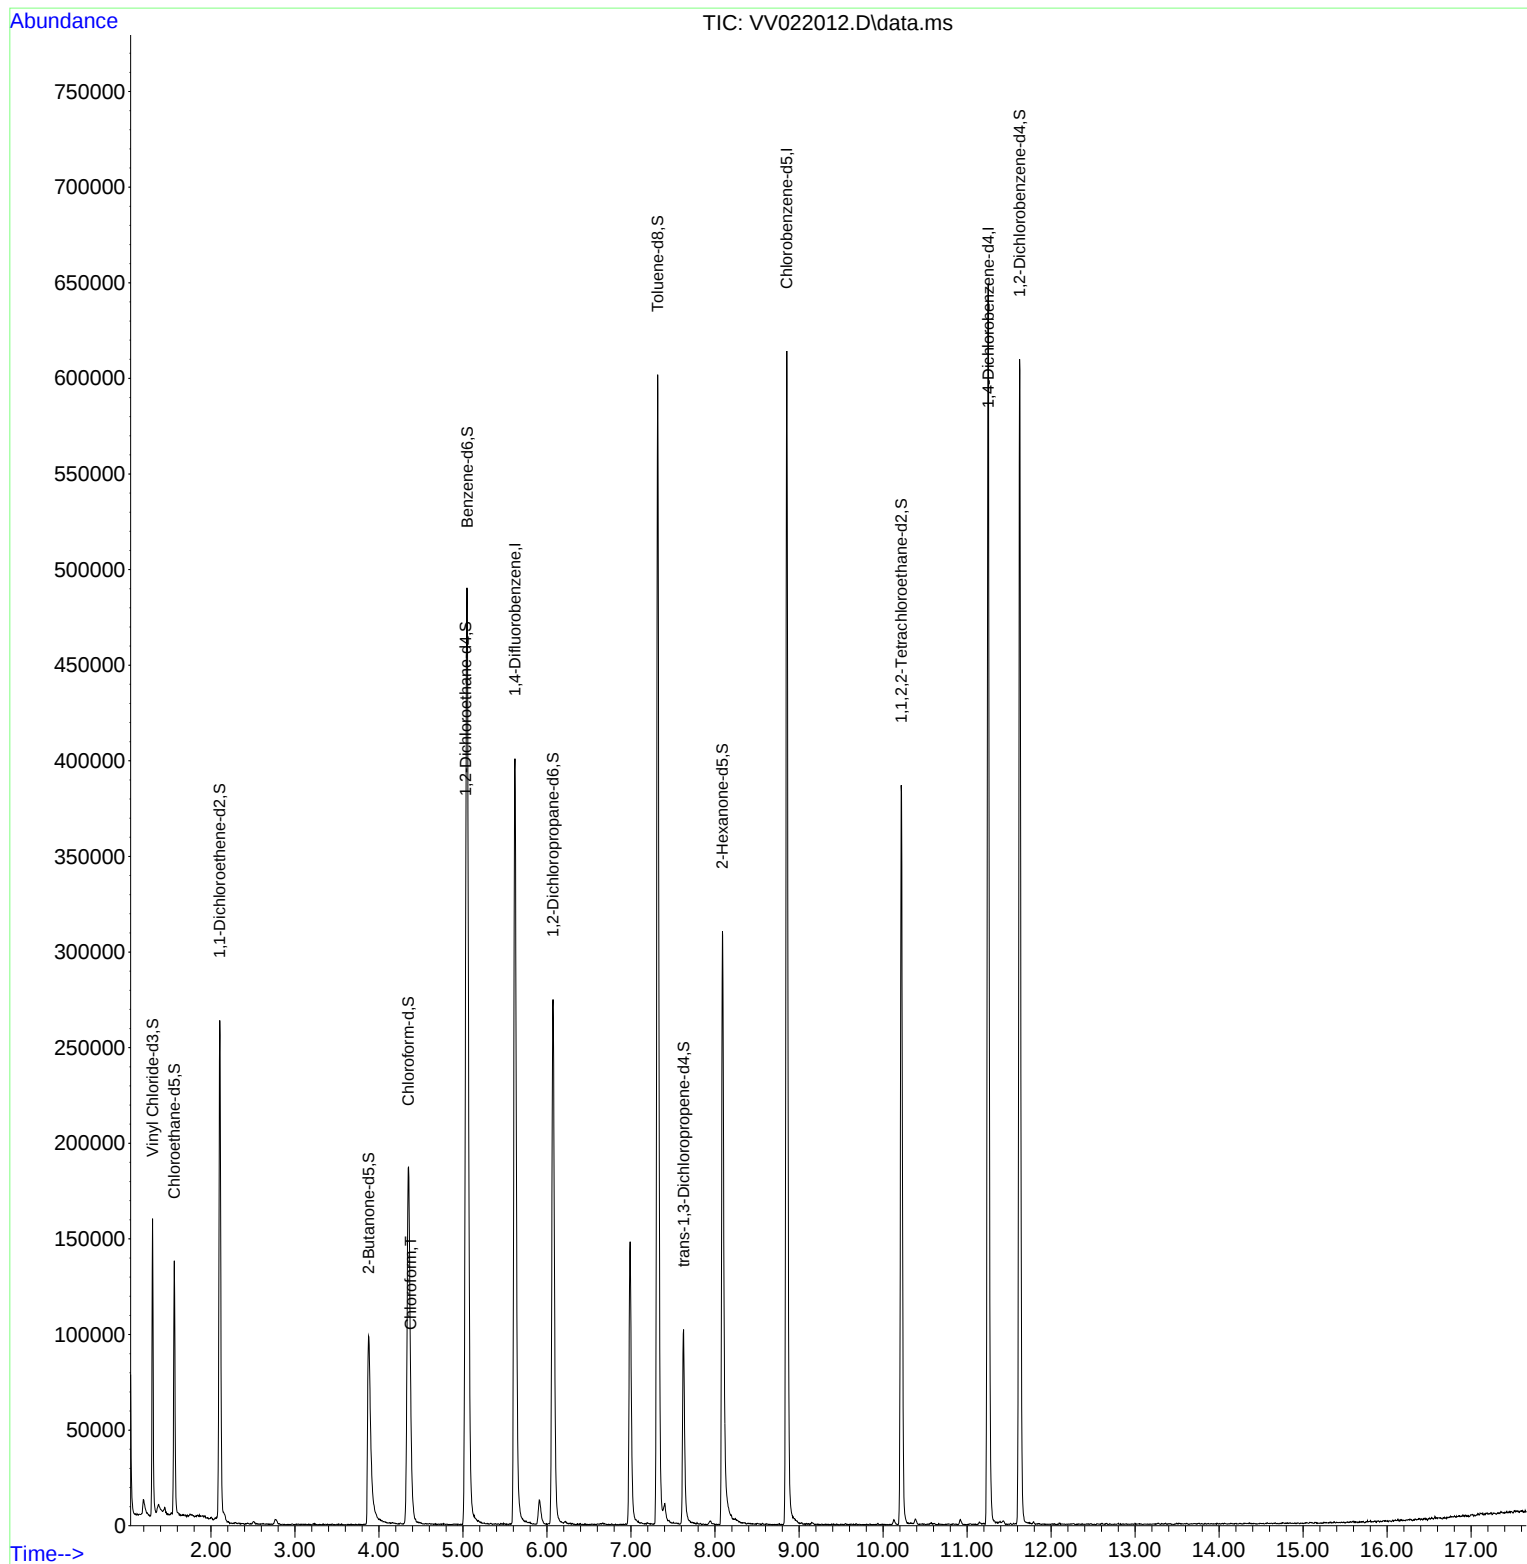

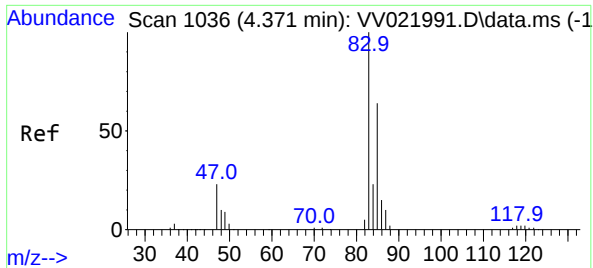

#25
Chloroform
Concen: 3.490 ug/L
RT: 4.378 min Scan# 1038
Delta R.T. 0.007 min
Lab File: VV022012.D
Acq: 30 Aug 2021 18:40

Instrument :
MSVOA_V
ClientSampleId :
DBKH2

Tgt Ion: 83 Resp: 16891
Ion Ratio Lower Upper
83 100
85 73.6 46.3 85.9

