

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW083021\
 Data File : VW022017.D
 Acq On : 30 Aug 2021 21:05
 Operator : SY/MD
 Sample : M3566-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKH8

Quant Time: Aug 31 04:30:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Aug 31 04:25:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	360789	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	350805	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	172338	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	93717	37.509	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	75.020%
7) Chloroethane-d5	1.565	69	83624	42.859	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.720%
11) 1,1-Dichloroethene-d2	2.105	63	133008	32.189	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	64.380%
21) 2-Butanone-d5	3.876	46	170587	99.554	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.550%
24) Chloroform-d	4.349	84	193796	42.538	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.080%
26) 1,2-Dichloroethane-d4	5.034	65	125206	46.659	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.320%
32) Benzene-d6	5.050	84	425630	44.732	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.460%
36) 1,2-Dichloropropane-d6	6.072	67	136163	45.504	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.000%
41) Toluene-d8	7.317	98	391481	43.585	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.180%
43) trans-1,3-Dichloroprop...	7.625	79	56547	39.703	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.400%
47) 2-Hexanone-d5	8.088	63	102285	89.086	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.090%
56) 1,1,2,2-Tetrachloroeth...	10.220	84	175951	45.912	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.820%
66) 1,2-Dichlorobenzene-d4	11.628	152	162322	47.911	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.820%
Target Compounds						
					Qvalue	
13) Acetone	2.159	43	5476	3.814	ug/L	# 76
25) Chloroform	4.375	83	11892	2.507	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022017.D
Acq On : 30 Aug 2021 21:05
Operator : SY/MD
Sample : M3566-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKH8

Quant Time: Aug 31 04:30:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Aug 31 04:25:57 2021
Response via : Initial Calibration




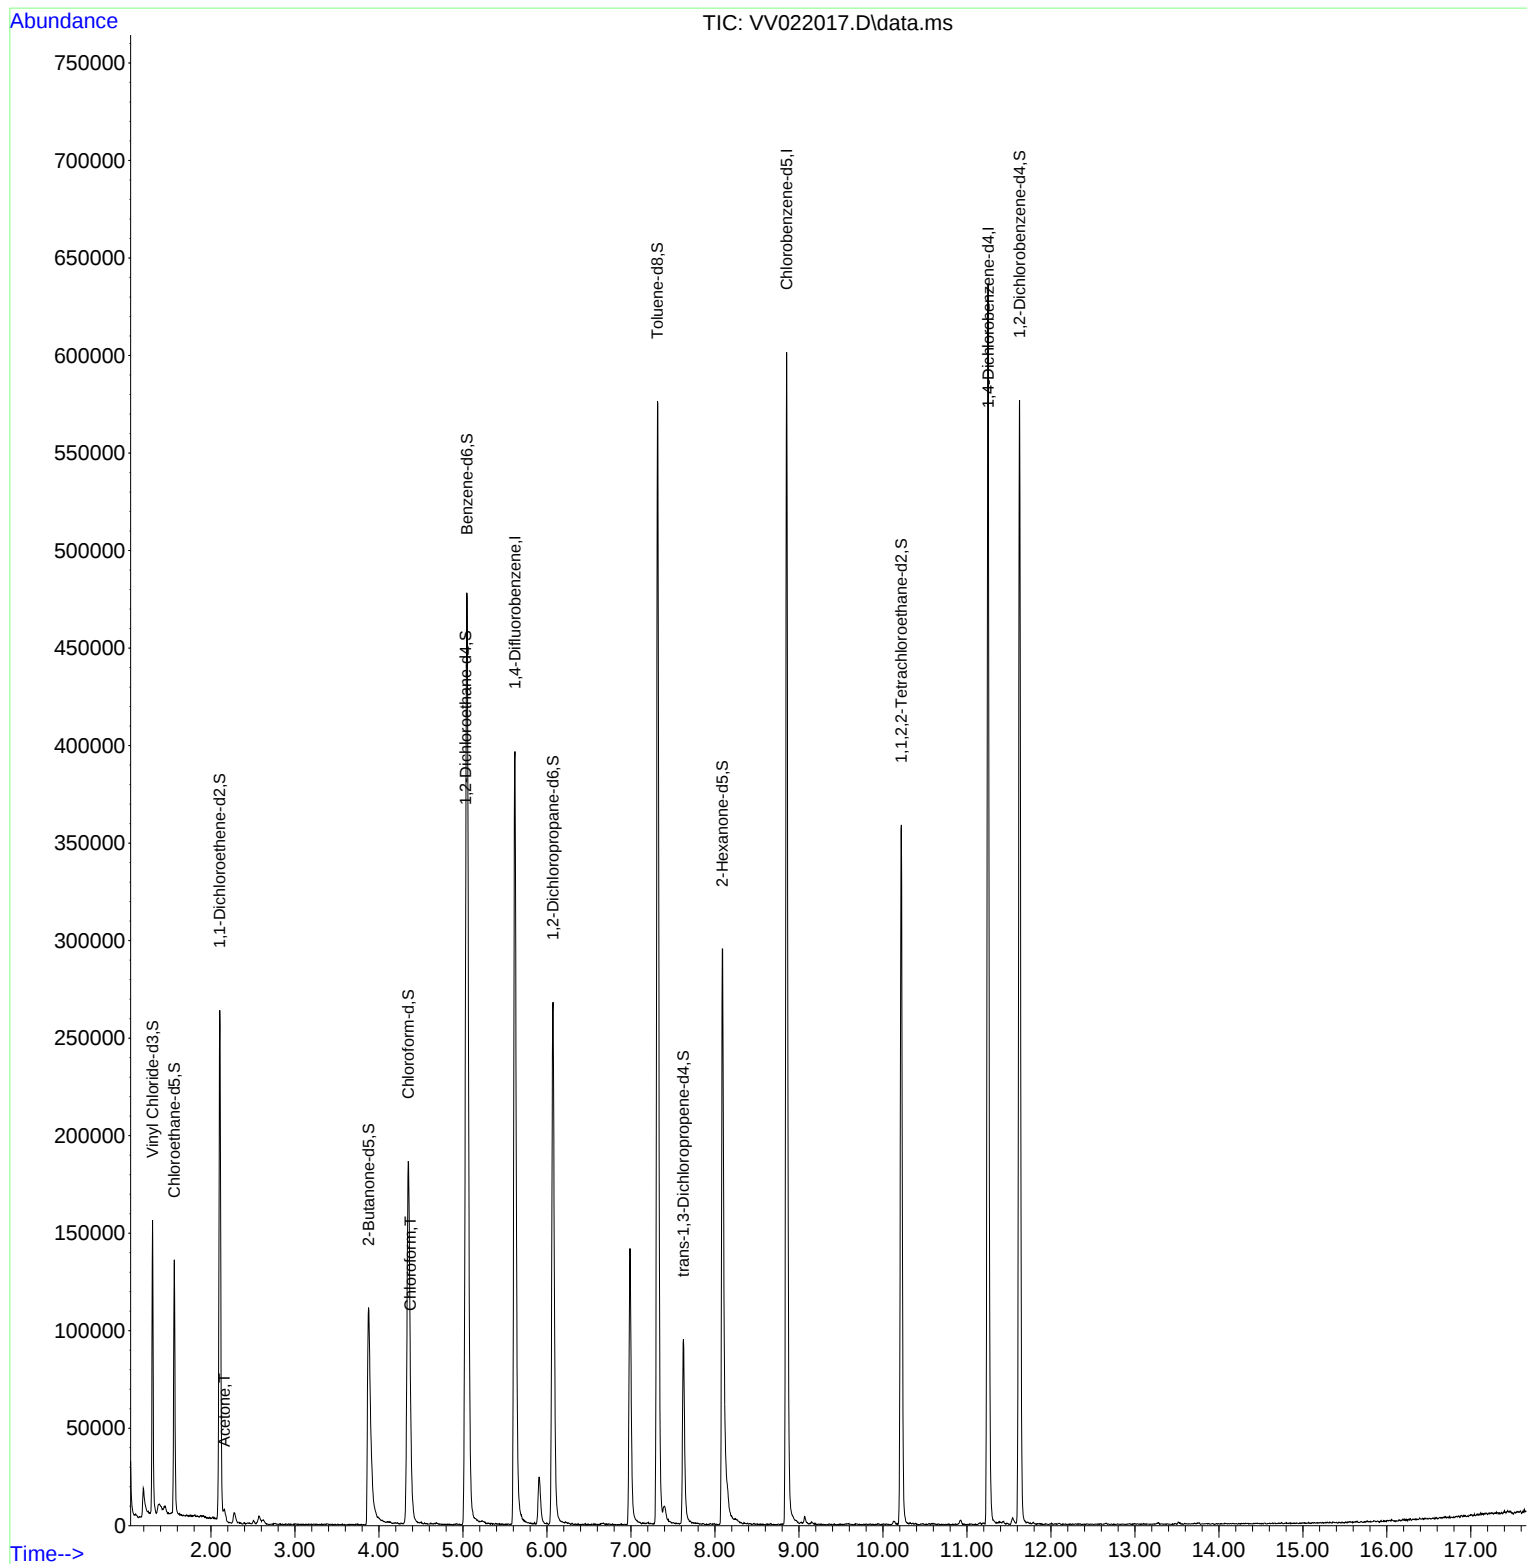


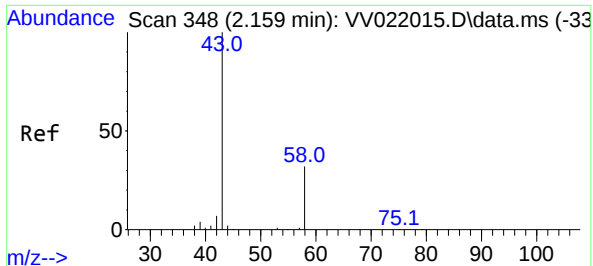

#13
Acetone
Concen: 3.814 ug/L
RT: 2.159 min Scan# 348
Delta R.T. -0.000 min
Lab File: VV022017.D
Acq: 30 Aug 2021 21:05

Instrument :
MSVOA_V
ClientSampleId :
DBKH8

Tgt Ion: 43 Resp: 5476
Ion Ratio Lower Upper
43 100
58 30.6 0.0 0.4#

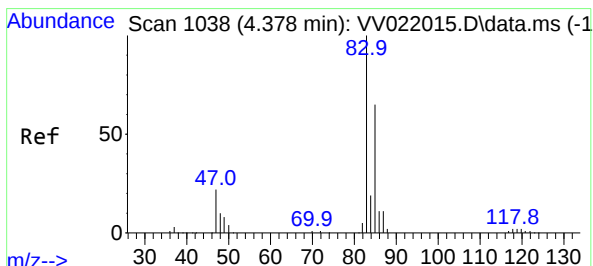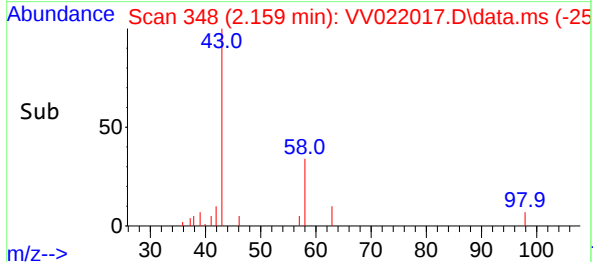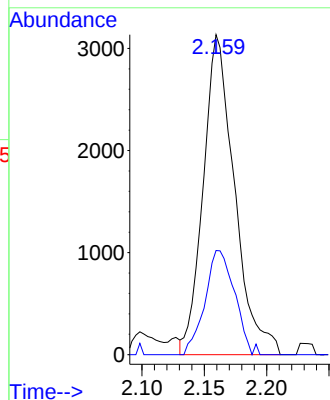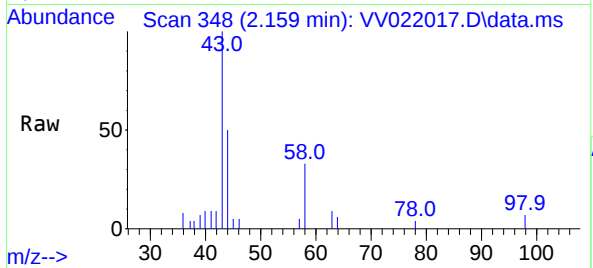

#25
Chloroform
Concen: 2.507 ug/L
RT: 4.375 min Scan# 1037
Delta R.T. -0.003 min
Lab File: VV022017.D
Acq: 30 Aug 2021 21:05

Tgt Ion: 83 Resp: 11892
Ion Ratio Lower Upper
83 100
85 62.2 46.3 85.9

