

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022005.D
 Acq On : 30 Aug 2021 15:26
 Operator : SY/MD
 Sample : M3573-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022005.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	89	rBV	171358	167725	13.04%	1.681%
2	1.565	157	163	183	rVB	138183	161731	12.58%	1.621%
3	2.105	323	331	355	rVB	287074	429080	33.37%	4.300%
4	2.565	472	474	478	rBV	280	188	0.01%	0.002%
5	2.606	485	487	490	rBV	540	316	0.02%	0.003%
6	2.690	510	513	514	rBV	455	274	0.02%	0.003%
7	2.741	523	529	533	rBV3	633	763	0.06%	0.008%
8	2.767	535	537	540	rVB2	582	252	0.02%	0.003%
9	2.786	541	543	546	rVB4	538	212	0.02%	0.002%
10	2.873	567	570	572	rBV2	463	243	0.02%	0.002%
11	2.915	580	583	586	rVB2	329	205	0.02%	0.002%
12	2.950	592	594	596	rBV2	408	204	0.02%	0.002%
13	3.108	639	643	645	rBV2	282	211	0.02%	0.002%
14	3.169	659	662	666	rVB2	479	290	0.02%	0.003%
15	3.230	678	681	684	rVV2	389	211	0.02%	0.002%
16	3.310	699	706	708	rBV2	566	569	0.04%	0.006%
17	3.333	711	713	718	rVB2	393	214	0.02%	0.002%
18	3.436	742	745	754	rVB3	305	391	0.03%	0.004%
19	3.481	755	759	763	rBV2	374	258	0.02%	0.003%
20	3.577	785	789	792	rBV3	453	365	0.03%	0.004%
21	3.629	803	805	807	rBV	449	207	0.02%	0.002%
22	3.674	817	819	821	rBV	326	173	0.01%	0.002%
23	3.876	872	882	917	rBV	106330	284576	22.13%	2.852%
24	4.352	1013	1030	1062	rBV	191874	502265	39.06%	5.033%
25	4.690	1133	1135	1139	rBV	572	390	0.03%	0.004%
26	4.841	1178	1182	1188	rVB5	410	410	0.03%	0.004%
27	4.876	1188	1193	1195	rBV4	469	423	0.03%	0.004%
28	4.912	1201	1204	1210	rVB4	514	450	0.03%	0.005%
29	5.047	1229	1246	1280	rBV2	502379	1285756	100.00%	12.884%
30	5.471	1374	1378	1384	rBV4	385	334	0.03%	0.003%
31	5.510	1388	1390	1393	rVV2	447	195	0.02%	0.002%
32	5.523	1393	1394	1398	rVV2	402	208	0.02%	0.002%
33	5.619	1412	1424	1457	rBV	391068	797661	62.04%	7.993%
34	5.912	1504	1515	1528	rBV4	10917	21975	1.71%	0.220%
35	5.995	1538	1541	1544	rVB2	423	240	0.02%	0.002%
36	6.072	1551	1565	1591	rBV	282322	575786	44.78%	5.770%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022005.D
 Acq On : 30 Aug 2021 15:26
 Operator : SY/MD
 Sample : M3573-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.310	1635	1639	1640	rBV2	474	255	0.02%	0.003%
38	6.343	1647	1649	1651	rBV3	350	181	0.01%	0.002%
39	6.613	1728	1733	1735	rBV2	340	312	0.02%	0.003%
40	6.622	1735	1736	1739	rBV2	308	209	0.02%	0.002%
41	6.722	1764	1767	1770	rVB2	349	217	0.02%	0.002%
42	6.789	1784	1788	1790	rBV	338	275	0.02%	0.003%
43	6.838	1798	1803	1804	rBV	251	193	0.02%	0.002%
44	6.941	1832	1835	1839	rBV3	415	350	0.03%	0.004%
45	6.989	1839	1850	1870	rBV	150887	279876	21.77%	2.804%
46	7.198	1912	1915	1916	rBV	475	273	0.02%	0.003%
47	7.317	1941	1952	1970	rBV	615018	1072735	83.43%	10.749%
48	7.548	2022	2024	2029	rBV3	494	348	0.03%	0.003%
49	7.625	2038	2048	2069	rBV	100698	179707	13.98%	1.801%
50	7.777	2093	2095	2096	rBV	436	176	0.01%	0.002%
51	7.812	2104	2106	2110	rVB	537	272	0.02%	0.003%
52	7.863	2119	2122	2125	rBV2	321	215	0.02%	0.002%
53	7.905	2131	2135	2139	rBV3	439	408	0.03%	0.004%
54	8.088	2182	2192	2226	rBV	326434	598651	46.56%	5.999%
55	8.471	2308	2311	2313	rBV	367	191	0.01%	0.002%
56	8.497	2317	2319	2322	rBV2	239	175	0.01%	0.002%
57	8.535	2327	2331	2333	rBV	477	325	0.03%	0.003%
58	8.760	2397	2401	2406	rBV2	399	335	0.03%	0.003%
59	8.854	2418	2430	2456	rBV	594552	970536	75.48%	9.725%
60	9.101	2505	2507	2514	rVB5	606	522	0.04%	0.005%
61	9.149	2519	2522	2529	rBV4	855	1083	0.08%	0.011%
62	9.236	2547	2549	2555	rVB3	359	185	0.01%	0.002%
63	9.285	2561	2564	2567	rBV2	325	236	0.02%	0.002%
64	9.455	2613	2617	2620	rVV4	336	287	0.02%	0.003%
65	9.545	2641	2645	2646	rBV2	385	262	0.02%	0.003%
66	9.657	2678	2680	2684	rBV2	406	340	0.03%	0.003%
67	9.760	2710	2712	2718	rVV	311	245	0.02%	0.002%
68	9.895	2752	2754	2759	rVB	571	378	0.03%	0.004%
69	9.937	2764	2767	2769	rBV2	406	238	0.02%	0.002%
70	10.066	2805	2807	2814	rVB2	251	172	0.01%	0.002%
71	10.098	2814	2817	2818	rBV	356	178	0.01%	0.002%
72	10.217	2842	2854	2876	rBV	397547	634911	49.38%	6.362%
73	10.461	2926	2930	2933	rBV3	623	539	0.04%	0.005%
74	10.481	2933	2936	2939	rVV3	325	219	0.02%	0.002%
75	10.538	2950	2954	2959	rBV4	619	573	0.04%	0.006%
76	10.567	2960	2963	2964	rBV2	357	191	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022005.D
 Acq On : 30 Aug 2021 15:26
 Operator : SY/MD
 Sample : M3573-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.580	2964	2967	2973	rVB3	661	681	0.05%	0.007%
78	10.747	3015	3019	3024	rBV3	364	379	0.03%	0.004%
79	10.847	3047	3050	3053	rVB2	634	437	0.03%	0.004%
80	10.870	3053	3057	3060	rBV2	623	490	0.04%	0.005%
81	10.918	3065	3072	3083	rVB6	2651	4236	0.33%	0.042%
82	10.976	3088	3090	3096	rVB	520	371	0.03%	0.004%
83	11.014	3099	3102	3104	rBV2	242	180	0.01%	0.002%
84	11.040	3105	3110	3116	rVB4	848	928	0.07%	0.009%
85	11.149	3139	3144	3150	rBV4	1304	1480	0.12%	0.015%
86	11.252	3164	3176	3196	rBV	631432	989034	76.92%	9.910%
87	11.625	3279	3292	3311	rBV	627356	995659	77.44%	9.977%
88	11.940	3387	3390	3394	rBV2	350	302	0.02%	0.003%
89	12.075	3430	3432	3433	rBV	429	185	0.01%	0.002%
90	12.259	3486	3489	3492	rBV2	357	226	0.02%	0.002%
91	12.281	3494	3496	3499	rVB2	468	224	0.02%	0.002%
92	12.481	3553	3558	3564	rBV3	432	477	0.04%	0.005%
93	12.522	3568	3571	3573	rBV	541	222	0.02%	0.002%
94	12.648	3608	3610	3611	rBV	410	207	0.02%	0.002%
95	13.201	3779	3782	3785	rVB2	663	375	0.03%	0.004%
96	13.243	3790	3795	3797	rBV4	624	510	0.04%	0.005%
97	13.516	3877	3880	3882	rBV2	731	532	0.04%	0.005%
98	13.734	3945	3948	3951	rBV2	495	347	0.03%	0.003%
99	13.763	3955	3957	3963	rVV2	533	398	0.03%	0.004%
100	13.825	3974	3976	3979	rBV2	398	279	0.02%	0.003%




Sum of corrected areas: 9979684

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022005.D
Acq On : 30 Aug 2021 15:26
Operator : SY/MD
Sample : M3573-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

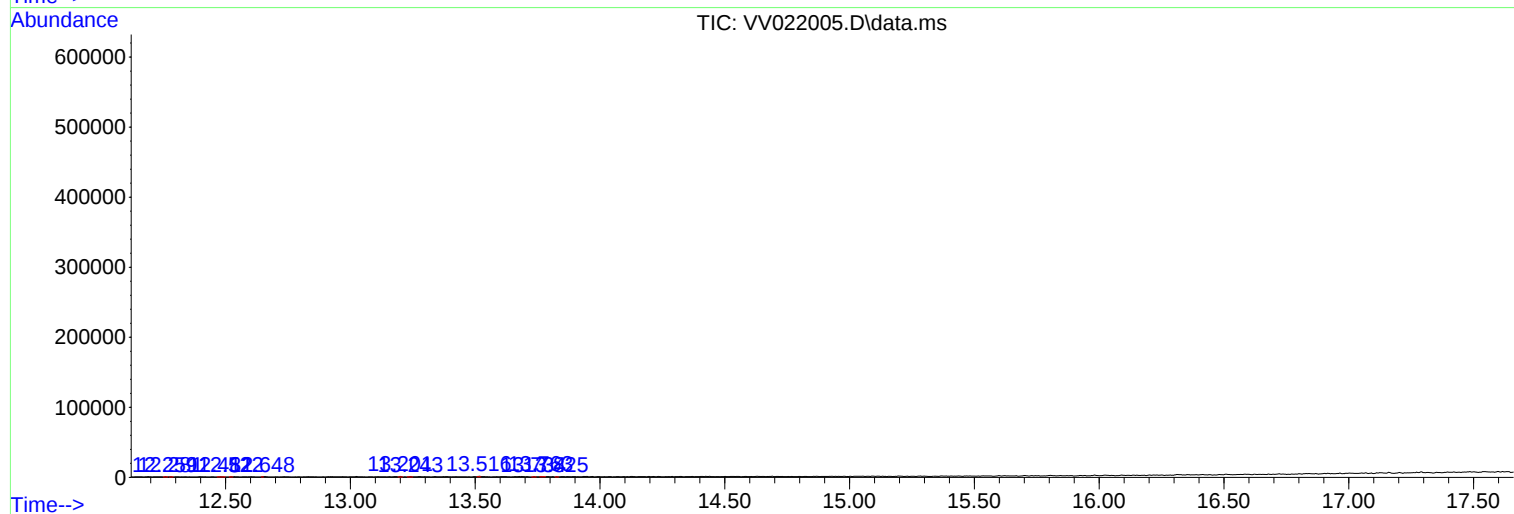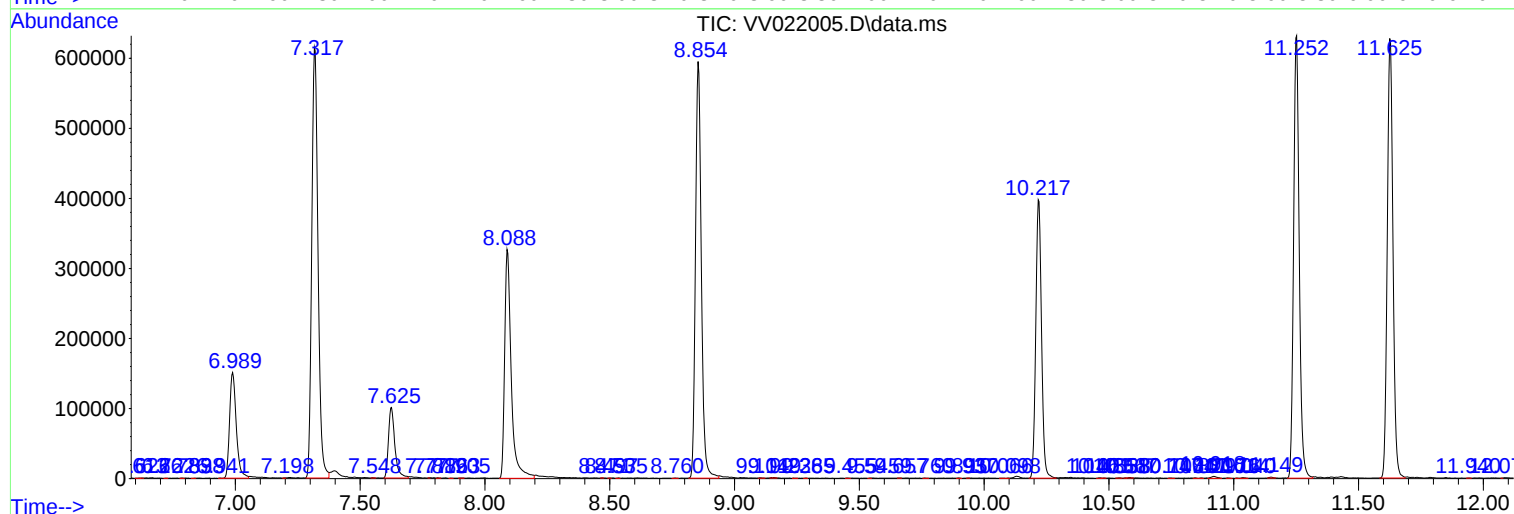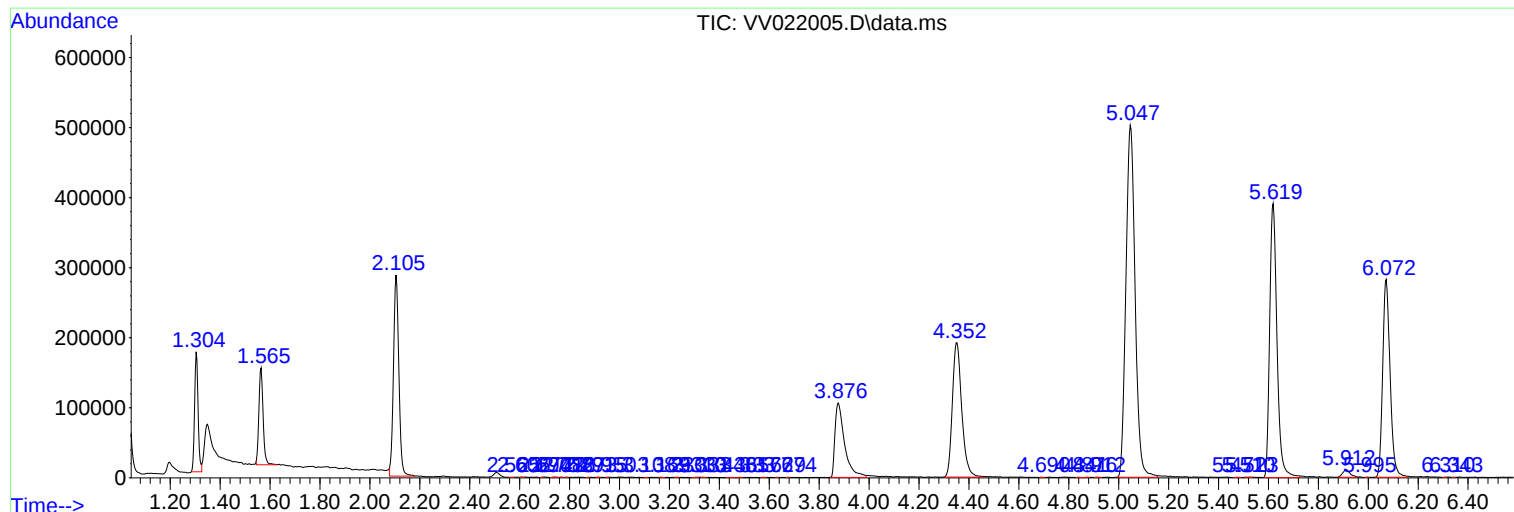

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022005.D
Acq On : 30 Aug 2021 15:26
Operator : SY/MD
Sample : M3573-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022005.D
Acq On : 30 Aug 2021 15:26
Operator : SY/MD
Sample : M3573-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
