

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022006.D
 Acq On : 30 Aug 2021 15:51
 Operator : SY/MD
 Sample : M3549-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	89	rBV	162516	161404	12.75%	1.638%
2	1.565	157	163	177	rVB	138633	156387	12.36%	1.587%
3	2.105	323	331	363	rVB	277721	424231	33.52%	4.306%
4	2.507	450	456	466	rVB4	6132	9876	0.78%	0.100%
5	2.587	478	481	483	rBV2	461	258	0.02%	0.003%
6	2.603	484	486	487	rBV	573	215	0.02%	0.002%
7	2.751	528	532	534	rBV3	241	258	0.02%	0.003%
8	2.764	534	536	539	rBV3	468	297	0.02%	0.003%
9	2.802	545	548	551	rVB2	347	209	0.02%	0.002%
10	2.825	552	555	556	rBV2	311	200	0.02%	0.002%
11	2.905	577	580	583	rBV2	328	267	0.02%	0.003%
12	2.992	604	607	610	rVB2	439	197	0.02%	0.002%
13	3.015	610	614	615	rBV2	222	132	0.01%	0.001%
14	3.024	615	617	620	rVB	298	136	0.01%	0.001%
15	3.056	622	627	631	rBV4	408	327	0.03%	0.003%
16	3.105	640	642	646	rBV	254	153	0.01%	0.002%
17	3.127	646	649	655	rVB3	453	388	0.03%	0.004%
18	3.368	721	724	729	rVV3	286	218	0.02%	0.002%
19	3.532	773	775	780	rVB2	285	176	0.01%	0.002%
20	3.603	794	797	799	rBV	237	156	0.01%	0.002%
21	3.806	858	860	864	rBV2	273	196	0.02%	0.002%
22	3.876	872	882	921	rBV	105702	297383	23.50%	3.018%
23	4.352	1012	1030	1057	rBV	191541	496046	39.20%	5.035%
24	4.709	1138	1141	1142	rBV2	497	227	0.02%	0.002%
25	4.741	1148	1151	1156	rBV3	474	472	0.04%	0.005%
26	4.767	1156	1159	1161	rBV	420	259	0.02%	0.003%
27	4.870	1187	1191	1192	rBV	365	214	0.02%	0.002%
28	4.899	1198	1200	1201	rBV	274	129	0.01%	0.001%
29	5.047	1228	1246	1285	rBV2	492471	1265522	100.00%	12.845%
30	5.346	1335	1339	1340	rBV3	536	371	0.03%	0.004%
31	5.397	1351	1355	1358	rBV3	592	464	0.04%	0.005%
32	5.558	1403	1405	1408	rBV2	271	194	0.02%	0.002%
33	5.619	1411	1424	1447	rBV	385948	769682	60.82%	7.812%
34	5.908	1505	1514	1534	rBV3	9417	19031	1.50%	0.193%
35	6.072	1550	1565	1594	rBV	277591	570001	45.04%	5.786%
36	6.333	1642	1646	1649	rBV3	807	424	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022006.D
 Acq On : 30 Aug 2021 15:51
 Operator : SY/MD
 Sample : M3549-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.349	1649	1651	1656	rVB3	327	256	0.02%	0.003%
38	6.371	1656	1658	1662	rBV	364	227	0.02%	0.002%
39	6.465	1685	1687	1688	rBV	219	117	0.01%	0.001%
40	6.506	1695	1700	1703	rBV	405	314	0.02%	0.003%
41	6.519	1703	1704	1707	rBV2	289	198	0.02%	0.002%
42	6.635	1737	1740	1742	rBV	270	191	0.02%	0.002%
43	6.654	1742	1746	1750	rVV4	735	624	0.05%	0.006%
44	6.696	1758	1759	1763	rVB3	640	262	0.02%	0.003%
45	6.719	1763	1766	1769	rBV2	540	321	0.03%	0.003%
46	6.735	1769	1771	1774	rVB2	291	137	0.01%	0.001%
47	6.760	1775	1779	1781	rBV	222	145	0.01%	0.001%
48	6.815	1792	1796	1797	rBV2	454	187	0.01%	0.002%
49	6.841	1802	1804	1805	rVV	344	135	0.01%	0.001%
50	6.989	1839	1850	1880	rBV	149409	274804	21.71%	2.789%
51	7.195	1910	1914	1918	rBV4	799	901	0.07%	0.009%
52	7.317	1940	1952	1972	rBV	596171	1052653	83.18%	10.684%
53	7.584	2032	2035	2037	rBV3	559	414	0.03%	0.004%
54	7.625	2037	2048	2065	rBV2	99634	176034	13.91%	1.787%
55	7.815	2105	2107	2110	rBV2	293	133	0.01%	0.001%
56	7.867	2121	2123	2129	rVB2	829	617	0.05%	0.006%
57	7.899	2130	2133	2135	rBV	283	162	0.01%	0.002%
58	7.912	2135	2137	2138	rBV	412	201	0.02%	0.002%
59	7.944	2143	2147	2149	rBV2	522	384	0.03%	0.004%
60	7.989	2158	2161	2165	rVB	573	387	0.03%	0.004%
61	8.034	2173	2175	2178	rBV	384	235	0.02%	0.002%
62	8.088	2182	2192	2226	rBV	334693	611129	48.29%	6.203%
63	8.529	2326	2329	2330	rBV	352	164	0.01%	0.002%
64	8.600	2346	2351	2352	rBV3	289	206	0.02%	0.002%
65	8.854	2418	2430	2457	rBV	579564	956450	75.58%	9.708%
66	9.140	2515	2519	2521	rBV3	1028	701	0.06%	0.007%
67	9.230	2544	2547	2550	rBV2	281	202	0.02%	0.002%
68	9.294	2565	2567	2570	rBV	242	174	0.01%	0.002%
69	9.317	2570	2574	2576	rVV2	201	134	0.01%	0.001%
70	9.394	2596	2598	2600	rBV2	397	171	0.01%	0.002%
71	9.484	2624	2626	2629	rVB2	350	207	0.02%	0.002%
72	9.535	2639	2642	2645	rBV2	339	228	0.02%	0.002%
73	9.831	2731	2734	2738	rBV2	271	250	0.02%	0.003%
74	9.857	2740	2742	2744	rBV	271	126	0.01%	0.001%
75	9.895	2751	2754	2755	rBV	215	127	0.01%	0.001%
76	10.101	2816	2818	2820	rBV	348	158	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022006.D
 Acq On : 30 Aug 2021 15:51
 Operator : SY/MD
 Sample : M3549-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.127	2820	2826	2836	rVV2	2567	4404	0.35%	0.045%
78	10.217	2842	2854	2880	rBV	401072	646277	51.07%	6.560%
79	10.635	2982	2984	2986	rBV	486	266	0.02%	0.003%
80	10.780	3027	3029	3031	rBV2	309	137	0.01%	0.001%
81	10.860	3051	3054	3057	rBV	282	192	0.02%	0.002%
82	10.921	3064	3073	3082	rVB7	2738	4836	0.38%	0.049%
83	10.963	3082	3086	3090	rBV3	431	340	0.03%	0.003%
84	11.252	3164	3176	3197	rBV	612710	962885	76.09%	9.773%
85	11.625	3280	3292	3313	rBV	601110	972253	76.83%	9.868%
86	11.844	3356	3360	3361	rBV2	431	253	0.02%	0.003%
87	12.104	3434	3441	3444	rBV4	644	608	0.05%	0.006%
88	12.185	3464	3466	3469	rVB	506	212	0.02%	0.002%
89	12.236	3479	3482	3485	rBV	257	190	0.02%	0.002%
90	12.474	3554	3556	3560	rVB	560	247	0.02%	0.003%
91	12.493	3560	3562	3566	rBV2	453	363	0.03%	0.004%
92	12.551	3578	3580	3582	rBV	348	154	0.01%	0.002%
93	12.731	3632	3636	3637	rBV	256	187	0.01%	0.002%
94	12.789	3649	3654	3655	rBV2	339	249	0.02%	0.003%
95	12.953	3703	3705	3707	rBV	381	171	0.01%	0.002%
96	13.040	3730	3732	3736	rBV2	337	262	0.02%	0.003%
97	13.156	3766	3768	3773	rVB3	610	410	0.03%	0.004%
98	13.188	3776	3778	3780	rBV2	308	128	0.01%	0.001%
99	13.316	3816	3818	3820	rBV2	358	164	0.01%	0.002%
100	13.487	3865	3871	3873	rBV2	449	470	0.04%	0.005%




Sum of corrected areas: 9852224

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022006.D
Acq On : 30 Aug 2021 15:51
Operator : SY/MD
Sample : M3549-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

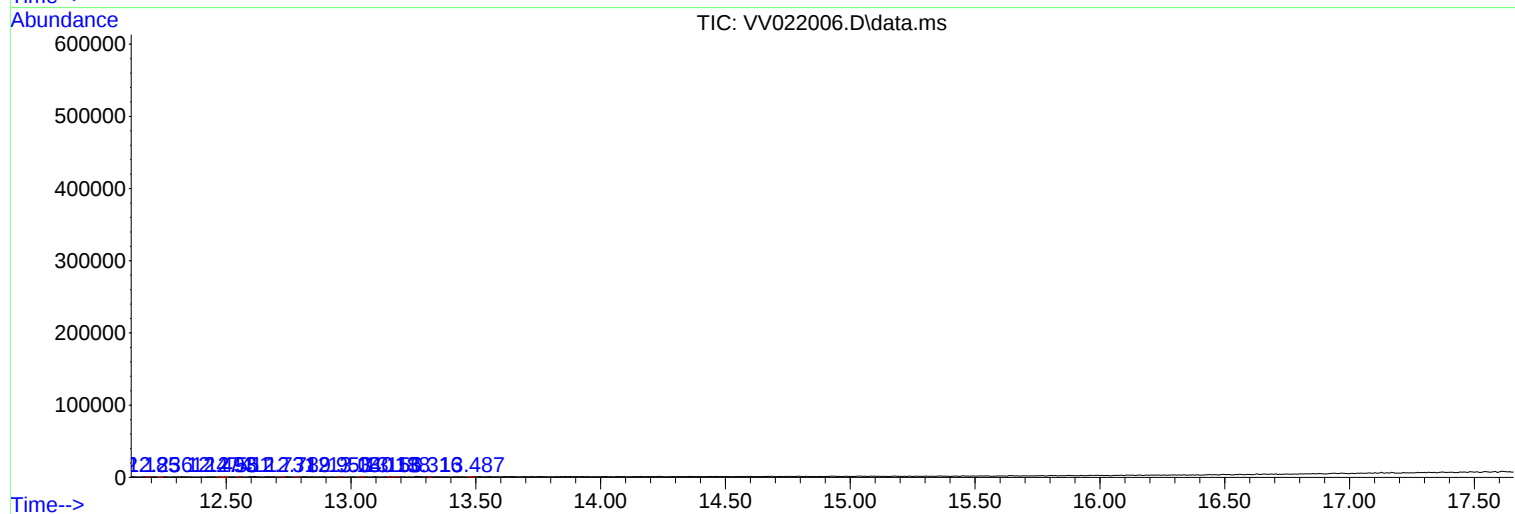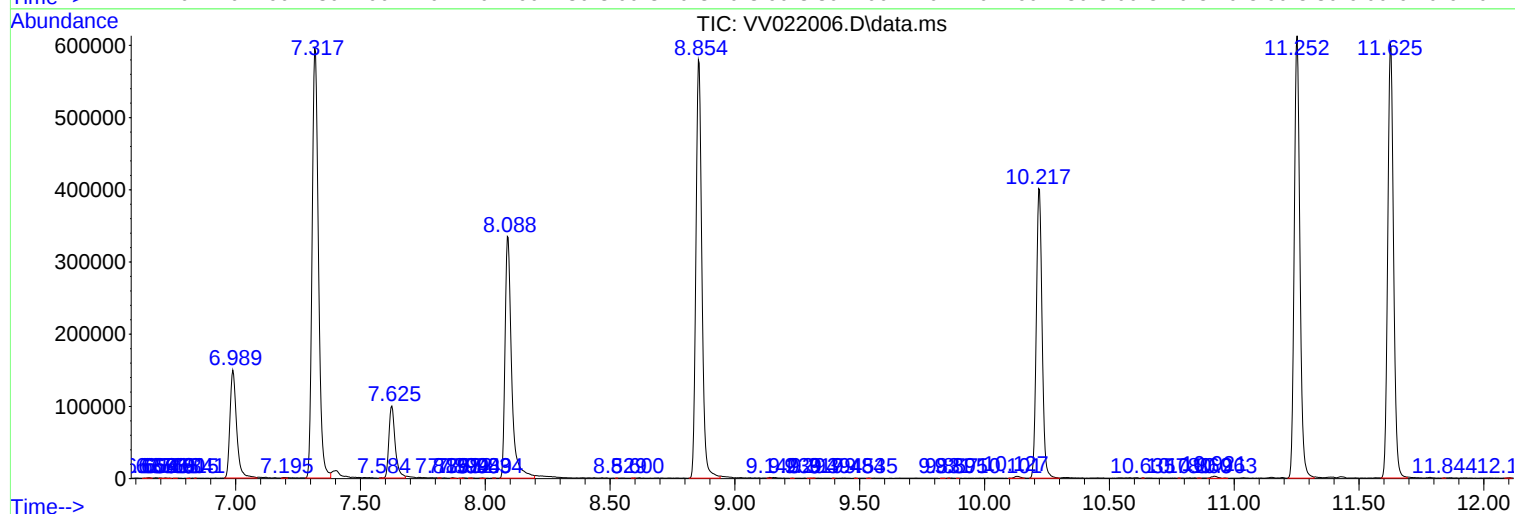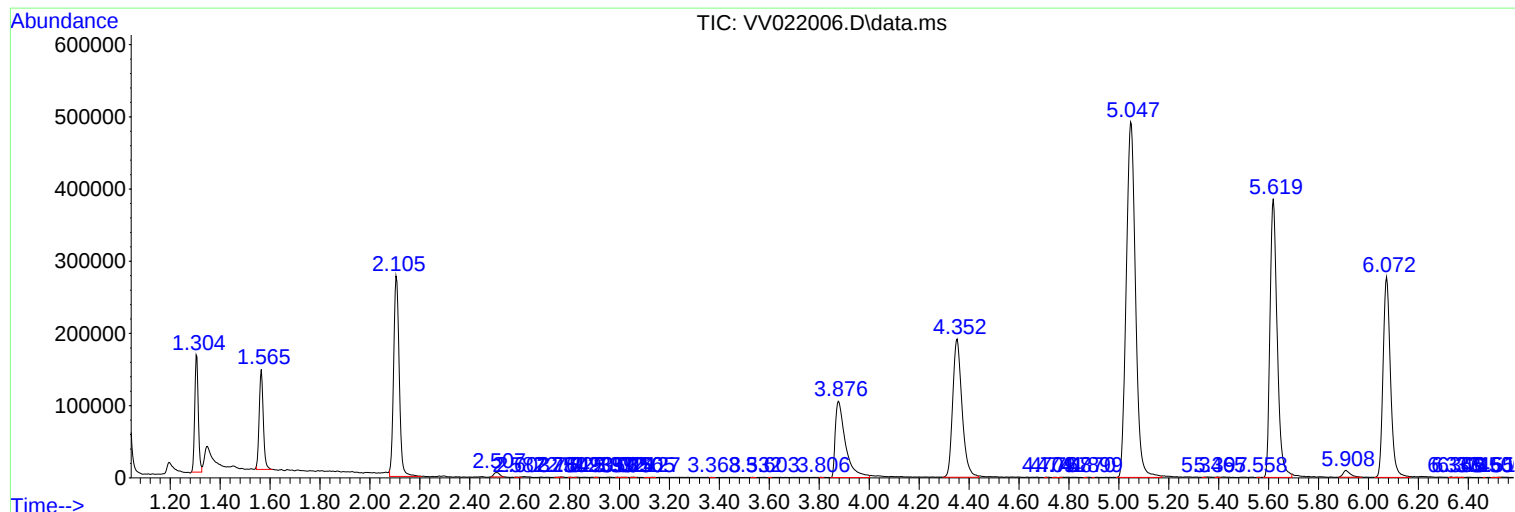

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022006.D
Acq On : 30 Aug 2021 15:51
Operator : SY/MD
Sample : M3549-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022006.D
Acq On : 30 Aug 2021 15:51
Operator : SY/MD
Sample : M3549-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------