

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022008.D
 Acq On : 30 Aug 2021 17:03
 Operator : SY/MD
 Sample : M3566-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022008.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.195	43	48	59	rBV	16900	29062	2.37%	0.296%
2	1.304	76	82	90	rBV	154378	153357	12.50%	1.563%
3	1.565	157	163	179	rVB	129385	151838	12.37%	1.548%
4	2.105	322	331	359	rVB	259503	396658	32.33%	4.043%
5	2.481	446	448	450	rBV2	390	242	0.02%	0.002%
6	2.539	464	466	469	rBV2	371	262	0.02%	0.003%
7	2.773	529	539	548	rBV9	2599	5030	0.41%	0.051%
8	2.851	556	563	566	rVB2	459	529	0.04%	0.005%
9	2.902	575	579	580	rBV2	341	194	0.02%	0.002%
10	2.960	595	597	600	rBV	260	193	0.02%	0.002%
11	3.166	658	661	662	rBV	400	171	0.01%	0.002%
12	3.285	695	698	704	rVB	9370	6345	0.52%	0.065%
13	3.542	773	778	780	rBV	180	160	0.01%	0.002%
14	3.812	858	862	864	rBV2	355	268	0.02%	0.003%
15	3.876	872	882	914	rBV	98185	268401	21.87%	2.736%
16	4.201	979	983	988	rVB4	880	769	0.06%	0.008%
17	4.352	1013	1030	1062	rBV	186756	479967	39.12%	4.892%
18	4.619	1110	1113	1117	rBV2	652	403	0.03%	0.004%
19	4.671	1125	1129	1132	rVB3	704	572	0.05%	0.006%
20	4.690	1132	1135	1136	rBV2	532	308	0.03%	0.003%
21	4.886	1194	1196	1200	rVB2	304	172	0.01%	0.002%
22	4.992	1227	1229	1230	rBV	414	173	0.01%	0.002%
23	5.047	1230	1246	1275	rBV2	478444	1227054	100.00%	12.507%
24	5.291	1319	1322	1325	rBV	360	293	0.02%	0.003%
25	5.359	1338	1343	1347	rBB3	664	509	0.04%	0.005%
26	5.413	1358	1360	1363	rVB2	502	249	0.02%	0.003%
27	5.429	1363	1365	1367	rBV	407	217	0.02%	0.002%
28	5.497	1383	1386	1389	rVV2	378	224	0.02%	0.002%
29	5.619	1410	1424	1460	rBV	413035	829688	67.62%	8.457%
30	5.912	1505	1515	1532	rBV4	6603	15167	1.24%	0.155%
31	5.989	1536	1539	1542	rBV2	444	360	0.03%	0.004%
32	6.072	1552	1565	1591	rBV	267543	553106	45.08%	5.638%
33	6.407	1666	1669	1671	rBV4	390	227	0.02%	0.002%
34	6.465	1684	1687	1689	rBV	370	177	0.01%	0.002%
35	6.632	1737	1739	1741	rBV2	378	231	0.02%	0.002%
36	6.693	1756	1758	1761	rVB	607	336	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022008.D
 Acq On : 30 Aug 2021 17:03
 Operator : SY/MD
 Sample : M3566-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.712	1761	1764	1766	rBV	589	366	0.03%	0.004%
38	6.786	1785	1787	1789	rVB2	429	207	0.02%	0.002%
39	6.805	1789	1793	1796	rVB2	300	287	0.02%	0.003%
40	6.822	1796	1798	1803	rVB2	284	196	0.02%	0.002%
41	6.850	1803	1807	1809	rBV2	375	216	0.02%	0.002%
42	6.902	1821	1823	1830	rVB4	364	343	0.03%	0.003%
43	6.989	1839	1850	1877	rBV	147780	271377	22.12%	2.766%
44	7.249	1927	1931	1933	rBV3	675	582	0.05%	0.006%
45	7.320	1940	1953	1971	rBV	586081	1019164	83.06%	10.388%
46	7.571	2026	2031	2033	rBV3	500	373	0.03%	0.004%
47	7.625	2037	2048	2071	rBV	97498	176201	14.36%	1.796%
48	7.789	2097	2099	2103	rBV4	477	377	0.03%	0.004%
49	7.850	2114	2118	2121	rVB2	700	538	0.04%	0.005%
50	7.947	2136	2148	2155	rBV4	3334	6543	0.53%	0.067%
51	8.014	2166	2169	2173	rVB3	509	390	0.03%	0.004%
52	8.088	2182	2192	2224	rBV	317314	574443	46.81%	5.855%
53	8.481	2312	2314	2317	rVB3	310	214	0.02%	0.002%
54	8.513	2322	2324	2326	rVB	516	203	0.02%	0.002%
55	8.548	2330	2335	2342	rBV4	671	880	0.07%	0.009%
56	8.587	2345	2347	2349	rVB2	397	179	0.01%	0.002%
57	8.677	2373	2375	2380	rVB2	377	276	0.02%	0.003%
58	8.702	2380	2383	2389	rVB	538	386	0.03%	0.004%
59	8.731	2389	2392	2393	rBV2	304	162	0.01%	0.002%
60	8.751	2393	2398	2400	rBV3	427	359	0.03%	0.004%
61	8.780	2405	2407	2410	rBV2	341	185	0.02%	0.002%
62	8.854	2418	2430	2461	rBV	608721	1007335	82.09%	10.268%
63	9.146	2516	2521	2522	rBV3	936	713	0.06%	0.007%
64	9.194	2533	2536	2542	rVB3	410	374	0.03%	0.004%
65	9.275	2557	2561	2563	rBV2	282	230	0.02%	0.002%
66	9.323	2572	2576	2577	rBV	324	214	0.02%	0.002%
67	9.400	2597	2600	2603	rVB	429	268	0.02%	0.003%
68	9.420	2603	2606	2608	rBV	381	268	0.02%	0.003%
69	9.590	2657	2659	2660	rBV	480	158	0.01%	0.002%
70	9.641	2673	2675	2678	rBV2	272	163	0.01%	0.002%
71	9.854	2739	2741	2746	rVB2	421	323	0.03%	0.003%
72	9.886	2746	2751	2752	rBV2	338	198	0.02%	0.002%
73	10.072	2806	2809	2812	rBV2	400	284	0.02%	0.003%
74	10.130	2818	2827	2838	rBV4	2466	4497	0.37%	0.046%
75	10.217	2842	2854	2875	rBV	396716	626995	51.10%	6.391%
76	10.387	2897	2907	2922	rVB2	5891	10191	0.83%	0.104%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022008.D
 Acq On : 30 Aug 2021 17:03
 Operator : SY/MD
 Sample : M3566-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.445	2922	2925	2929	rBV	377	334	0.03%	0.003%
78	10.526	2946	2950	2951	rBV2	336	235	0.02%	0.002%
79	10.583	2965	2968	2972	rBV2	1001	680	0.06%	0.007%
80	10.664	2988	2993	2998	rBV5	565	615	0.05%	0.006%
81	10.844	3047	3049	3051	rBV	267	168	0.01%	0.002%
82	10.860	3052	3054	3057	rBV2	316	167	0.01%	0.002%
83	11.085	3121	3124	3126	rBV	378	244	0.02%	0.002%
84	11.149	3138	3144	3151	rBV6	1309	1715	0.14%	0.017%
85	11.252	3164	3176	3208	rBV	644950	1019813	83.11%	10.395%
86	11.522	3257	3260	3263	rBV	422	249	0.02%	0.003%
87	11.538	3263	3265	3267	rBV2	627	316	0.03%	0.003%
88	11.554	3267	3270	3273	rVB3	443	357	0.03%	0.004%
89	11.625	3281	3292	3312	rBV	591840	944066	76.94%	9.623%
90	11.931	3384	3387	3390	rBV2	441	283	0.02%	0.003%
91	12.072	3428	3431	3433	rBV	406	239	0.02%	0.002%
92	12.169	3459	3461	3468	rVB	426	330	0.03%	0.003%
93	12.210	3468	3474	3475	rBV	361	281	0.02%	0.003%
94	12.252	3483	3487	3496	rVB4	1031	1218	0.10%	0.012%
95	12.345	3514	3516	3523	rVV3	354	366	0.03%	0.004%
96	12.873	3675	3680	3686	rBV3	500	668	0.05%	0.007%
97	13.265	3796	3802	3812	rBV5	1595	2443	0.20%	0.025%
98	13.516	3873	3880	3888	rBV2	2164	3505	0.29%	0.036%
99	13.751	3948	3953	3962	rBV5	1949	2420	0.20%	0.025%
100	13.844	3978	3982	3984	rBV2	483	380	0.03%	0.004%




Sum of corrected areas: 9810662

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022008.D
Acq On : 30 Aug 2021 17:03
Operator : SY/MD
Sample : M3566-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

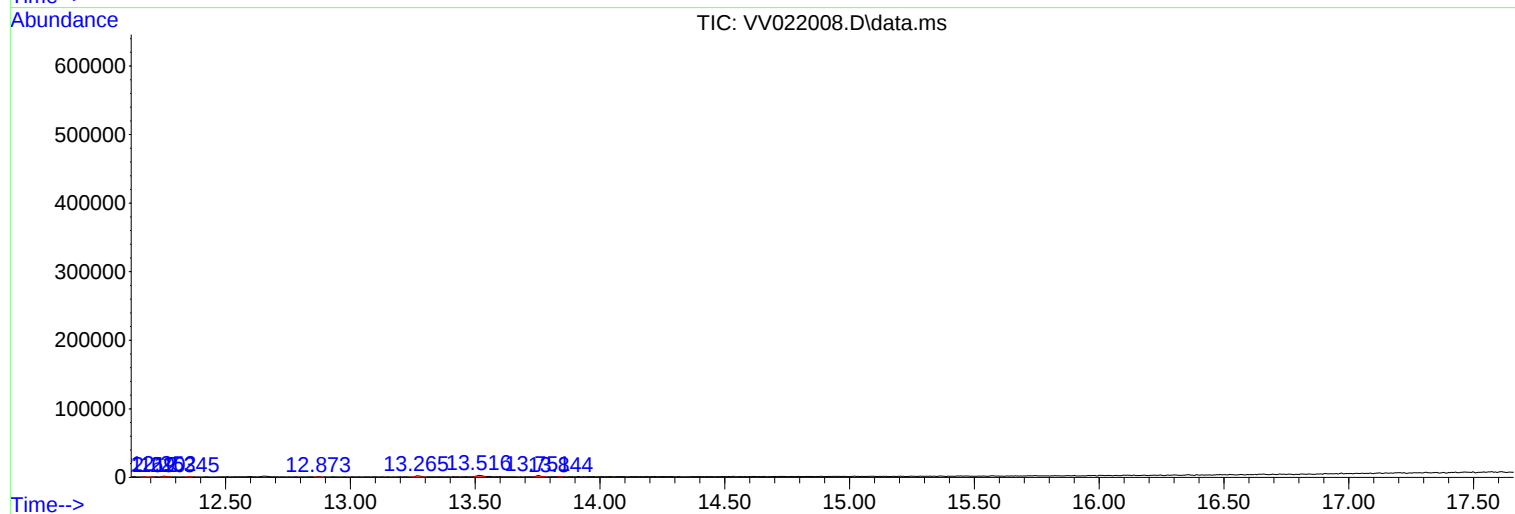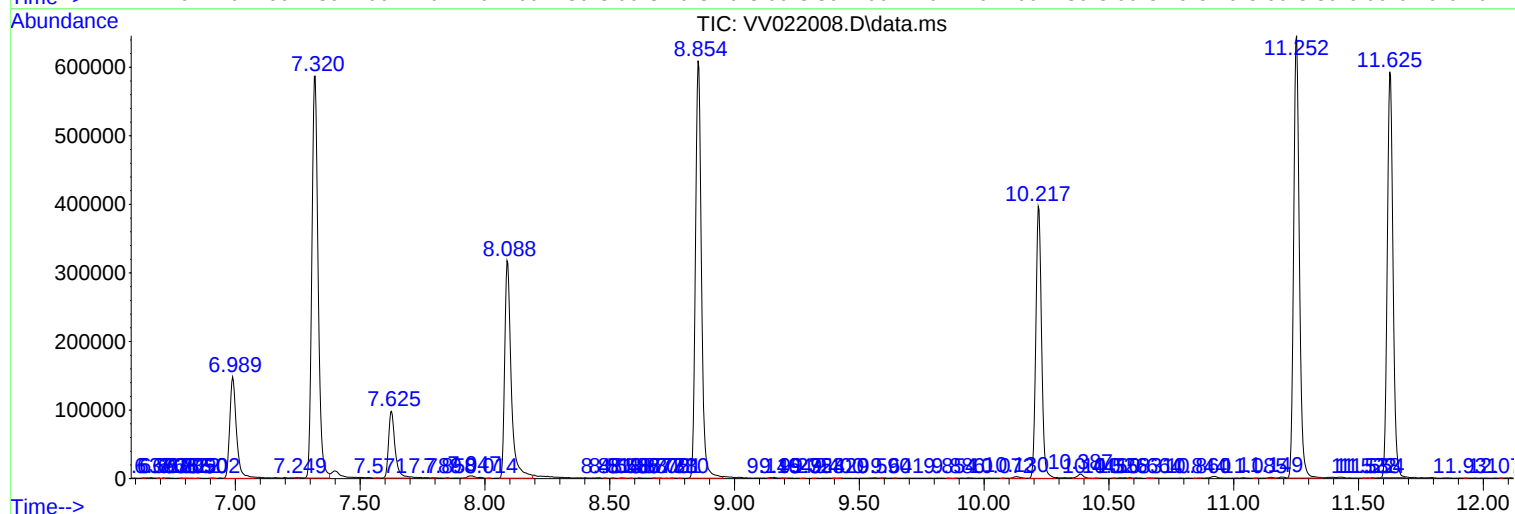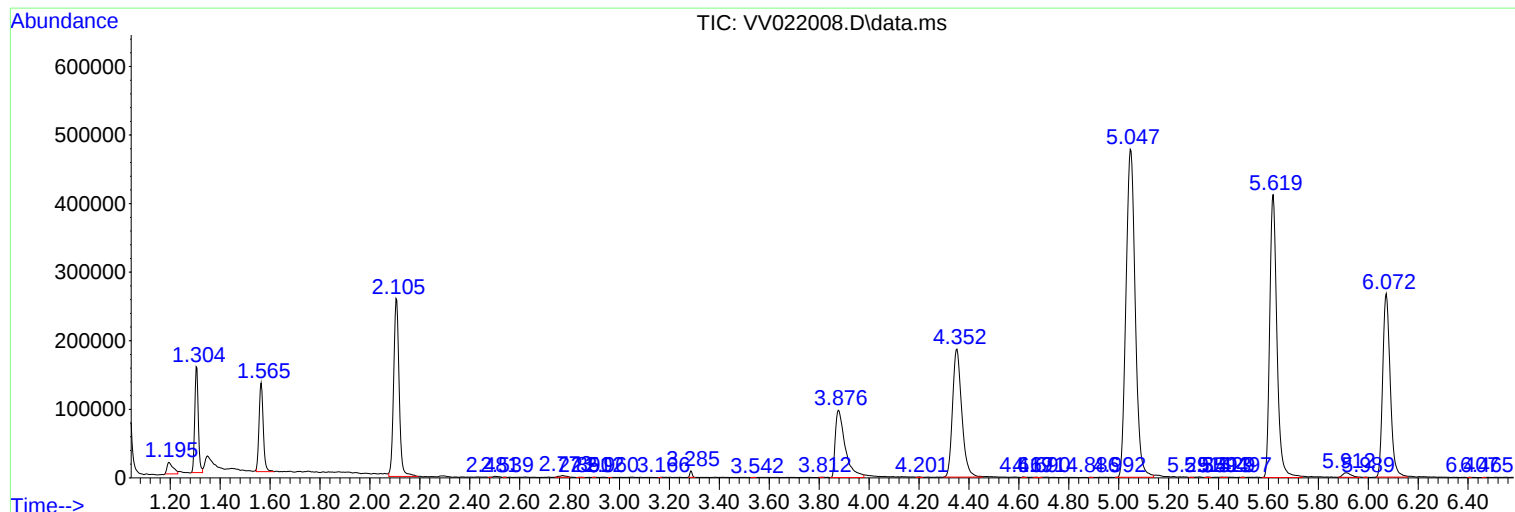

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022008.D
Acq On : 30 Aug 2021 17:03
Operator : SY/MD
Sample : M3566-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022008.D
Acq On : 30 Aug 2021 17:03
Operator : SY/MD
Sample : M3566-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
