

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022009.D
 Acq On : 30 Aug 2021 17:28
 Operator : SY/MD
 Sample : M3566-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022009.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	91	rBV	154865	152994	12.45%	1.555%
2	1.564	156	163	178	rVB	131715	154196	12.54%	1.567%
3	2.105	322	331	357	rVB	272054	408846	33.26%	4.156%
4	2.584	476	480	483	rBV4	384	386	0.03%	0.004%
5	2.635	492	496	500	rBV3	385	398	0.03%	0.004%
6	2.741	523	529	530	rBV4	508	433	0.04%	0.004%
7	2.773	530	539	548	rVB8	2281	4983	0.41%	0.051%
8	2.867	565	568	573	rVB2	373	279	0.02%	0.003%
9	3.037	616	621	623	rBV2	443	264	0.02%	0.003%
10	3.085	633	636	642	rBV3	485	337	0.03%	0.003%
11	3.175	662	664	668	rBV2	369	171	0.01%	0.002%
12	3.307	702	705	707	rBV3	499	272	0.02%	0.003%
13	3.342	712	716	719	rBV2	360	248	0.02%	0.003%
14	3.432	741	744	747	rBV	279	190	0.02%	0.002%
15	3.584	788	791	795	rBV2	249	247	0.02%	0.003%
16	3.635	804	807	810	rBV2	371	215	0.02%	0.002%
17	3.793	853	856	859	rBV2	295	210	0.02%	0.002%
18	3.876	872	882	915	rBV	103417	277621	22.59%	2.822%
19	4.352	1015	1030	1062	rBV	189384	481735	39.19%	4.897%
20	4.596	1101	1106	1110	rBV3	721	561	0.05%	0.006%
21	4.625	1110	1115	1120	rBV5	436	410	0.03%	0.004%
22	4.712	1140	1142	1147	rVB3	625	406	0.03%	0.004%
23	4.815	1170	1174	1175	rBV	303	180	0.01%	0.002%
24	4.957	1214	1218	1220	rBV2	316	243	0.02%	0.002%
25	5.047	1229	1246	1272	rBV2	479828	1229219	100.00%	12.495%
26	5.374	1346	1348	1350	rVB2	384	164	0.01%	0.002%
27	5.571	1407	1409	1411	rVB3	716	272	0.02%	0.003%
28	5.619	1411	1424	1460	rBV	404315	829702	67.50%	8.434%
29	5.908	1505	1514	1527	rBV6	9189	20083	1.63%	0.204%
30	6.072	1551	1565	1586	rBV	270670	552914	44.98%	5.620%
31	6.313	1637	1640	1641	rBV3	462	212	0.02%	0.002%
32	6.326	1641	1644	1652	rVB5	598	438	0.04%	0.004%
33	6.387	1660	1663	1666	rBV3	356	224	0.02%	0.002%
34	6.484	1690	1693	1696	rBV3	355	231	0.02%	0.002%
35	6.509	1699	1701	1705	rBV3	369	221	0.02%	0.002%
36	6.587	1721	1725	1728	rBV2	220	242	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022009.D
 Acq On : 30 Aug 2021 17:28
 Operator : SY/MD
 Sample : M3566-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.645	1734	1743	1746	rBV2	915	1077	0.09%	0.011%
38	6.767	1779	1781	1786	rVB2	467	242	0.02%	0.002%
39	6.812	1792	1795	1797	rBV2	378	197	0.02%	0.002%
40	6.841	1801	1804	1808	rVB	592	277	0.02%	0.003%

41	6.940	1829	1835	1836	rBV	185	161	0.01%	0.002%
42	6.989	1839	1850	1880	rBV	146763	272916	22.20%	2.774%
43	7.246	1927	1930	1933	rBV2	475	379	0.03%	0.004%
44	7.317	1939	1952	1971	rBV	582562	1022911	83.22%	10.398%
45	7.625	2038	2048	2071	rBV	98446	174336	14.18%	1.772%

46	7.780	2094	2096	2099	rBV3	414	268	0.02%	0.003%
47	7.834	2109	2113	2117	rBV3	627	516	0.04%	0.005%
48	7.902	2130	2134	2138	rBV5	835	845	0.07%	0.009%
49	7.940	2138	2146	2155	rVV3	2970	5027	0.41%	0.051%
50	7.979	2156	2158	2161	rVV2	745	482	0.04%	0.005%

51	7.998	2163	2164	2169	rVB3	601	243	0.02%	0.002%
52	8.027	2169	2173	2175	rBV3	277	222	0.02%	0.002%
53	8.088	2180	2192	2226	rBV	321567	589549	47.96%	5.993%
54	8.419	2293	2295	2299	rVV	426	207	0.02%	0.002%
55	8.439	2299	2301	2306	rVB2	341	207	0.02%	0.002%

56	8.625	2356	2359	2364	rVB4	641	546	0.04%	0.006%
57	8.683	2375	2377	2381	rVB2	361	191	0.02%	0.002%
58	8.699	2381	2382	2385	rBV2	352	170	0.01%	0.002%
59	8.853	2418	2430	2455	rBV	613705	1011086	82.25%	10.278%
60	9.021	2478	2482	2493	rVB7	1086	1542	0.13%	0.016%

61	9.143	2516	2520	2522	rBV4	824	679	0.06%	0.007%
62	9.223	2543	2545	2548	rVB2	509	251	0.02%	0.003%
63	9.242	2548	2551	2555	rBV2	288	301	0.02%	0.003%
64	9.384	2591	2595	2599	rVB2	231	192	0.02%	0.002%
65	9.435	2605	2611	2616	rBV2	448	476	0.04%	0.005%

66	9.551	2643	2647	2648	rBV2	289	207	0.02%	0.002%
67	9.583	2654	2657	2660	rBV2	427	335	0.03%	0.003%
68	9.741	2703	2706	2708	rBV3	262	167	0.01%	0.002%
69	9.776	2714	2717	2719	rBV	239	162	0.01%	0.002%
70	9.828	2731	2733	2735	rBV2	278	160	0.01%	0.002%

71	9.863	2743	2744	2749	rBV2	213	158	0.01%	0.002%
72	10.088	2810	2814	2817	rBV	264	240	0.02%	0.002%
73	10.127	2820	2826	2829	rBV2	1892	2162	0.18%	0.022%
74	10.217	2842	2854	2877	rBV	391552	625265	50.87%	6.356%
75	10.545	2951	2956	2961	rBV5	463	628	0.05%	0.006%

76	10.599	2971	2973	2979	rVB3	562	423	0.03%	0.004%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022009.D
 Acq On : 30 Aug 2021 17:28
 Operator : SY/MD
 Sample : M3566-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.696	2999	3003	3004	rBV	289	195	0.02%	0.002%
78	10.757	3019	3022	3024	rBV2	445	260	0.02%	0.003%
79	10.834	3042	3046	3047	rBV2	449	221	0.02%	0.002%
80	11.024	3101	3105	3107	rBV3	608	488	0.04%	0.005%
81	11.140	3138	3141	3142	rBV2	516	312	0.03%	0.003%
82	11.194	3151	3158	3164	rBV2	884	1121	0.09%	0.011%
83	11.252	3164	3176	3195	rBV	655475	1029180	83.73%	10.462%
84	11.538	3262	3265	3268	rBV2	418	255	0.02%	0.003%
85	11.625	3281	3292	3313	rBV	602825	963316	78.37%	9.792%
86	11.892	3372	3375	3376	rBV	334	221	0.02%	0.002%
87	12.004	3406	3410	3413	rBV3	658	520	0.04%	0.005%
88	12.101	3435	3440	3442	rVV4	630	559	0.05%	0.006%
89	12.178	3462	3464	3467	rBV2	349	230	0.02%	0.002%
90	12.255	3480	3488	3496	rBV2	696	1252	0.10%	0.013%
91	12.471	3552	3555	3556	rBV	341	169	0.01%	0.002%
92	12.590	3590	3592	3596	rBV2	288	211	0.02%	0.002%
93	12.654	3606	3612	3616	rBV3	942	959	0.08%	0.010%
94	12.783	3649	3652	3654	rBV	298	200	0.02%	0.002%
95	12.853	3671	3674	3676	rBV2	326	212	0.02%	0.002%
96	13.268	3800	3803	3807	rBV3	1026	839	0.07%	0.009%
97	13.754	3948	3954	3959	rBV4	1057	1278	0.10%	0.013%
98	13.937	4009	4011	4013	rBV	463	201	0.02%	0.002%
99	14.072	4051	4053	4055	rBV2	386	215	0.02%	0.002%
100	14.606	4217	4219	4220	rBV	631	160	0.01%	0.002%




Sum of corrected areas: 9837724

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022009.D
Acq On : 30 Aug 2021 17:28
Operator : SY/MD
Sample : M3566-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

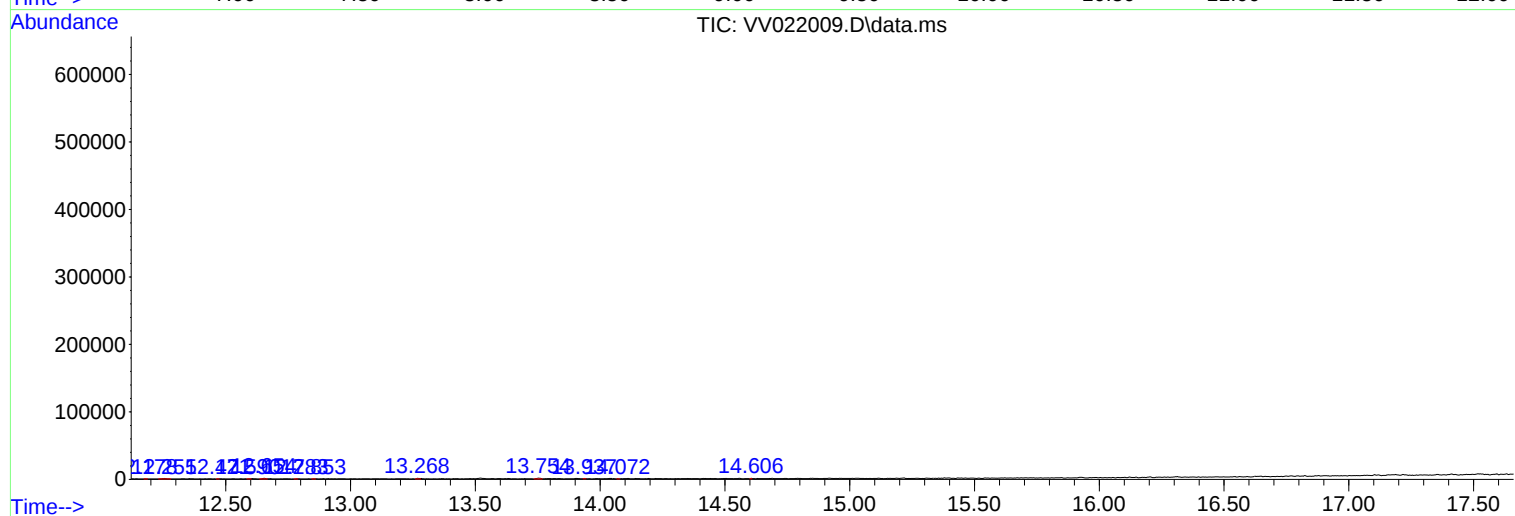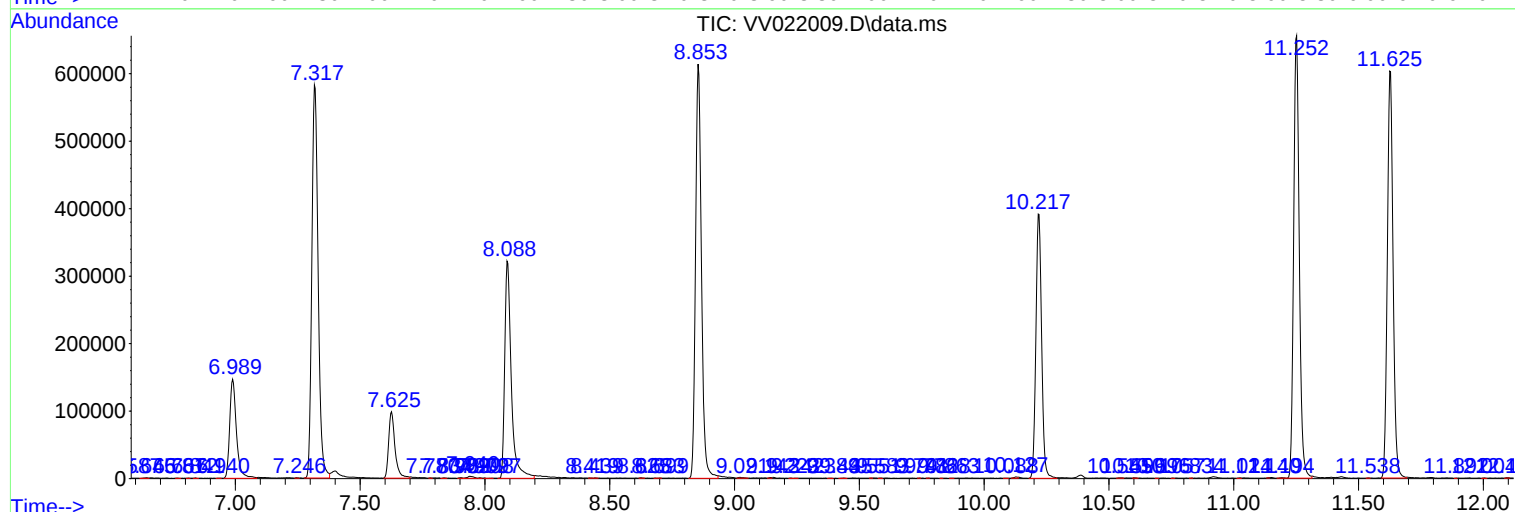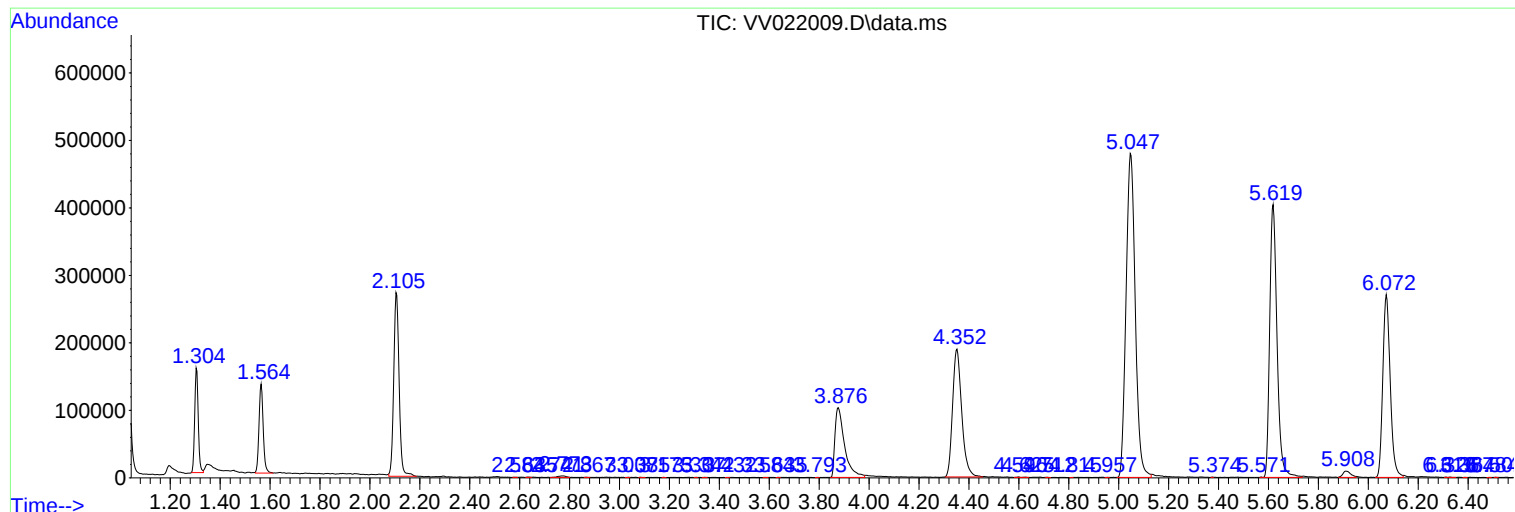

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022009.D
Acq On : 30 Aug 2021 17:28
Operator : SY/MD
Sample : M3566-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022009.D
Acq On : 30 Aug 2021 17:28
Operator : SY/MD
Sample : M3566-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
