

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022010.D
 Acq On : 30 Aug 2021 17:52
 Operator : SY/MD
 Sample : M3566-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022010.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	92	rBV	155537	154890	12.57%	1.588%
2	1.564	156	163	175	rVB	130429	148547	12.05%	1.523%
3	2.105	322	331	346	rBV	262394	378147	30.69%	3.877%
4	2.886	569	574	575	rBV2	243	187	0.02%	0.002%
5	2.928	585	587	589	rBV2	302	170	0.01%	0.002%
6	3.018	613	615	617	rVB2	371	145	0.01%	0.001%
7	3.079	629	634	635	rBV2	259	204	0.02%	0.002%
8	3.198	669	671	674	rVV3	449	210	0.02%	0.002%
9	3.252	686	688	691	rVB2	474	251	0.02%	0.003%
10	3.307	703	705	708	rVB4	304	224	0.02%	0.002%
11	3.568	781	786	788	rBV	266	193	0.02%	0.002%
12	3.677	818	820	827	rVB3	380	316	0.03%	0.003%
13	3.738	834	839	843	rVB2	436	367	0.03%	0.004%
14	3.757	843	845	847	rBV	293	149	0.01%	0.002%
15	3.876	872	882	919	rBV	98735	269761	21.89%	2.766%
16	4.352	1013	1030	1059	rBV	187812	484596	39.32%	4.969%
17	4.770	1157	1160	1163	rBV2	348	214	0.02%	0.002%
18	4.799	1166	1169	1172	rVB	547	293	0.02%	0.003%
19	4.825	1175	1177	1179	rVV2	455	181	0.01%	0.002%
20	5.050	1229	1247	1275	rBV2	482988	1232331	100.00%	12.635%
21	5.352	1339	1341	1344	rBV3	304	179	0.01%	0.002%
22	5.384	1349	1351	1356	rVB3	532	384	0.03%	0.004%
23	5.416	1359	1361	1366	rVB3	864	674	0.05%	0.007%
24	5.442	1366	1369	1372	rBV3	378	254	0.02%	0.003%
25	5.619	1409	1424	1454	rBV	404312	825822	67.01%	8.467%
26	5.912	1504	1515	1533	rBV3	11045	23358	1.90%	0.239%
27	6.072	1551	1565	1589	rBV	268159	555822	45.10%	5.699%
28	6.410	1666	1670	1671	rBV2	445	262	0.02%	0.003%
29	6.423	1671	1674	1679	rVB3	600	414	0.03%	0.004%
30	6.448	1679	1682	1684	rBV2	262	162	0.01%	0.002%
31	6.529	1704	1707	1710	rBV3	491	360	0.03%	0.004%
32	6.574	1718	1721	1725	rBV2	494	426	0.03%	0.004%
33	6.680	1752	1754	1758	rVB2	995	406	0.03%	0.004%
34	6.712	1759	1764	1768	rBV2	606	451	0.04%	0.005%
35	6.815	1794	1796	1801	rVB2	396	245	0.02%	0.003%
36	6.866	1809	1812	1815	rBV2	263	187	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022010.D
 Acq On : 30 Aug 2021 17:52
 Operator : SY/MD
 Sample : M3566-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.989	1839	1850	1872	rBV	146972	269725	21.89%	2.766%
38	7.317	1941	1952	1971	rBV	584862	1021509	82.89%	10.474%
39	7.625	2037	2048	2066	rBV	96589	172426	13.99%	1.768%
40	7.841	2113	2115	2116	rBV	435	167	0.01%	0.002%
41	7.892	2125	2131	2133	rBV2	509	407	0.03%	0.004%
42	7.944	2138	2147	2156	rBV5	2295	4403	0.36%	0.045%
43	7.979	2156	2158	2164	rVB3	671	477	0.04%	0.005%
44	8.021	2168	2171	2175	rBV2	277	247	0.02%	0.003%
45	8.088	2182	2192	2226	rBV	313441	568558	46.14%	5.830%
46	8.439	2299	2301	2305	rVB2	661	310	0.03%	0.003%
47	8.567	2337	2341	2344	rBV3	347	276	0.02%	0.003%
48	8.600	2349	2351	2355	rVB2	352	202	0.02%	0.002%
49	8.622	2355	2358	2367	rVB2	824	612	0.05%	0.006%
50	8.657	2367	2369	2373	rBV3	492	241	0.02%	0.002%
51	8.690	2376	2379	2382	rBV3	377	346	0.03%	0.004%
52	8.763	2400	2402	2405	rBV2	383	226	0.02%	0.002%
53	8.854	2418	2430	2462	rBV	616098	1012748	82.18%	10.384%
54	9.075	2498	2499	2501	rBV2	328	143	0.01%	0.001%
55	9.108	2505	2509	2510	rBV3	439	307	0.02%	0.003%
56	9.143	2516	2520	2523	rBV2	847	922	0.07%	0.009%
57	9.233	2547	2548	2554	rBV3	362	311	0.03%	0.003%
58	9.259	2554	2556	2557	rVV3	402	155	0.01%	0.002%
59	9.297	2565	2568	2575	rVB	441	438	0.04%	0.004%
60	9.333	2575	2579	2580	rBV	281	164	0.01%	0.002%
61	9.342	2580	2582	2584	rBV	285	142	0.01%	0.001%
62	9.554	2642	2648	2650	rBV2	455	379	0.03%	0.004%
63	9.718	2696	2699	2702	rVB2	268	142	0.01%	0.001%
64	9.741	2702	2706	2707	rBV	285	233	0.02%	0.002%
65	9.931	2763	2765	2769	rBV3	272	195	0.02%	0.002%
66	10.027	2793	2795	2797	rBV2	253	152	0.01%	0.002%
67	10.124	2816	2825	2826	rBV3	1794	1622	0.13%	0.017%
68	10.217	2842	2854	2878	rBV	391193	615881	49.98%	6.315%
69	10.387	2900	2907	2916	rVB2	3156	4536	0.37%	0.047%
70	10.493	2938	2940	2942	rBV2	290	148	0.01%	0.002%
71	10.525	2947	2950	2953	rBV2	473	387	0.03%	0.004%
72	10.638	2982	2985	2986	rBV	377	201	0.02%	0.002%
73	10.657	2989	2991	2993	rVV	536	265	0.02%	0.003%
74	10.680	2996	2998	3002	rVV	358	142	0.01%	0.001%
75	10.699	3002	3004	3007	rVB	352	197	0.02%	0.002%
76	10.722	3008	3011	3013	rBV2	218	142	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022010.D
 Acq On : 30 Aug 2021 17:52
 Operator : SY/MD
 Sample : M3566-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.767	3021	3025	3029	rBV	420	457	0.04%	0.005%
78	10.802	3031	3036	3041	rVV2	276	322	0.03%	0.003%
79	10.892	3062	3064	3066	rVV	477	302	0.02%	0.003%
80	10.921	3070	3073	3081	rVV5	2932	3074	0.25%	0.032%
81	11.040	3106	3110	3113	rBV2	673	628	0.05%	0.006%
82	11.120	3132	3135	3136	rVB2	431	191	0.02%	0.002%
83	11.146	3139	3143	3148	rBV5	1258	1637	0.13%	0.017%
84	11.191	3154	3157	3163	rVB5	713	677	0.05%	0.007%
85	11.252	3165	3176	3197	rBV	647673	1022227	82.95%	10.481%
86	11.570	3272	3275	3278	rVB3	524	307	0.02%	0.003%
87	11.628	3281	3293	3317	rBV	600460	958605	77.79%	9.829%
88	11.802	3345	3347	3352	rVV2	520	343	0.03%	0.004%
89	11.837	3355	3358	3362	rBV2	536	316	0.03%	0.003%
90	11.969	3395	3399	3400	rBV	371	218	0.02%	0.002%
91	12.458	3548	3551	3554	rBV2	312	261	0.02%	0.003%
92	12.487	3558	3560	3563	rVV3	450	218	0.02%	0.002%
93	12.561	3581	3583	3587	rVB2	344	202	0.02%	0.002%
94	12.654	3608	3612	3614	rBV2	704	586	0.05%	0.006%
95	12.818	3660	3663	3665	rBV2	285	156	0.01%	0.002%
96	12.905	3688	3690	3695	rVB2	673	386	0.03%	0.004%
97	12.959	3705	3707	3711	rBV	339	221	0.02%	0.002%
98	13.265	3800	3802	3803	rBV	406	156	0.01%	0.002%
99	13.355	3825	3830	3833	rBV2	483	459	0.04%	0.005%
100	13.940	4010	4012	4014	rBV2	283	146	0.01%	0.001%




Sum of corrected areas: 9752961

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022010.D
Acq On : 30 Aug 2021 17:52
Operator : SY/MD
Sample : M3566-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

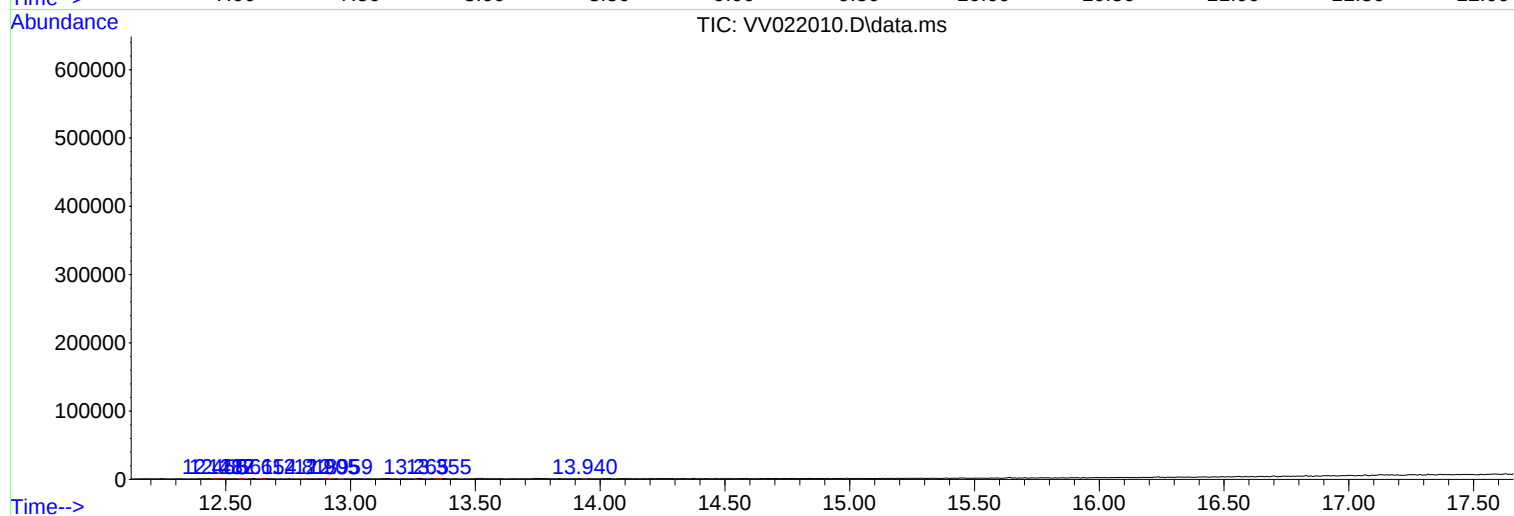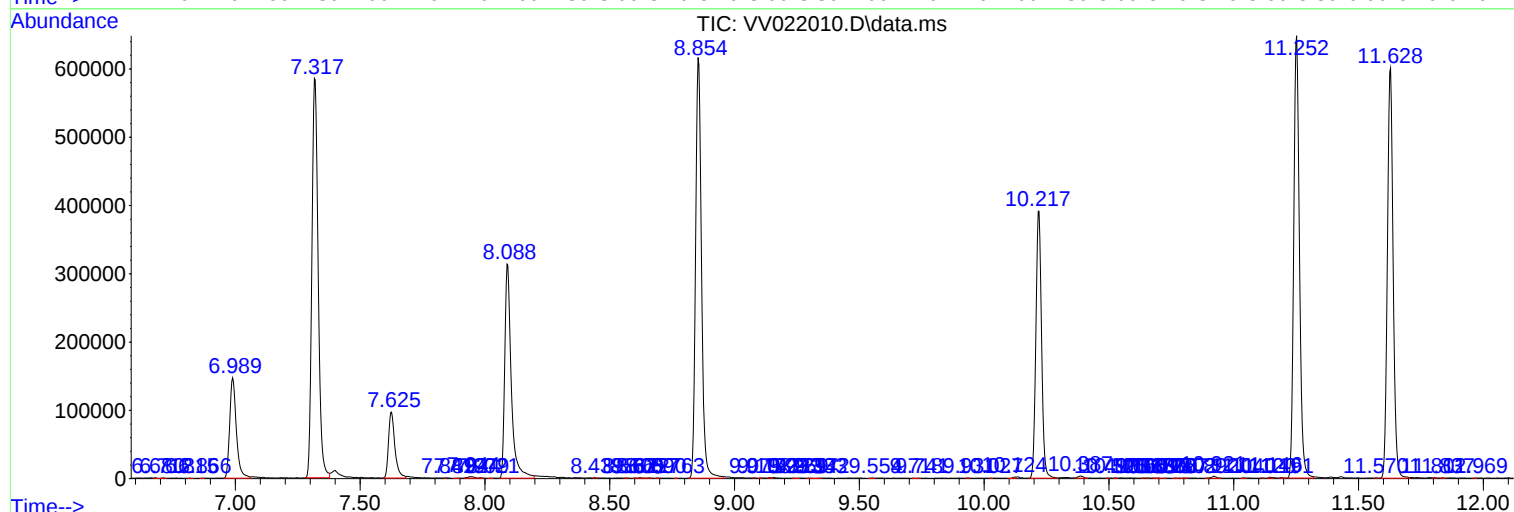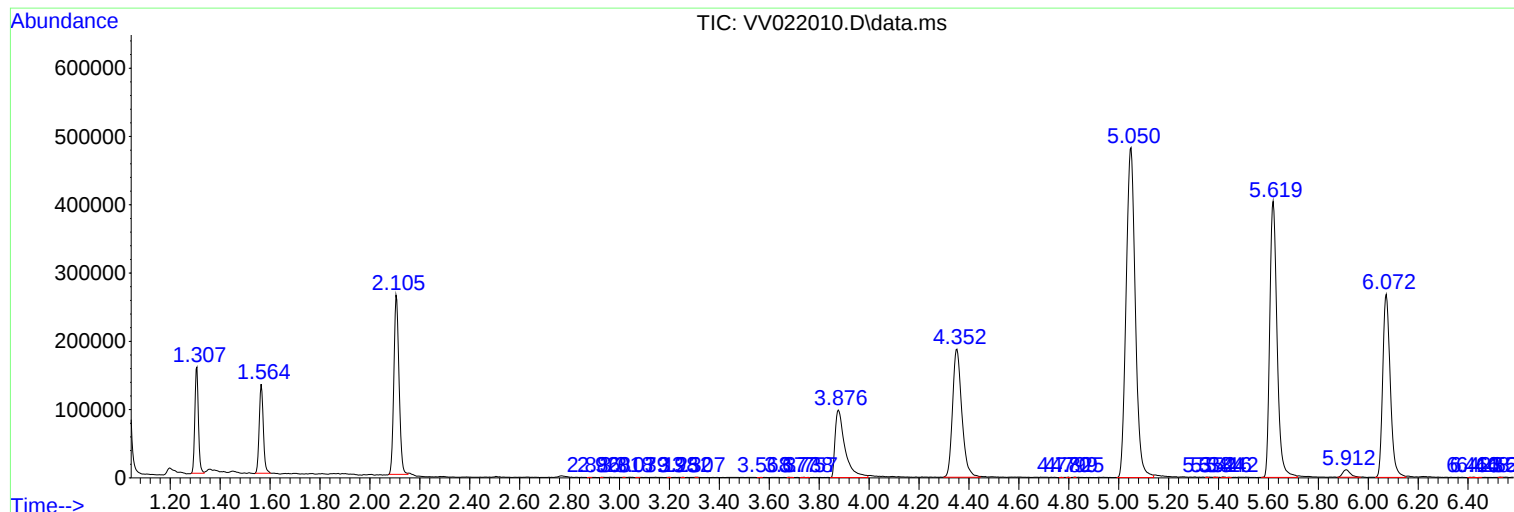

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022010.D
Acq On : 30 Aug 2021 17:52
Operator : SY/MD
Sample : M3566-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022010.D
Acq On : 30 Aug 2021 17:52
Operator : SY/MD
Sample : M3566-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKG9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
