

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022011.D
 Acq On : 30 Aug 2021 18:16
 Operator : SY/MD
 Sample : M3566-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	93	rBV	153695	151211	12.07%	1.528%
2	1.565	156	163	176	rVB	134798	155148	12.38%	1.568%
3	2.105	322	331	345	rBV	257250	365218	29.15%	3.691%
4	2.507	449	456	466	rBV6	2192	3618	0.29%	0.037%
5	2.587	479	481	484	rBV3	368	207	0.02%	0.002%
6	2.661	502	504	506	rBV	331	131	0.01%	0.001%
7	2.690	510	513	518	rBV3	398	353	0.03%	0.004%
8	2.754	525	533	534	rBV2	641	642	0.05%	0.006%
9	2.799	545	547	551	rBV	306	195	0.02%	0.002%
10	2.941	589	591	593	rBV	308	128	0.01%	0.001%
11	3.024	615	617	618	rBV	217	122	0.01%	0.001%
12	3.185	665	667	671	rBV2	315	185	0.01%	0.002%
13	3.249	684	687	691	rBV	219	142	0.01%	0.001%
14	3.275	691	695	698	rBV	322	319	0.03%	0.003%
15	3.339	713	715	719	rBV2	440	259	0.02%	0.003%
16	3.507	762	767	769	rBV	345	307	0.02%	0.003%
17	3.574	785	788	789	rBV	415	214	0.02%	0.002%
18	3.597	793	795	798	rVB2	352	192	0.02%	0.002%
19	3.635	805	807	811	rBV	222	202	0.02%	0.002%
20	3.751	839	843	846	rBV	322	259	0.02%	0.003%
21	3.880	873	883	917	rBV	101980	282978	22.58%	2.860%
22	4.352	1012	1030	1056	rBV	191821	496936	39.66%	5.022%
23	4.593	1101	1105	1111	rBV3	756	676	0.05%	0.007%
24	4.793	1164	1167	1168	rBV	392	205	0.02%	0.002%
25	4.883	1191	1195	1197	rBV3	353	251	0.02%	0.003%
26	4.931	1205	1210	1214	rBV3	347	365	0.03%	0.004%
27	5.047	1228	1246	1276	rBV2	492285	1253033	100.00%	12.663%
28	5.333	1332	1335	1337	rBV2	355	241	0.02%	0.002%
29	5.574	1404	1410	1411	rBV4	510	450	0.04%	0.005%
30	5.619	1412	1424	1449	rBV	415861	832077	66.41%	8.409%
31	5.912	1504	1515	1537	rVB3	11744	27583	2.20%	0.279%
32	5.989	1537	1539	1543	rVB3	651	335	0.03%	0.003%
33	6.011	1543	1546	1550	rBV3	394	278	0.02%	0.003%
34	6.072	1551	1565	1587	rBV	277840	567833	45.32%	5.738%
35	6.375	1657	1659	1663	rBV	368	232	0.02%	0.002%
36	6.439	1673	1679	1682	rBV3	361	394	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022011.D
 Acq On : 30 Aug 2021 18:16
 Operator : SY/MD
 Sample : M3566-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.490	1693	1695	1700	rBV	406	235	0.02%	0.002%
38	6.590	1723	1726	1728	rBV2	301	183	0.01%	0.002%
39	6.686	1753	1756	1760	rBV2	637	470	0.04%	0.005%
40	6.773	1781	1783	1786	rBV	343	225	0.02%	0.002%

41	6.838	1800	1803	1804	rBV	233	137	0.01%	0.001%
42	6.860	1807	1810	1813	rBV	276	180	0.01%	0.002%
43	6.892	1818	1820	1823	rVB2	316	173	0.01%	0.002%
44	6.940	1829	1835	1836	rBV	328	271	0.02%	0.003%
45	6.989	1839	1850	1867	rBV	147186	269368	21.50%	2.722%

46	7.268	1934	1937	1940	rBV4	492	403	0.03%	0.004%
47	7.317	1941	1952	1972	rBV	589036	1027855	82.03%	10.387%
48	7.625	2038	2048	2074	rBV	97943	175808	14.03%	1.777%
49	7.796	2099	2101	2105	rVB4	721	429	0.03%	0.004%
50	7.867	2119	2123	2125	rBV3	292	256	0.02%	0.003%

51	7.944	2136	2147	2157	rVB2	2972	4767	0.38%	0.048%
52	7.989	2157	2161	2164	rBB3	343	253	0.02%	0.003%
53	8.092	2182	2193	2227	rBV	327732	602340	48.07%	6.087%
54	8.420	2293	2295	2298	rVB2	454	248	0.02%	0.003%
55	8.493	2315	2318	2320	rBV2	404	300	0.02%	0.003%

56	8.606	2351	2353	2354	rBV2	416	204	0.02%	0.002%
57	8.715	2385	2387	2388	rBV2	439	192	0.02%	0.002%
58	8.854	2418	2430	2465	rBV	620927	1024183	81.74%	10.350%
59	9.333	2576	2579	2580	rBV	355	167	0.01%	0.002%
60	9.455	2614	2617	2621	rVB	423	269	0.02%	0.003%

61	9.477	2621	2624	2629	rBV2	188	152	0.01%	0.002%
62	9.583	2654	2657	2658	rBV2	377	192	0.02%	0.002%
63	9.622	2667	2669	2673	rVB3	268	151	0.01%	0.002%
64	9.686	2686	2689	2692	rVB	377	192	0.02%	0.002%
65	9.699	2692	2693	2696	rBV	206	123	0.01%	0.001%

66	9.735	2702	2704	2708	rVB2	372	188	0.02%	0.002%
67	9.802	2722	2725	2727	rBV2	269	178	0.01%	0.002%
68	9.844	2736	2738	2741	rVB	327	157	0.01%	0.002%
69	9.928	2762	2764	2765	rBV	365	164	0.01%	0.002%
70	10.127	2822	2826	2841	rVB6	2399	3986	0.32%	0.040%

71	10.217	2842	2854	2875	rBV	390960	630223	50.30%	6.369%
72	10.387	2899	2907	2916	rVB2	4439	6880	0.55%	0.070%
73	10.458	2924	2929	2936	rBV2	430	573	0.05%	0.006%
74	10.538	2951	2954	2959	rBV	515	499	0.04%	0.005%
75	10.574	2963	2965	2966	rBV	388	162	0.01%	0.002%

76	10.632	2981	2983	2988	rVB	541	295	0.02%	0.003%
----	--------	------	------	------	-----	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022011.D
 Acq On : 30 Aug 2021 18:16
 Operator : SY/MD
 Sample : M3566-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.741	3015	3017	3021	rVB2	326	159	0.01%	0.002%
78	10.837	3044	3047	3051	rVB2	468	336	0.03%	0.003%
79	10.921	3065	3073	3084	rVB6	2622	3802	0.30%	0.038%
80	11.156	3138	3146	3150	rBV6	1370	1963	0.16%	0.020%
81	11.191	3153	3157	3159	rBV2	387	348	0.03%	0.004%
82	11.252	3164	3176	3198	rBV	647359	1023358	81.67%	10.342%
83	11.532	3259	3263	3264	rBV2	400	235	0.02%	0.002%
84	11.548	3264	3268	3271	rBV4	688	711	0.06%	0.007%
85	11.628	3280	3293	3319	rBV	600411	964051	76.94%	9.743%
86	11.886	3371	3373	3377	rVB2	399	209	0.02%	0.002%
87	12.050	3422	3424	3427	rBV	343	232	0.02%	0.002%
88	12.172	3459	3462	3464	rBV	279	180	0.01%	0.002%
89	12.210	3471	3474	3475	rBV2	271	143	0.01%	0.001%
90	12.339	3512	3514	3515	rBV	531	248	0.02%	0.003%
91	12.384	3526	3528	3530	rBV	343	159	0.01%	0.002%
92	12.516	3566	3569	3570	rBV2	273	125	0.01%	0.001%
93	12.529	3571	3573	3575	rVV2	393	169	0.01%	0.002%
94	12.554	3580	3581	3583	rVB	522	186	0.01%	0.002%
95	12.661	3609	3614	3617	rVB3	556	531	0.04%	0.005%
96	12.715	3628	3631	3638	rBV2	434	386	0.03%	0.004%
97	12.744	3638	3640	3643	rVB	289	148	0.01%	0.001%
98	13.217	3783	3787	3788	rBV	431	264	0.02%	0.003%
99	13.516	3875	3880	3883	rBV3	956	925	0.07%	0.009%
100	13.796	3963	3967	3970	rVB3	492	346	0.03%	0.003%




Sum of corrected areas: 9895164

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022011.D
Acq On : 30 Aug 2021 18:16
Operator : SY/MD
Sample : M3566-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

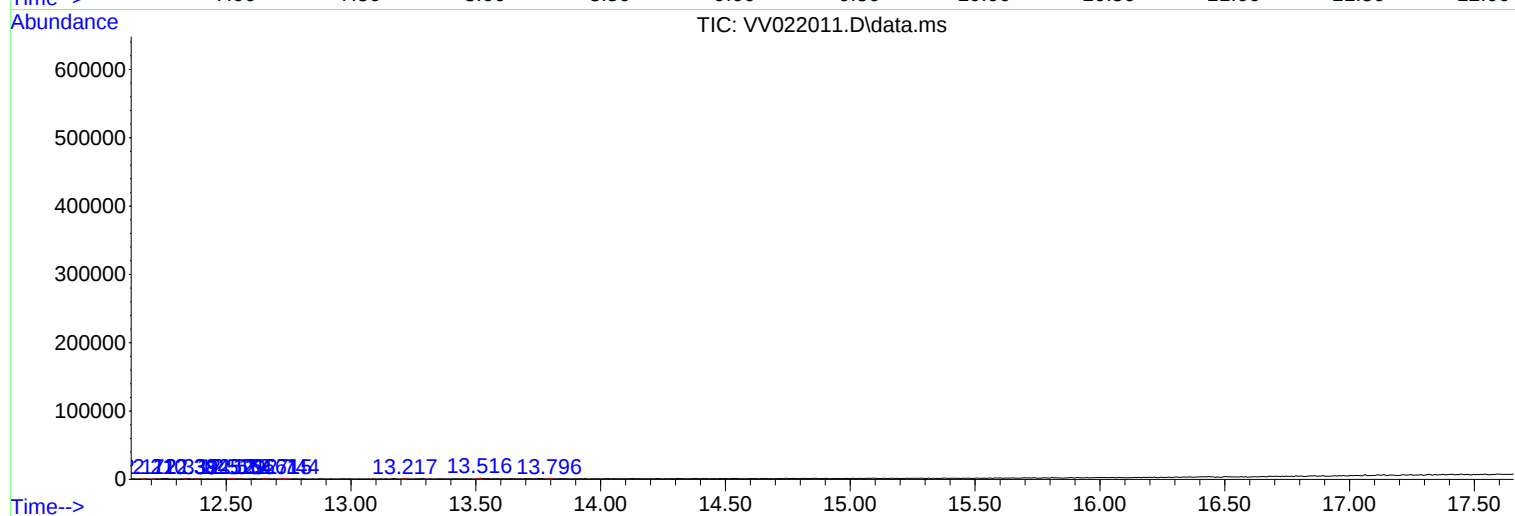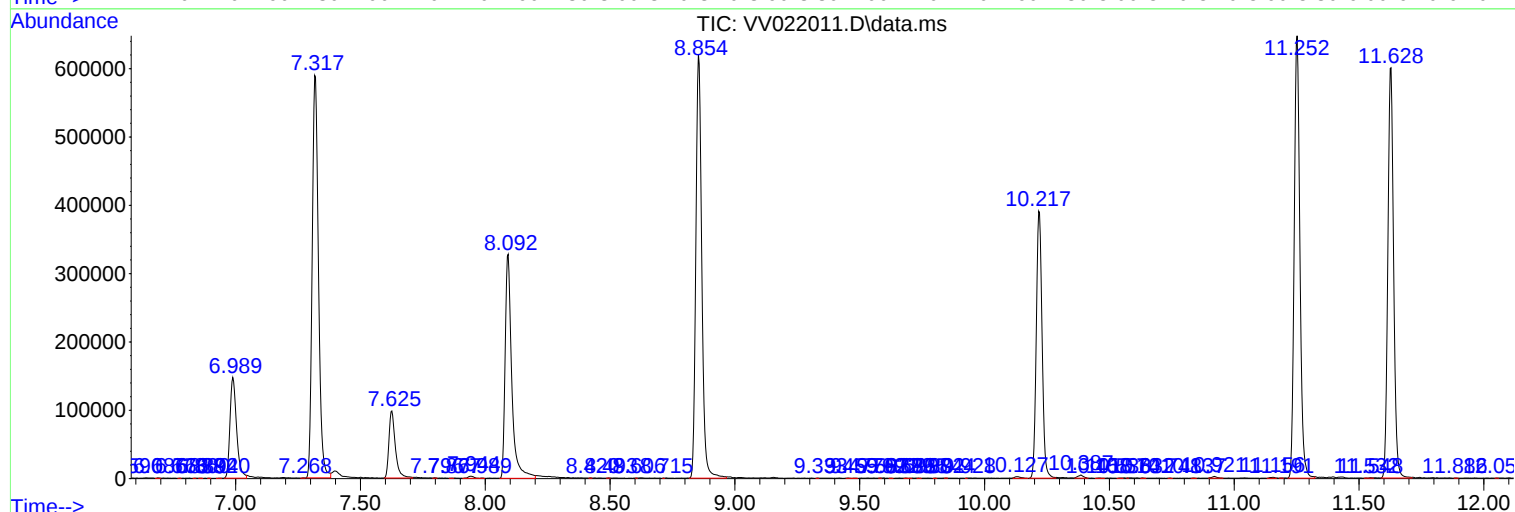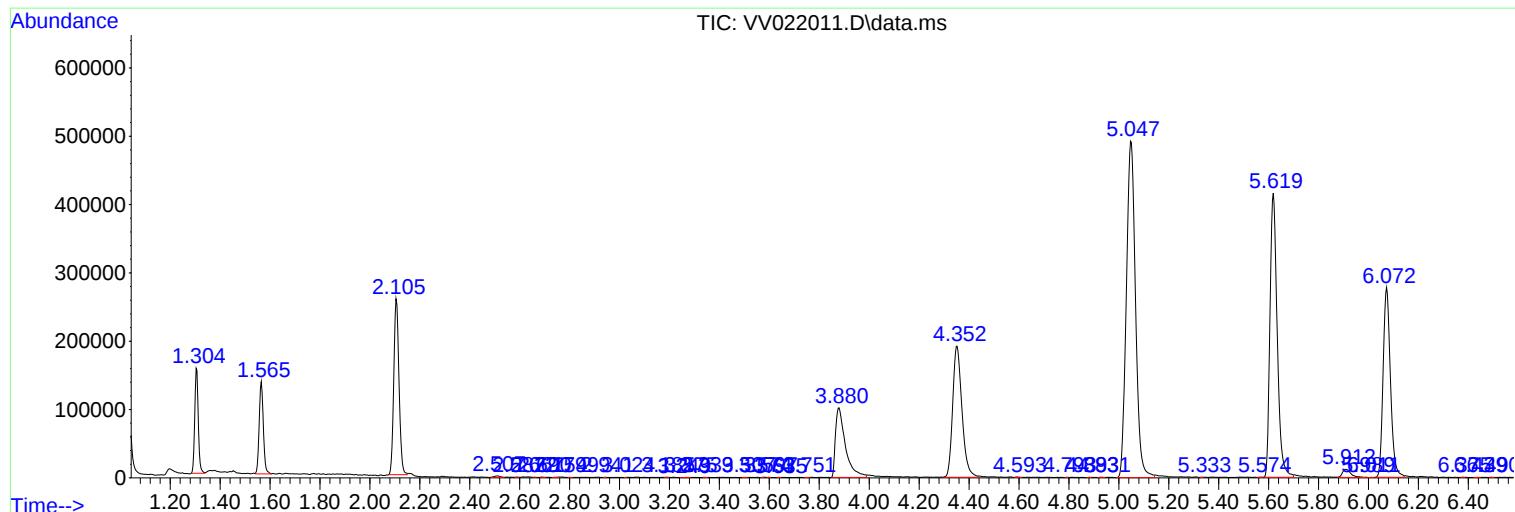

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022011.D
Acq On : 30 Aug 2021 18:16
Operator : SY/MD
Sample : M3566-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022011.D
Acq On : 30 Aug 2021 18:16
Operator : SY/MD
Sample : M3566-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
