

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022012.D
 Acq On : 30 Aug 2021 18:40
 Operator : SY/MD
 Sample : M3566-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022012.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rBV	154318	152137	12.24%	1.554%
2	1.565	156	163	175	rVB	131729	150536	12.11%	1.537%
3	2.105	322	331	358	rVB	262298	400597	32.22%	4.091%
4	2.413	424	427	429	rBV3	526	317	0.03%	0.003%
5	2.471	443	445	448	rBV2	361	210	0.02%	0.002%
6	2.507	449	456	460	rBV5	1317	1855	0.15%	0.019%
7	2.542	465	467	470	rBV2	405	269	0.02%	0.003%
8	2.745	527	530	531	rBV2	433	244	0.02%	0.002%
9	2.764	531	536	538	rBV5	2077	1995	0.16%	0.020%
10	3.166	659	661	665	rVB2	439	200	0.02%	0.002%
11	3.211	671	675	676	rBV2	399	275	0.02%	0.003%
12	3.233	680	682	685	rVV2	539	281	0.02%	0.003%
13	3.500	757	765	768	rBV2	270	346	0.03%	0.004%
14	3.526	770	773	777	rVV2	319	286	0.02%	0.003%
15	3.555	779	782	786	rBV2	532	329	0.03%	0.003%
16	3.667	812	817	819	rBV2	379	223	0.02%	0.002%
17	3.722	831	834	837	rBV2	327	195	0.02%	0.002%
18	3.876	873	882	919	rBV	98316	268294	21.58%	2.740%
19	4.352	1014	1030	1054	rBV	186048	488157	39.27%	4.985%
20	4.674	1129	1130	1133	rVB	585	189	0.02%	0.002%
21	4.732	1145	1148	1151	rVB3	337	219	0.02%	0.002%
22	4.751	1151	1154	1156	rBV2	395	277	0.02%	0.003%
23	4.770	1159	1160	1165	rBV3	448	277	0.02%	0.003%
24	4.941	1211	1213	1217	rBV3	303	253	0.02%	0.003%
25	5.047	1230	1246	1272	rBV2	489791	1243210	100.00%	12.695%
26	5.330	1330	1334	1341	rVB4	574	663	0.05%	0.007%
27	5.452	1368	1372	1375	rBV3	705	554	0.04%	0.006%
28	5.468	1375	1377	1380	rVV2	412	220	0.02%	0.002%
29	5.535	1394	1398	1400	rBV	345	289	0.02%	0.003%
30	5.558	1400	1405	1406	rBV	537	360	0.03%	0.004%
31	5.619	1409	1424	1451	rBV	400443	816850	65.70%	8.341%
32	5.908	1504	1514	1533	rBV3	12653	28284	2.28%	0.289%
33	6.072	1552	1565	1592	rBV	274171	563903	45.36%	5.758%
34	6.297	1632	1635	1640	rBV4	575	535	0.04%	0.005%
35	6.323	1640	1643	1647	rVB	381	261	0.02%	0.003%
36	6.397	1662	1666	1668	rBV5	535	341	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022012.D
 Acq On : 30 Aug 2021 18:40
 Operator : SY/MD
 Sample : M3566-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.449	1679	1682	1684	rBV	476	276	0.02%	0.003%
38	6.526	1703	1706	1708	rBV2	471	271	0.02%	0.003%
39	6.606	1724	1731	1734	rBV2	472	576	0.05%	0.006%
40	6.680	1752	1754	1762	rVB5	465	443	0.04%	0.005%
41	6.770	1780	1782	1788	rVB2	511	399	0.03%	0.004%
42	6.815	1792	1796	1800	rBV2	351	232	0.02%	0.002%
43	6.867	1807	1812	1814	rBV2	265	206	0.02%	0.002%
44	6.989	1837	1850	1870	rBV	147786	267589	21.52%	2.733%
45	7.191	1911	1913	1915	rBV2	630	377	0.03%	0.004%
46	7.236	1925	1927	1931	rBV2	376	253	0.02%	0.003%
47	7.275	1938	1939	1941	rBV2	390	217	0.02%	0.002%
48	7.317	1941	1952	1971	rBV	600792	1035607	83.30%	10.575%
49	7.625	2036	2048	2068	rBV2	101670	176018	14.16%	1.797%
50	7.783	2095	2097	2098	rBV	603	215	0.02%	0.002%
51	7.825	2108	2110	2115	rVB2	711	542	0.04%	0.006%
52	7.847	2115	2117	2120	rBV2	285	186	0.01%	0.002%
53	7.889	2128	2130	2134	rBB	359	208	0.02%	0.002%
54	7.944	2134	2147	2154	rBV5	1970	3869	0.31%	0.040%
55	8.018	2166	2170	2173	rBV	339	266	0.02%	0.003%
56	8.088	2182	2192	2224	rBV	310068	577741	46.47%	5.900%
57	8.500	2317	2320	2322	rBV2	551	413	0.03%	0.004%
58	8.567	2336	2341	2344	rBV4	534	405	0.03%	0.004%
59	8.760	2397	2401	2402	rBV	437	270	0.02%	0.003%
60	8.854	2417	2430	2452	rBV	613618	993852	79.94%	10.149%
61	9.088	2500	2503	2507	rBV3	741	645	0.05%	0.007%
62	9.133	2514	2517	2518	rBV	443	245	0.02%	0.003%
63	9.149	2520	2522	2530	rVV4	1188	1654	0.13%	0.017%
64	9.217	2538	2543	2546	rVB3	360	288	0.02%	0.003%
65	9.236	2546	2549	2553	rVB3	376	289	0.02%	0.003%
66	9.275	2556	2561	2565	rBV3	267	254	0.02%	0.003%
67	9.391	2594	2597	2602	rBV2	299	193	0.02%	0.002%
68	9.413	2602	2604	2610	rVB2	458	268	0.02%	0.003%
69	9.448	2610	2615	2617	rBV2	380	259	0.02%	0.003%
70	9.551	2642	2647	2652	rBV2	570	582	0.05%	0.006%
71	9.622	2664	2669	2672	rBV	335	374	0.03%	0.004%
72	9.680	2684	2687	2690	rBV2	459	307	0.02%	0.003%
73	9.841	2733	2737	2738	rBV	312	213	0.02%	0.002%
74	9.937	2763	2767	2775	rVB	718	515	0.04%	0.005%
75	10.127	2819	2826	2836	rBV5	2545	3931	0.32%	0.040%
76	10.217	2842	2854	2876	rBV	386605	612969	49.31%	6.259%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022012.D
 Acq On : 30 Aug 2021 18:40
 Operator : SY/MD
 Sample : M3566-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.384	2899	2906	2919	rVB4	2889	4924	0.40%	0.050%
78	10.487	2936	2938	2945	rVB3	443	350	0.03%	0.004%
79	10.593	2969	2971	2973	rBV3	328	220	0.02%	0.002%
80	10.664	2990	2993	2995	rBV2	565	285	0.02%	0.003%
81	10.821	3039	3042	3044	rBV2	426	197	0.02%	0.002%
82	10.921	3065	3073	3082	rVB4	2597	3878	0.31%	0.040%
83	11.146	3139	3143	3146	rBV3	1099	941	0.08%	0.010%
84	11.252	3164	3176	3197	rBV	648983	1008795	81.14%	10.302%
85	11.625	3280	3292	3314	rBV	609083	962030	77.38%	9.824%
86	12.037	3417	3420	3423	rVB2	453	358	0.03%	0.004%
87	12.095	3436	3438	3440	rVV	610	359	0.03%	0.004%
88	12.323	3505	3509	3510	rBV	369	238	0.02%	0.002%
89	12.545	3573	3578	3580	rBV	485	397	0.03%	0.004%
90	12.603	3593	3596	3597	rBV2	470	243	0.02%	0.002%
91	13.001	3718	3720	3723	rVB	519	223	0.02%	0.002%
92	13.249	3795	3797	3799	rBV	379	221	0.02%	0.002%
93	13.265	3799	3802	3803	rBV2	368	187	0.02%	0.002%
94	13.313	3814	3817	3820	rBV	465	278	0.02%	0.003%
95	13.493	3871	3873	3875	rBV2	486	256	0.02%	0.003%
96	13.831	3975	3978	3983	rVB3	544	413	0.03%	0.004%
97	13.972	4020	4022	4023	rBV	582	264	0.02%	0.003%
98	14.191	4087	4090	4091	rBV	330	211	0.02%	0.002%
99	14.294	4120	4122	4125	rBV2	394	256	0.02%	0.003%
100	15.175	4393	4396	4398	rBV2	468	262	0.02%	0.003%




Sum of corrected areas: 9792634

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022012.D
Acq On : 30 Aug 2021 18:40
Operator : SY/MD
Sample : M3566-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

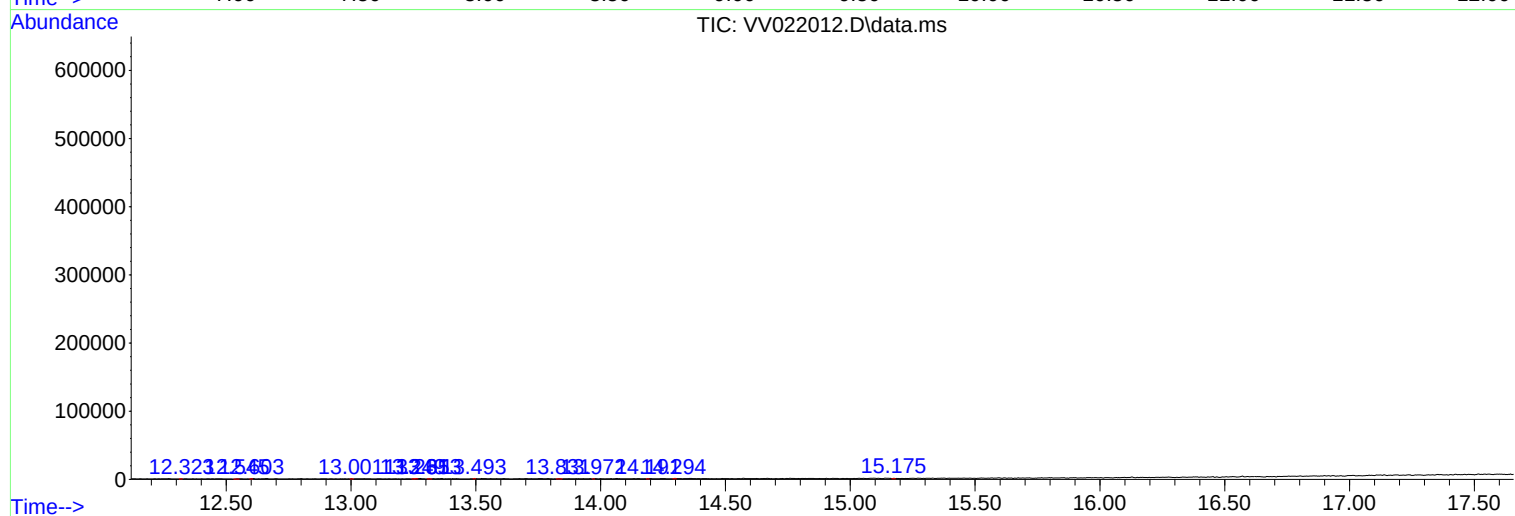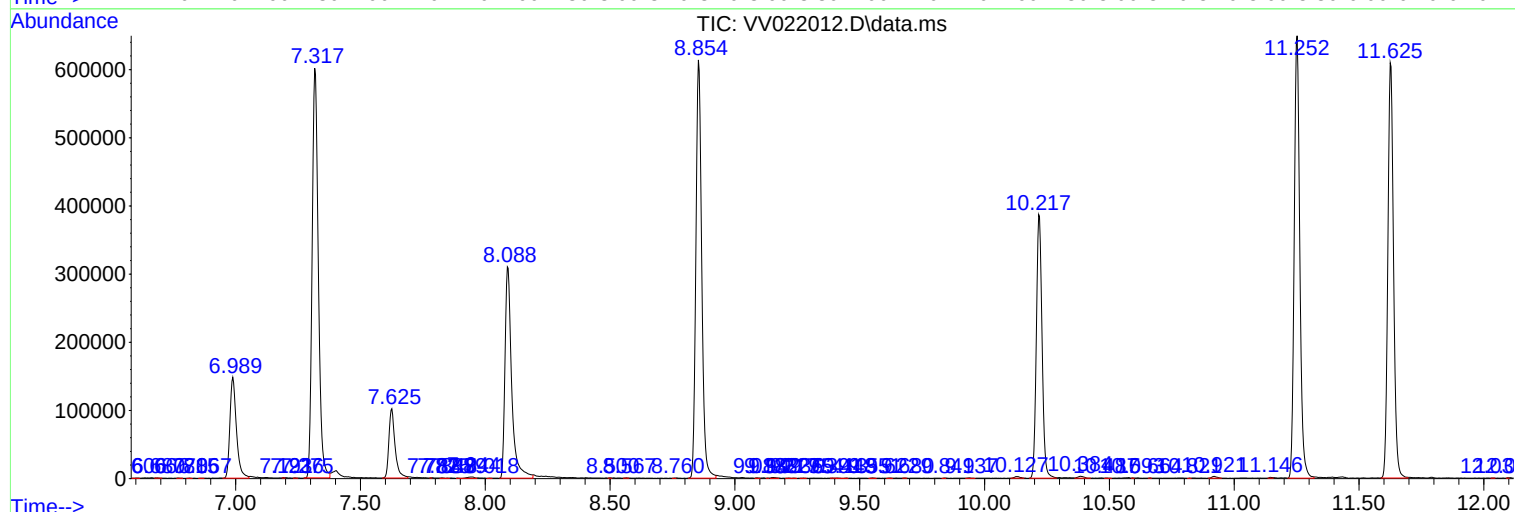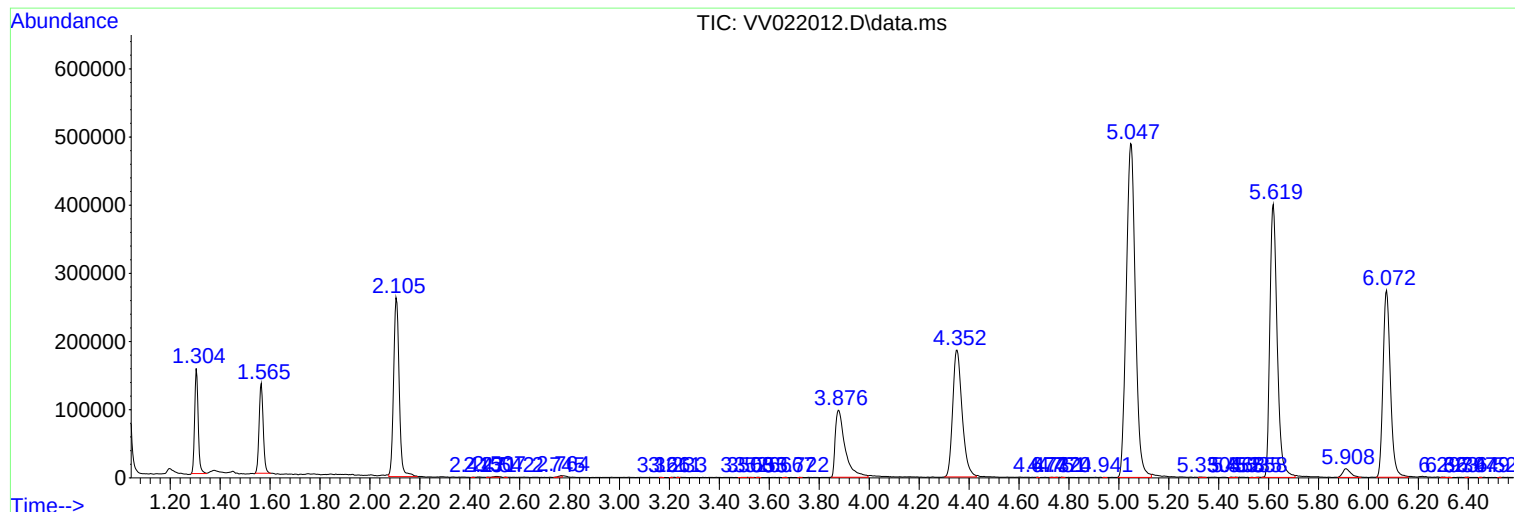

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022012.D
Acq On : 30 Aug 2021 18:40
Operator : SY/MD
Sample : M3566-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022012.D
Acq On : 30 Aug 2021 18:40
Operator : SY/MD
Sample : M3566-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
