

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V083021\
 Data File : VV022013.D
 Acq On : 30 Aug 2021 19:04
 Operator : SY/MD
 Sample : M3566-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022013.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rBV	148603	147618	12.21%	1.539%
2	1.564	157	163	178	rVB	129270	147283	12.18%	1.536%
3	2.105	323	331	346	rVB	258630	374328	30.95%	3.904%
4	2.439	430	435	439	rBV4	1016	1111	0.09%	0.012%
5	2.542	465	467	470	rBV2	340	202	0.02%	0.002%
6	2.690	510	513	515	rBV	302	234	0.02%	0.002%
7	2.770	524	538	549	rBV3	5253	11618	0.96%	0.121%
8	2.844	559	561	563	rBV3	298	179	0.01%	0.002%
9	2.979	600	603	607	rBV2	460	319	0.03%	0.003%
10	3.018	613	615	617	rBV	248	131	0.01%	0.001%
11	3.220	676	678	681	rVB	420	192	0.02%	0.002%
12	3.243	681	685	689	rBV2	255	194	0.02%	0.002%
13	3.288	697	699	704	rVV2	234	181	0.01%	0.002%
14	3.310	704	706	709	rVB2	303	163	0.01%	0.002%
15	3.452	746	750	753	rBV2	353	372	0.03%	0.004%
16	3.484	757	760	763	rBV2	521	375	0.03%	0.004%
17	3.593	791	794	797	rBV2	253	166	0.01%	0.002%
18	3.670	816	818	824	rVB	241	137	0.01%	0.001%
19	3.703	824	828	833	rVB	333	289	0.02%	0.003%
20	3.725	833	835	838	rBV	197	130	0.01%	0.001%
21	3.825	860	866	870	rVB4	425	367	0.03%	0.004%
22	3.876	871	882	915	rBV	105285	279052	23.07%	2.910%
23	4.240	993	995	998	rBV3	520	314	0.03%	0.003%
24	4.352	1015	1030	1060	rBV	187719	472538	39.07%	4.928%
25	4.654	1120	1124	1125	rBV2	388	255	0.02%	0.003%
26	4.828	1173	1178	1183	rBV3	602	600	0.05%	0.006%
27	4.867	1187	1190	1194	rVB2	327	246	0.02%	0.003%
28	5.047	1229	1246	1275	rBV2	474297	1209474	100.00%	12.613%
29	5.522	1392	1394	1396	rBV2	407	184	0.02%	0.002%
30	5.558	1402	1405	1408	rBV2	421	336	0.03%	0.004%
31	5.574	1408	1410	1411	rBV	316	134	0.01%	0.001%
32	5.619	1411	1424	1453	rVV	396007	797680	65.95%	8.319%
33	5.911	1505	1515	1527	rBV4	8150	16326	1.35%	0.170%
34	6.011	1544	1546	1548	rBV	277	166	0.01%	0.002%
35	6.072	1550	1565	1592	rVV	262874	550254	45.50%	5.738%
36	6.275	1624	1628	1632	rVB4	1128	904	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022013.D
 Acq On : 30 Aug 2021 19:04
 Operator : SY/MD
 Sample : M3566-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.294	1632	1634	1637	rBV3	493	196	0.02%	0.002%
38	6.352	1648	1652	1655	rBV2	370	303	0.03%	0.003%
39	6.371	1655	1658	1660	rBV	547	360	0.03%	0.004%
40	6.407	1666	1669	1674	rVB3	603	543	0.04%	0.006%
41	6.513	1697	1702	1704	rBV2	200	142	0.01%	0.001%
42	6.532	1704	1708	1709	rBV2	380	269	0.02%	0.003%
43	6.918	1825	1828	1830	rVB2	337	167	0.01%	0.002%
44	6.940	1830	1835	1837	rBV2	248	285	0.02%	0.003%
45	6.989	1839	1850	1878	rVV	142278	260555	21.54%	2.717%
46	7.149	1898	1900	1904	rBV3	623	411	0.03%	0.004%
47	7.201	1912	1916	1918	rBV3	431	362	0.03%	0.004%
48	7.317	1940	1952	1971	rBV	573689	1001097	82.77%	10.440%
49	7.625	2038	2048	2072	rBV	95436	168917	13.97%	1.762%
50	7.815	2105	2107	2109	rBV	334	167	0.01%	0.002%
51	7.828	2109	2111	2116	rVB4	403	339	0.03%	0.004%
52	7.882	2123	2128	2131	rVB2	373	360	0.03%	0.004%
53	7.902	2131	2134	2135	rBV	342	155	0.01%	0.002%
54	7.940	2140	2146	2158	rVB5	1955	3143	0.26%	0.033%
55	8.040	2175	2177	2181	rVB2	352	215	0.02%	0.002%
56	8.088	2181	2192	2228	rBV	315841	581237	48.06%	6.062%
57	8.596	2347	2350	2354	rBV3	381	326	0.03%	0.003%
58	8.641	2361	2364	2368	rVB2	325	251	0.02%	0.003%
59	8.657	2368	2369	2375	rVB	367	202	0.02%	0.002%
60	8.693	2378	2380	2383	rBV2	334	204	0.02%	0.002%
61	8.747	2395	2397	2399	rBV	348	150	0.01%	0.002%
62	8.853	2419	2430	2450	rBV	603765	976917	80.77%	10.188%
63	9.111	2505	2510	2512	rBV2	315	248	0.02%	0.003%
64	9.252	2551	2554	2558	rBV2	223	168	0.01%	0.002%
65	9.313	2570	2573	2575	rBV	294	176	0.01%	0.002%
66	9.648	2673	2677	2679	rVB	319	164	0.01%	0.002%
67	9.763	2711	2713	2719	rVB2	429	290	0.02%	0.003%
68	9.860	2740	2743	2748	rVB2	515	367	0.03%	0.004%
69	10.091	2813	2815	2819	rVB	253	129	0.01%	0.001%
70	10.130	2819	2827	2838	rBV5	1985	3278	0.27%	0.034%
71	10.175	2838	2841	2843	rVB	440	219	0.02%	0.002%
72	10.220	2843	2855	2877	rBV	387199	615122	50.86%	6.415%
73	10.387	2899	2907	2916	rVB5	2378	3488	0.29%	0.036%
74	10.455	2925	2928	2931	rVB2	321	165	0.01%	0.002%
75	10.474	2931	2934	2935	rBV	267	153	0.01%	0.002%
76	10.497	2938	2941	2944	rBV2	330	281	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022013.D
 Acq On : 30 Aug 2021 19:04
 Operator : SY/MD
 Sample : M3566-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKH3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.545	2951	2956	2960	rBV4	610	644	0.05%	0.007%
78	10.638	2982	2985	2987	rBV	378	198	0.02%	0.002%
79	10.667	2992	2994	2999	rVB2	501	280	0.02%	0.003%
80	10.744	3014	3018	3022	rBV3	583	497	0.04%	0.005%
81	10.783	3025	3030	3034	rBV2	322	333	0.03%	0.003%
82	10.844	3043	3049	3050	rBV2	298	305	0.03%	0.003%
83	10.876	3056	3059	3062	rBV2	375	172	0.01%	0.002%
84	10.963	3084	3086	3092	rVB	368	220	0.02%	0.002%
85	11.014	3100	3102	3105	rBV2	271	172	0.01%	0.002%
86	11.040	3105	3110	3114	rVB3	636	670	0.06%	0.007%
87	11.059	3114	3116	3118	rBV	320	167	0.01%	0.002%
88	11.146	3138	3143	3146	rBV3	1008	1010	0.08%	0.011%
89	11.188	3153	3156	3157	rBV3	535	260	0.02%	0.003%
90	11.252	3163	3176	3198	rBV	642423	1001817	82.83%	10.448%
91	11.625	3280	3292	3319	rBV	592048	943728	78.03%	9.842%
92	11.918	3381	3383	3385	rBV2	273	157	0.01%	0.002%
93	12.101	3435	3440	3444	rBV3	613	655	0.05%	0.007%
94	12.349	3514	3517	3518	rBV3	230	137	0.01%	0.001%
95	12.358	3518	3520	3522	rBV	421	201	0.02%	0.002%
96	13.107	3750	3753	3756	rBV2	355	293	0.02%	0.003%
97	13.406	3843	3846	3849	rVB2	634	393	0.03%	0.004%
98	13.490	3870	3872	3874	rBV	460	244	0.02%	0.003%
99	13.747	3951	3952	3954	rBV	668	302	0.02%	0.003%
100	13.850	3979	3984	3987	rBV2	438	513	0.04%	0.005%



Sum of corrected areas: 9588941

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022013.D
Acq On : 30 Aug 2021 19:04
Operator : SY/MD
Sample : M3566-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

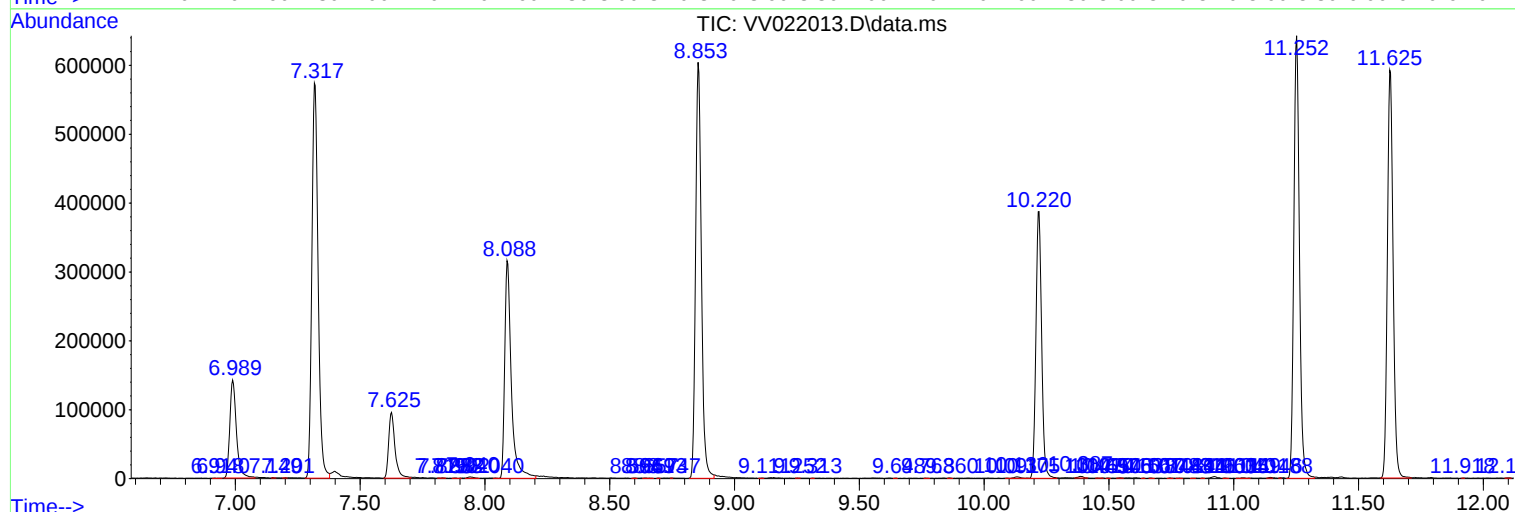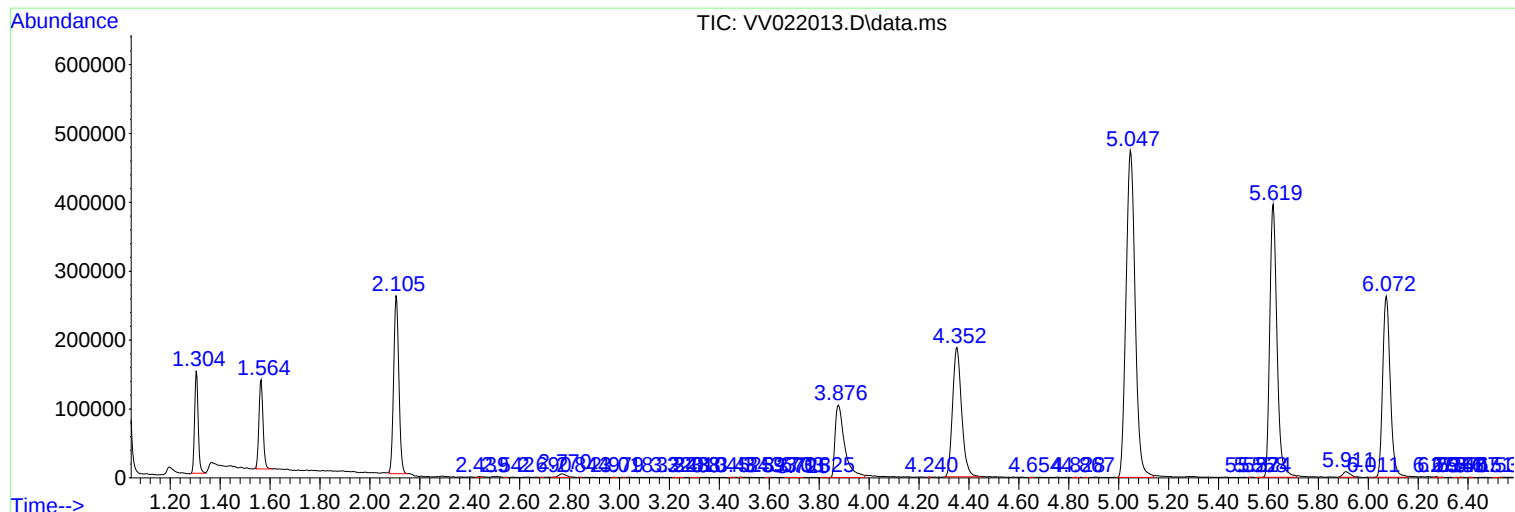

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022013.D
Acq On : 30 Aug 2021 19:04
Operator : SY/MD
Sample : M3566-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022013.D
Acq On : 30 Aug 2021 19:04
Operator : SY/MD
Sample : M3566-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKH3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
