

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022016.D
 Acq On : 30 Aug 2021 20:41
 Operator : SY/MD
 Sample : VV0830WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK244

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022016.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	163208	157963	12.64%	1.612%
2	1.565	156	163	178	rVB	130578	153467	12.28%	1.566%
3	2.105	321	331	345	rBV	264586	385598	30.86%	3.935%
4	2.507	449	456	467	rVB4	5246	8684	0.70%	0.089%
5	2.667	503	506	508	rBV	343	177	0.01%	0.002%
6	2.751	528	532	534	rBV3	699	536	0.04%	0.005%
7	2.828	553	556	561	rVB2	522	309	0.02%	0.003%
8	2.876	567	571	573	rBV2	309	272	0.02%	0.003%
9	2.902	576	579	584	rBV3	368	291	0.02%	0.003%
10	2.950	589	594	599	rBV2	343	398	0.03%	0.004%
11	3.294	698	701	703	rBV	349	221	0.02%	0.002%
12	3.336	711	714	717	rVB	341	178	0.01%	0.002%
13	3.426	738	742	746	rBV2	207	220	0.02%	0.002%
14	3.526	766	773	778	rBV4	451	497	0.04%	0.005%
15	3.619	798	802	806	rVB	283	208	0.02%	0.002%
16	3.664	813	816	819	rBV	251	233	0.02%	0.002%
17	3.687	819	823	827	rVB3	443	388	0.03%	0.004%
18	3.876	863	882	919	rBV	106562	288411	23.08%	2.943%
19	4.352	1013	1030	1058	rBV	187065	489001	39.14%	4.990%
20	4.828	1176	1178	1182	rBV2	289	205	0.02%	0.002%
21	4.880	1191	1194	1199	rVB3	423	284	0.02%	0.003%
22	4.908	1199	1203	1204	rBV2	532	317	0.03%	0.003%
23	5.047	1229	1246	1275	rBV2	488869	1249424	100.00%	12.751%
24	5.336	1334	1336	1338	rBV	452	213	0.02%	0.002%
25	5.436	1363	1367	1369	rBV2	468	360	0.03%	0.004%
26	5.471	1375	1378	1380	rBV2	283	195	0.02%	0.002%
27	5.577	1407	1411	1412	rBV	345	249	0.02%	0.003%
28	5.619	1412	1424	1458	rVV	400679	812723	65.05%	8.294%
29	5.908	1503	1514	1530	rBV2	16722	36951	2.96%	0.377%
30	6.072	1551	1565	1589	rBV	274499	563810	45.13%	5.754%
31	6.314	1638	1640	1645	rVB	515	277	0.02%	0.003%
32	6.359	1649	1654	1658	rBV4	634	479	0.04%	0.005%
33	6.442	1677	1680	1681	rBV	427	187	0.01%	0.002%
34	6.555	1713	1715	1718	rBV3	380	213	0.02%	0.002%
35	6.703	1758	1761	1763	rVB	424	228	0.02%	0.002%
36	6.728	1767	1769	1773	rVB2	557	288	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022016.D
 Acq On : 30 Aug 2021 20:41
 Operator : SY/MD
 Sample : VV0830WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK244

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.812	1793	1795	1798	rBV2	302	221	0.02%	0.002%
38	6.989	1838	1850	1872	rBV	142216	265041	21.21%	2.705%
39	7.233	1924	1926	1928	rBV	481	187	0.01%	0.002%
40	7.317	1941	1952	1972	rBV	593369	1030898	82.51%	10.520%
41	7.625	2038	2048	2073	rBV	96906	172813	13.83%	1.764%
42	7.992	2155	2162	2165	rVB6	754	839	0.07%	0.009%
43	8.088	2182	2192	2222	rBV	316170	590222	47.24%	6.023%
44	8.400	2287	2289	2294	rBV4	382	198	0.02%	0.002%
45	8.484	2314	2315	2318	rBV	355	187	0.01%	0.002%
46	8.555	2333	2337	2339	rBV3	334	256	0.02%	0.003%
47	8.600	2349	2351	2354	rBV2	445	221	0.02%	0.002%
48	8.619	2354	2357	2360	rBV3	502	346	0.03%	0.004%
49	8.773	2403	2405	2411	rBV2	370	301	0.02%	0.003%
50	8.854	2419	2430	2453	rBV	600555	985862	78.91%	10.061%
51	9.117	2509	2512	2516	rVB2	470	268	0.02%	0.003%
52	9.153	2516	2523	2527	rBV4	1164	1486	0.12%	0.015%
53	9.233	2544	2548	2554	rVB3	269	297	0.02%	0.003%
54	9.371	2588	2591	2594	rBV2	274	236	0.02%	0.002%
55	9.487	2621	2627	2629	rBV2	568	388	0.03%	0.004%
56	9.522	2634	2638	2642	rBV2	236	207	0.02%	0.002%
57	9.548	2642	2646	2648	rBV3	389	367	0.03%	0.004%
58	9.686	2685	2689	2691	rBV2	413	247	0.02%	0.003%
59	9.735	2700	2704	2707	rVB2	440	348	0.03%	0.004%
60	9.757	2707	2711	2714	rBV	234	208	0.02%	0.002%
61	9.850	2737	2740	2744	rBV	359	259	0.02%	0.003%
62	9.944	2766	2769	2772	rBV3	849	439	0.04%	0.004%
63	10.082	2809	2812	2816	rBV2	275	252	0.02%	0.003%
64	10.127	2820	2826	2838	rVB4	2471	3830	0.31%	0.039%
65	10.217	2842	2854	2881	rBV	379728	607012	48.58%	6.195%
66	10.313	2882	2884	2885	rBV	660	307	0.02%	0.003%
67	10.387	2903	2907	2914	rVB3	907	836	0.07%	0.009%
68	10.471	2927	2933	2935	rBV3	478	501	0.04%	0.005%
69	10.535	2951	2953	2954	rBV	560	256	0.02%	0.003%
70	10.654	2987	2990	2992	rBV2	604	324	0.03%	0.003%
71	10.802	3029	3036	3038	rBV3	315	355	0.03%	0.004%
72	10.924	3064	3074	3080	rBV4	2752	4604	0.37%	0.047%
73	10.989	3089	3094	3096	rBV2	326	243	0.02%	0.002%
74	11.143	3137	3142	3150	rVB6	1048	1576	0.13%	0.016%
75	11.198	3153	3159	3164	rVB2	960	1054	0.08%	0.011%
76	11.252	3164	3176	3196	rBV	644964	996472	79.75%	10.169%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022016.D
 Acq On : 30 Aug 2021 20:41
 Operator : SY/MD
 Sample : VV0830WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK244

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	11.471	3242	3244	3248	rVB2	386	233	0.02%	0.002%
78	11.625	3281	3292	3314	rBV	606176	961091	76.92%	9.808%
79	11.786	3338	3342	3343	rBV3	766	512	0.04%	0.005%
80	11.889	3372	3374	3376	rBV2	433	196	0.02%	0.002%
81	12.082	3429	3434	3436	rBV3	501	392	0.03%	0.004%
82	12.133	3446	3450	3453	rBV2	375	327	0.03%	0.003%
83	12.156	3455	3457	3460	rBV3	307	191	0.02%	0.002%
84	12.355	3515	3519	3525	rVB	363	361	0.03%	0.004%
85	12.458	3546	3551	3555	rBV2	461	495	0.04%	0.005%
86	12.529	3571	3573	3575	rBV	461	234	0.02%	0.002%
87	12.574	3582	3587	3588	rBV	382	230	0.02%	0.002%
88	12.654	3607	3612	3620	rBV4	1269	1528	0.12%	0.016%
89	12.905	3686	3690	3693	rBV2	290	225	0.02%	0.002%
90	13.143	3761	3764	3767	rBV2	389	226	0.02%	0.002%
91	13.217	3785	3787	3792	rBV2	331	214	0.02%	0.002%
92	13.271	3797	3804	3806	rBV4	1742	1710	0.14%	0.017%
93	13.371	3831	3835	3836	rBV2	360	251	0.02%	0.003%
94	13.406	3843	3846	3850	rBV2	455	300	0.02%	0.003%
95	13.455	3858	3861	3864	rBV2	378	278	0.02%	0.003%
96	13.519	3874	3881	3886	rBV4	2063	2842	0.23%	0.029%
97	13.628	3911	3915	3916	rBV	365	243	0.02%	0.002%
98	13.725	3942	3945	3948	rVB2	378	237	0.02%	0.002%
99	13.754	3948	3954	3961	rBV3	1779	2963	0.24%	0.030%
100	14.519	4189	4192	4193	rBV2	485	315	0.03%	0.003%




Sum of corrected areas: 9799013

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022016.D
Acq On : 30 Aug 2021 20:41
Operator : SY/MD
Sample : VV0830WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

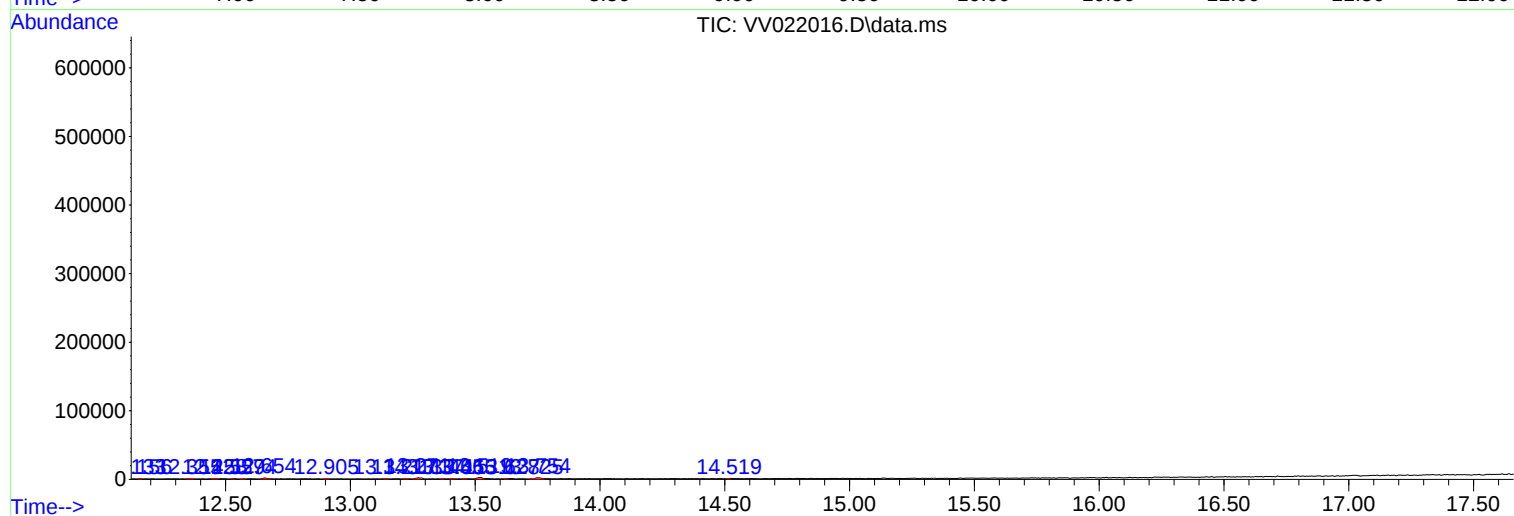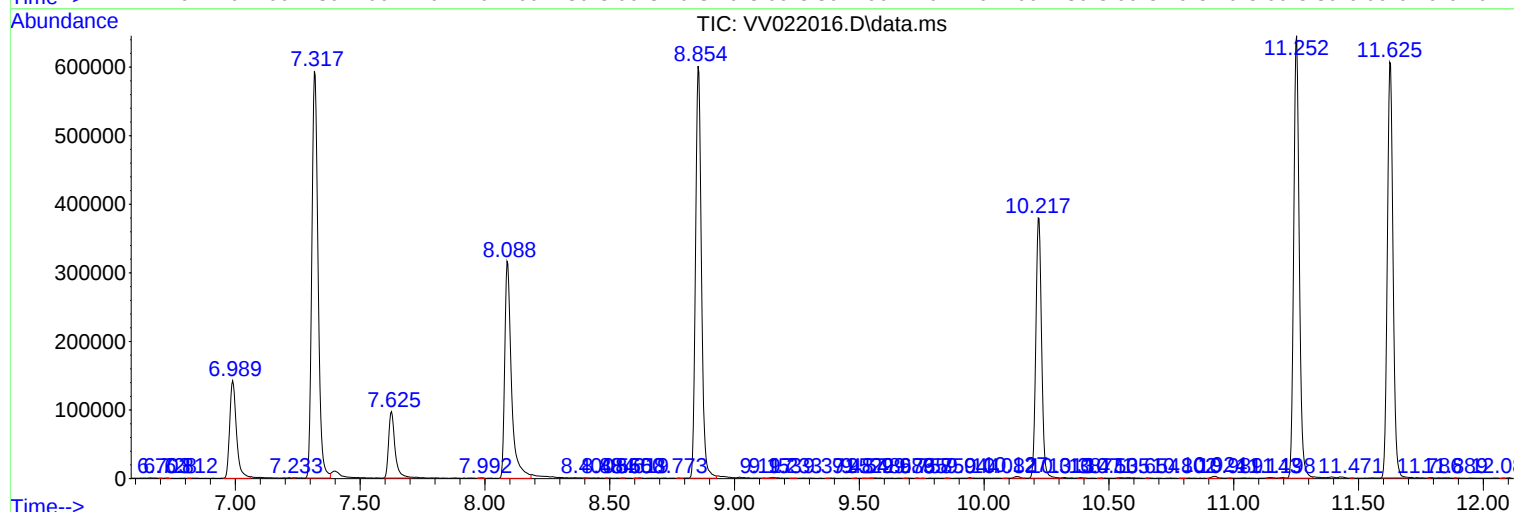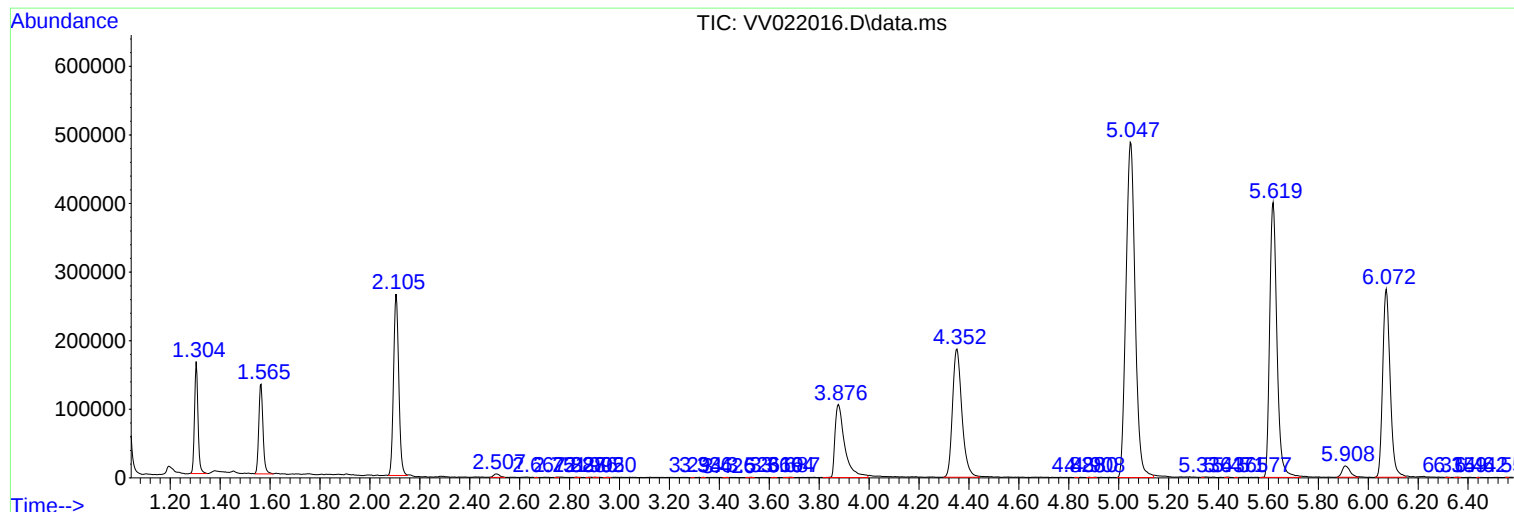

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022016.D
Acq On : 30 Aug 2021 20:41
Operator : SY/MD
Sample : VV0830WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022016.D
Acq On : 30 Aug 2021 20:41
Operator : SY/MD
Sample : VV0830WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK244

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
