

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022018.D
 Acq On : 30 Aug 2021 21:29
 Operator : SY/MD
 Sample : M3566-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	92	rBV	148600	145701	12.10%	1.533%
2	1.565	156	163	179	rVB	125249	146270	12.14%	1.539%
3	2.105	322	331	345	rBV	247752	358675	29.78%	3.773%
4	2.500	450	454	455	rBV2	1247	774	0.06%	0.008%
5	2.600	483	485	487	rBV	442	299	0.02%	0.003%
6	2.957	592	596	605	rBV3	570	758	0.06%	0.008%
7	3.118	642	646	648	rBV	285	214	0.02%	0.002%
8	3.201	669	672	674	rBV3	365	197	0.02%	0.002%
9	3.330	709	712	714	rVV2	482	334	0.03%	0.004%
10	3.355	718	720	726	rVV2	477	389	0.03%	0.004%
11	3.394	728	732	739	rVB2	600	655	0.05%	0.007%
12	3.426	739	742	745	rBV2	215	188	0.02%	0.002%
13	3.536	773	776	782	rVB2	385	339	0.03%	0.004%
14	3.574	782	788	791	rBV2	183	193	0.02%	0.002%
15	3.606	796	798	803	rVB2	438	318	0.03%	0.003%
16	3.687	820	823	826	rVB	313	176	0.01%	0.002%
17	3.876	872	882	922	rBV	102374	275202	22.85%	2.895%
18	4.352	1014	1030	1064	rBV	181909	471801	39.17%	4.963%
19	4.613	1108	1111	1112	rBV2	454	216	0.02%	0.002%
20	4.825	1175	1177	1181	rBV2	472	260	0.02%	0.003%
21	4.908	1202	1203	1208	rBV	247	200	0.02%	0.002%
22	5.047	1229	1246	1276	rBV2	469128	1204563	100.00%	12.672%
23	5.317	1326	1330	1333	rVB3	607	514	0.04%	0.005%
24	5.343	1336	1338	1341	rVB3	712	349	0.03%	0.004%
25	5.378	1347	1349	1351	rBV	438	211	0.02%	0.002%
26	5.494	1382	1385	1389	rVB4	662	322	0.03%	0.003%
27	5.513	1389	1391	1395	rVB2	437	213	0.02%	0.002%
28	5.552	1397	1403	1406	rBV5	854	818	0.07%	0.009%
29	5.619	1411	1424	1449	rBV	393622	797717	66.22%	8.392%
30	5.908	1504	1514	1531	rBV2	17653	38655	3.21%	0.407%
31	6.072	1550	1565	1589	rBV	263338	543999	45.16%	5.723%
32	6.272	1625	1627	1630	rVB2	451	260	0.02%	0.003%
33	6.304	1635	1637	1642	rVB3	472	357	0.03%	0.004%
34	6.362	1651	1655	1657	rBV	560	421	0.03%	0.004%
35	6.426	1670	1675	1677	rBV3	439	286	0.02%	0.003%
36	6.436	1677	1678	1681	rVB2	455	186	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022018.D
 Acq On : 30 Aug 2021 21:29
 Operator : SY/MD
 Sample : M3566-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.732	1767	1770	1773	rVB	483	293	0.02%	0.003%
38	6.751	1773	1776	1779	rBV3	333	226	0.02%	0.002%
39	6.783	1785	1786	1791	rVB2	398	210	0.02%	0.002%
40	6.889	1815	1819	1821	rBV	312	221	0.02%	0.002%
41	6.941	1831	1835	1839	rBV3	262	232	0.02%	0.002%
42	6.989	1839	1850	1873	rBV	137192	253782	21.07%	2.670%
43	7.317	1940	1952	1971	rBV	569704	996134	82.70%	10.480%
44	7.577	2031	2033	2034	rBV2	433	183	0.02%	0.002%
45	7.625	2038	2048	2073	rVV	94632	166454	13.82%	1.751%
46	7.815	2104	2107	2110	rBV3	462	362	0.03%	0.004%
47	7.879	2124	2127	2131	rVV2	328	237	0.02%	0.002%
48	7.947	2140	2148	2155	rVV5	1726	2418	0.20%	0.025%
49	8.088	2182	2192	2224	rBV	299162	575761	47.80%	6.057%
50	8.600	2349	2351	2355	rBV3	338	238	0.02%	0.003%
51	8.661	2366	2370	2372	rBV2	309	179	0.01%	0.002%
52	8.693	2375	2380	2382	rVV2	343	278	0.02%	0.003%
53	8.706	2382	2384	2388	rVV4	330	220	0.02%	0.002%
54	8.744	2392	2396	2398	rBV2	416	289	0.02%	0.003%
55	8.854	2416	2430	2462	rBV	595454	987096	81.95%	10.384%
56	9.050	2490	2491	2494	rBV2	324	192	0.02%	0.002%
57	9.069	2494	2497	2501	rVV3	472	384	0.03%	0.004%
58	9.146	2518	2521	2524	rBV2	1018	864	0.07%	0.009%
59	9.201	2537	2538	2542	rVB3	573	261	0.02%	0.003%
60	9.352	2580	2585	2587	rBV3	325	214	0.02%	0.002%
61	9.384	2591	2595	2598	rVB2	318	280	0.02%	0.003%
62	9.471	2619	2622	2626	rBV2	208	184	0.02%	0.002%
63	9.551	2642	2647	2654	rBV5	648	740	0.06%	0.008%
64	9.580	2654	2656	2661	rVB3	451	306	0.03%	0.003%
65	9.674	2683	2685	2687	rBV	334	177	0.01%	0.002%
66	9.911	2753	2759	2761	rBV2	436	362	0.03%	0.004%
67	10.034	2794	2797	2800	rBV	345	209	0.02%	0.002%
68	10.127	2820	2826	2841	rVB8	2038	3445	0.29%	0.036%
69	10.220	2841	2855	2874	rBV	366242	582423	48.35%	6.127%
70	10.349	2893	2895	2897	rBV3	417	182	0.02%	0.002%
71	10.384	2901	2906	2913	rVB7	1910	2546	0.21%	0.027%
72	10.609	2972	2976	2977	rBV2	502	329	0.03%	0.003%
73	10.690	2998	3001	3004	rBV	254	183	0.02%	0.002%
74	10.799	3033	3035	3037	rBV2	514	233	0.02%	0.002%
75	10.921	3066	3073	3084	rVB4	2376	4020	0.33%	0.042%
76	11.021	3101	3104	3106	rBV	520	310	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022018.D
 Acq On : 30 Aug 2021 21:29
 Operator : SY/MD
 Sample : M3566-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKH9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	11.059	3114	3116	3118	rVB2	424	181	0.02%	0.002%
78	11.252	3164	3176	3197	rBV	640661	993430	82.47%	10.451%
79	11.391	3214	3219	3222	rBV5	1076	1178	0.10%	0.012%
80	11.471	3240	3244	3246	rBV	382	234	0.02%	0.002%
81	11.628	3281	3293	3314	rBV	581361	930614	77.26%	9.790%
82	11.854	3361	3363	3367	rBV2	490	422	0.04%	0.004%
83	11.940	3387	3390	3392	rBV	405	247	0.02%	0.003%
84	11.989	3402	3405	3407	rBV	291	213	0.02%	0.002%
85	12.005	3408	3410	3414	rVV2	412	265	0.02%	0.003%
86	12.021	3414	3415	3421	rVB2	288	248	0.02%	0.003%
87	12.127	3445	3448	3451	rBV4	498	325	0.03%	0.003%
88	12.227	3476	3479	3482	rBV3	314	266	0.02%	0.003%
89	12.342	3512	3515	3518	rBV2	263	223	0.02%	0.002%
90	12.458	3548	3551	3557	rVB3	551	394	0.03%	0.004%
91	12.712	3626	3630	3632	rBV2	393	320	0.03%	0.003%
92	12.802	3655	3658	3659	rBV	348	204	0.02%	0.002%
93	12.972	3709	3711	3715	rBV2	446	282	0.02%	0.003%
94	13.085	3742	3746	3747	rBV	369	232	0.02%	0.002%
95	13.207	3783	3784	3788	rVB2	331	183	0.02%	0.002%
96	13.429	3850	3853	3855	rBV2	530	322	0.03%	0.003%
97	13.468	3863	3865	3868	rBV	358	220	0.02%	0.002%
98	13.751	3950	3953	3955	rBV2	625	400	0.03%	0.004%
99	13.886	3993	3995	3997	rBV3	440	180	0.01%	0.002%
100	14.461	4172	4174	4178	rBV2	534	251	0.02%	0.003%


Sum of corrected areas: 9505521

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022018.D
Acq On : 30 Aug 2021 21:29
Operator : SY/MD
Sample : M3566-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
DBKH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

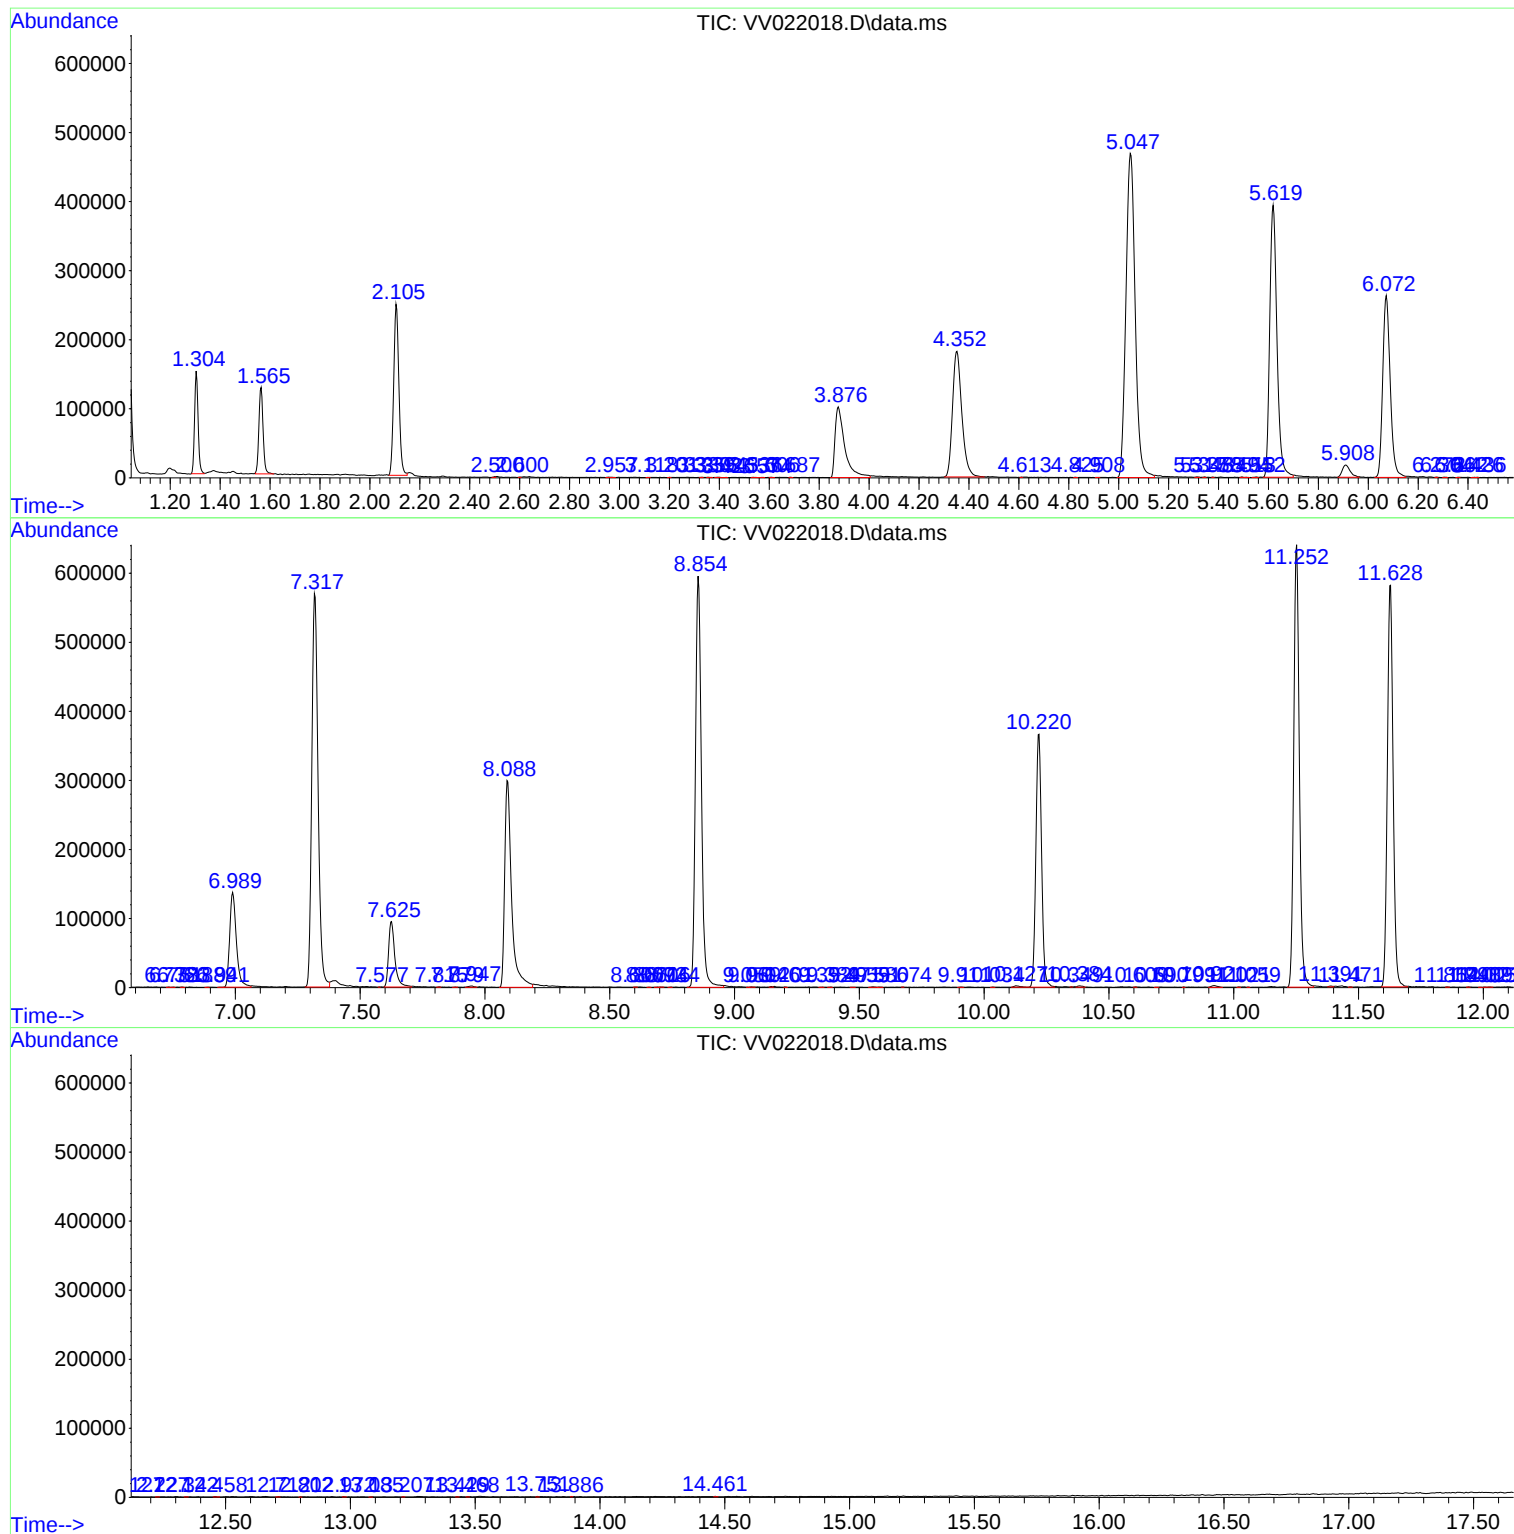

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022018.D
Acq On : 30 Aug 2021 21:29
Operator : SY/MD
Sample : M3566-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022018.D
Acq On : 30 Aug 2021 21:29
Operator : SY/MD
Sample : M3566-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKH9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
