

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022021.D
 Acq On : 30 Aug 2021 22:42
 Operator : SY/MD
 Sample : M3566-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022021.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	101	rVB	152190	149022	12.23%	1.543%
2	1.564	156	163	175	rVB	126049	143258	11.76%	1.483%
3	2.105	322	331	345	rBV	254032	369329	30.31%	3.824%
4	2.600	483	485	488	rBV2	384	166	0.01%	0.002%
5	2.622	490	492	493	rBV	556	249	0.02%	0.003%
6	2.767	530	537	538	rBV3	927	1051	0.09%	0.011%
7	2.815	550	552	557	rBV2	281	240	0.02%	0.002%
8	2.905	577	580	582	rBV	333	176	0.01%	0.002%
9	3.031	612	619	620	rBV2	401	419	0.03%	0.004%
10	3.182	664	666	672	rVV	276	213	0.02%	0.002%
11	3.223	676	679	681	rVB	247	162	0.01%	0.002%
12	3.413	736	738	743	rVV	335	231	0.02%	0.002%
13	3.436	743	745	751	rVB2	241	189	0.02%	0.002%
14	3.770	845	849	853	rBV2	336	298	0.02%	0.003%
15	3.876	872	882	919	rBV2	102480	280345	23.01%	2.903%
16	4.352	1015	1030	1057	rBV2	180287	469922	38.57%	4.866%
17	4.670	1127	1129	1133	rVB3	281	155	0.01%	0.002%
18	4.686	1133	1134	1137	rBV3	359	160	0.01%	0.002%
19	4.767	1156	1159	1161	rBV2	485	292	0.02%	0.003%
20	4.825	1174	1177	1183	rVB3	426	329	0.03%	0.003%
21	4.863	1186	1189	1190	rBV3	314	171	0.01%	0.002%
22	4.895	1196	1199	1201	rBV	442	267	0.02%	0.003%
23	4.937	1209	1212	1216	rVB	378	232	0.02%	0.002%
24	5.047	1229	1246	1277	rBV2	475647	1218319	100.00%	12.615%
25	5.519	1390	1393	1396	rVB4	369	236	0.02%	0.002%
26	5.561	1404	1406	1409	rVB3	387	186	0.02%	0.002%
27	5.619	1411	1424	1456	rBV	398103	813686	66.79%	8.425%
28	5.908	1503	1514	1536	rBB3	18172	39286	3.22%	0.407%
29	6.072	1551	1565	1587	rBV	269231	548225	45.00%	5.676%
30	6.313	1638	1640	1643	rVB2	777	369	0.03%	0.004%
31	6.358	1653	1654	1657	rBV	386	195	0.02%	0.002%
32	6.429	1673	1676	1680	rVB3	382	271	0.02%	0.003%
33	6.452	1680	1683	1686	rBV	307	219	0.02%	0.002%
34	6.526	1703	1706	1708	rBV	263	188	0.02%	0.002%
35	6.580	1718	1723	1726	rBV3	556	523	0.04%	0.005%
36	6.638	1738	1741	1743	rBV2	707	399	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022021.D
 Acq On : 30 Aug 2021 22:42
 Operator : SY/MD
 Sample : M3566-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.680	1750	1754	1761	rVB3	730	889	0.07%	0.009%
38	6.712	1761	1764	1767	rVB3	417	270	0.02%	0.003%
39	6.821	1796	1798	1804	rVB	310	215	0.02%	0.002%
40	6.860	1804	1810	1812	rBV3	279	225	0.02%	0.002%
41	6.918	1822	1828	1829	rBV	272	168	0.01%	0.002%
42	6.940	1833	1835	1838	rVB2	399	194	0.02%	0.002%
43	6.989	1838	1850	1872	rBV	137717	254936	20.93%	2.640%
44	7.317	1940	1952	1972	rBV	581164	1011886	83.06%	10.477%
45	7.625	2038	2048	2073	rBV2	94422	167254	13.73%	1.732%
46	7.854	2114	2119	2121	rBV3	309	207	0.02%	0.002%
47	7.870	2121	2124	2127	rVB	211	165	0.01%	0.002%
48	7.889	2127	2130	2133	rBV2	400	204	0.02%	0.002%
49	7.905	2133	2135	2137	rBV	458	203	0.02%	0.002%
50	7.921	2137	2140	2141	rBV	597	305	0.03%	0.003%
51	7.982	2156	2159	2163	rBV3	751	475	0.04%	0.005%
52	8.088	2183	2192	2238	rBV2	307212	592245	48.61%	6.132%
53	8.474	2311	2312	2315	rVB3	735	285	0.02%	0.003%
54	8.538	2327	2332	2333	rBV2	346	234	0.02%	0.002%
55	8.587	2341	2347	2349	rBV3	402	386	0.03%	0.004%
56	8.654	2364	2368	2370	rBV4	565	371	0.03%	0.004%
57	8.690	2377	2379	2382	rBV	364	174	0.01%	0.002%
58	8.786	2405	2409	2413	rBV2	587	496	0.04%	0.005%
59	8.853	2417	2430	2458	rBV	615896	1002312	82.27%	10.378%
60	9.082	2499	2501	2505	rBV2	468	404	0.03%	0.004%
61	9.136	2516	2518	2519	rBV2	410	169	0.01%	0.002%
62	9.226	2544	2546	2551	rVB2	398	201	0.02%	0.002%
63	9.262	2554	2557	2558	rVB	408	189	0.02%	0.002%
64	9.355	2583	2586	2588	rBV2	409	187	0.02%	0.002%
65	9.879	2742	2749	2752	rBV2	309	281	0.02%	0.003%
66	9.898	2752	2755	2756	rBV2	347	181	0.01%	0.002%
67	9.940	2761	2768	2770	rBV2	585	595	0.05%	0.006%
68	9.982	2777	2781	2783	rBV	292	214	0.02%	0.002%
69	10.091	2810	2815	2816	rBV2	373	243	0.02%	0.003%
70	10.133	2819	2828	2838	rBB5	2298	3354	0.28%	0.035%
71	10.220	2842	2855	2876	rBV	370559	588849	48.33%	6.097%
72	10.368	2899	2901	2902	rBV2	537	269	0.02%	0.003%
73	10.426	2915	2919	2922	rBV2	409	312	0.03%	0.003%
74	10.461	2926	2930	2933	rBV3	363	334	0.03%	0.003%
75	10.545	2951	2956	2957	rBV	578	429	0.04%	0.004%
76	10.580	2963	2967	2973	rBV5	729	832	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022021.D
 Acq On : 30 Aug 2021 22:42
 Operator : SY/MD
 Sample : M3566-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.606	2973	2975	2979	rVB3	564	234	0.02%	0.002%
78	10.738	3013	3016	3019	rBV3	339	300	0.02%	0.003%
79	10.914	3068	3071	3073	rBV3	1265	966	0.08%	0.010%
80	11.040	3103	3110	3116	rBV4	639	765	0.06%	0.008%
81	11.149	3139	3144	3147	rBV5	1011	1008	0.08%	0.010%
82	11.252	3164	3176	3198	rBV	644178	1004511	82.45%	10.401%
83	11.532	3259	3263	3264	rBV	559	333	0.03%	0.003%
84	11.541	3264	3266	3268	rBV2	720	455	0.04%	0.005%
85	11.625	3281	3292	3314	rBV	600011	938126	77.00%	9.713%
86	11.943	3389	3391	3398	rVB3	599	473	0.04%	0.005%
87	11.982	3398	3403	3406	rBV	392	376	0.03%	0.004%
88	12.049	3420	3424	3429	rVB2	473	399	0.03%	0.004%
89	12.117	3437	3445	3454	rVB6	2408	3613	0.30%	0.037%
90	12.168	3457	3461	3466	rBV2	308	247	0.02%	0.003%
91	12.249	3481	3486	3489	rBV3	409	346	0.03%	0.004%
92	12.365	3517	3522	3530	rBV7	1435	1938	0.16%	0.020%
93	12.606	3593	3597	3599	rBV2	291	233	0.02%	0.002%
94	12.889	3682	3685	3687	rBV3	721	323	0.03%	0.003%
95	13.178	3773	3775	3778	rBV	420	217	0.02%	0.002%
96	13.271	3800	3804	3807	rBV2	744	527	0.04%	0.005%
97	13.313	3810	3817	3823	rBV4	1232	1986	0.16%	0.021%
98	13.406	3843	3846	3847	rBV	373	192	0.02%	0.002%
99	13.506	3869	3877	3890	rBV	12749	21470	1.76%	0.222%
100	13.635	3908	3917	3925	rBV	5645	8834	0.73%	0.091%




Sum of corrected areas: 9657992

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022021.D
Acq On : 30 Aug 2021 22:42
Operator : SY/MD
Sample : M3566-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

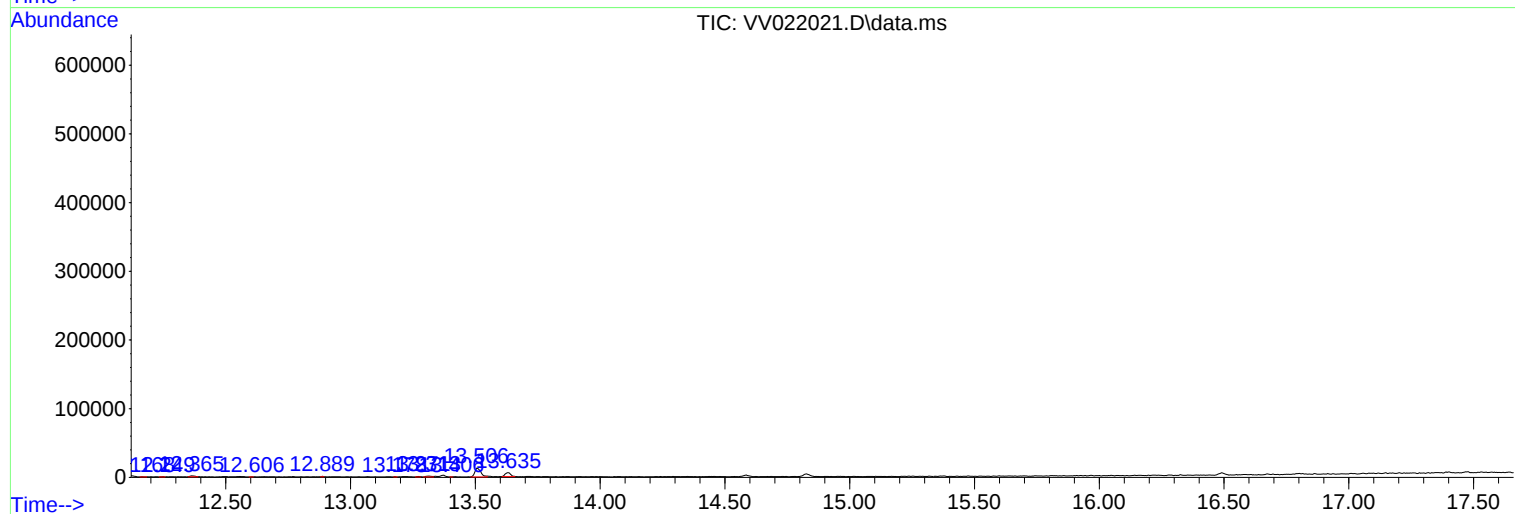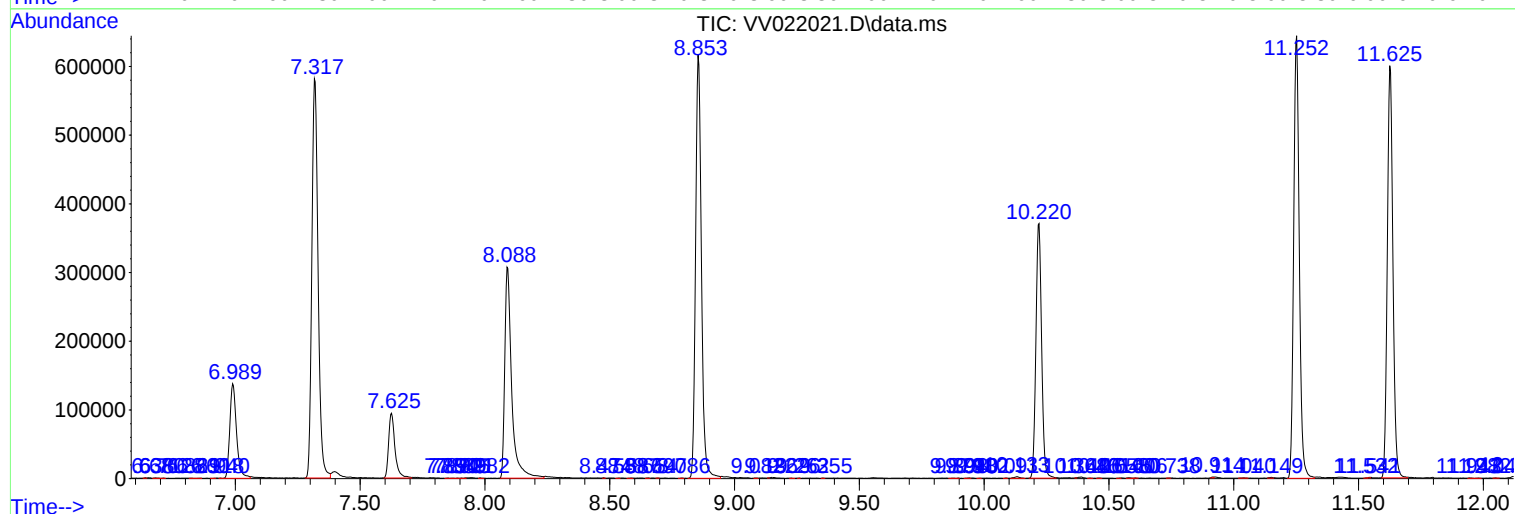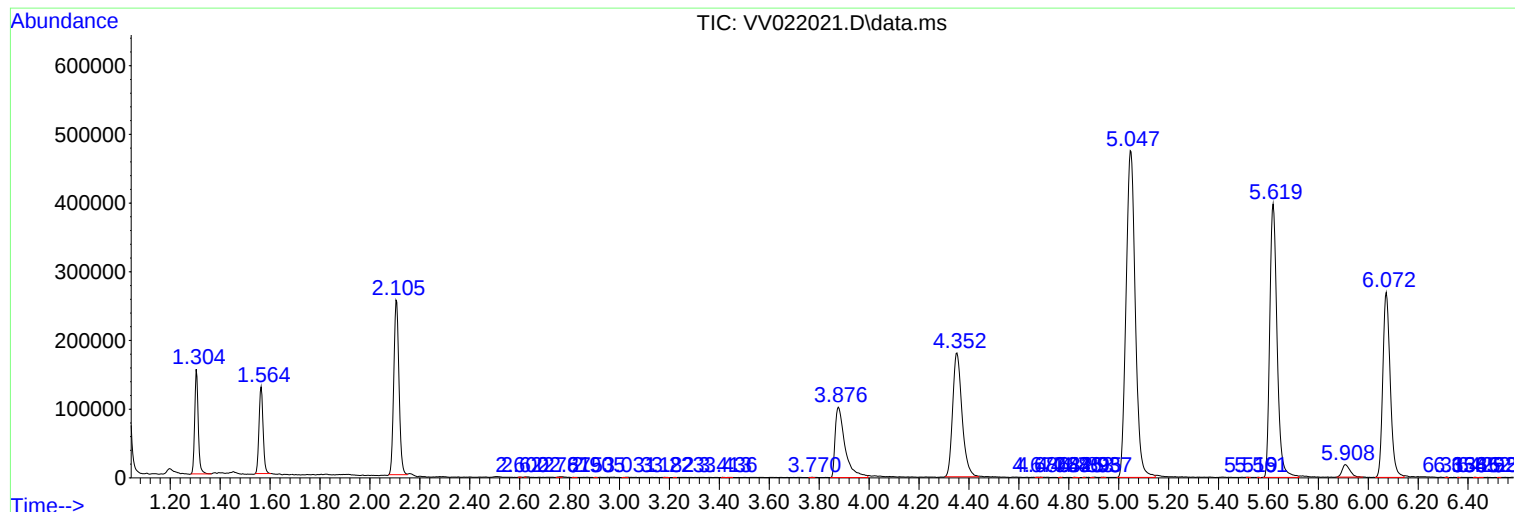

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022021.D
Acq On : 30 Aug 2021 22:42
Operator : SY/MD
Sample : M3566-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022021.D
Acq On : 30 Aug 2021 22:42
Operator : SY/MD
Sample : M3566-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
