

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022022.D
 Acq On : 30 Aug 2021 23:06
 Operator : SY/MD
 Sample : M3566-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022022.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rBV	142936	145227	11.97%	1.517%
2	1.564	157	163	177	rVB	127220	146622	12.08%	1.532%
3	2.108	323	332	344	rVB	241317	350785	28.91%	3.665%
4	2.722	517	523	527	rBV	517	466	0.04%	0.005%
5	2.761	530	535	536	rBV4	666	531	0.04%	0.006%
6	2.812	548	551	553	rBV2	407	249	0.02%	0.003%
7	2.944	589	592	595	rBV3	363	332	0.03%	0.003%
8	2.995	605	608	610	rVB	453	261	0.02%	0.003%
9	3.056	624	627	630	rVB	297	208	0.02%	0.002%
10	3.191	665	669	675	rVB4	428	475	0.04%	0.005%
11	3.310	703	706	709	rVB2	462	236	0.02%	0.002%
12	3.725	831	835	838	rBV4	510	387	0.03%	0.004%
13	3.876	870	882	919	rBV	104415	283370	23.35%	2.960%
14	4.352	1016	1030	1057	rVB	184791	465162	38.33%	4.859%
15	4.580	1099	1101	1106	rVB2	560	329	0.03%	0.003%
16	4.654	1119	1124	1126	rBV2	441	305	0.03%	0.003%
17	4.735	1147	1149	1156	rVB3	470	410	0.03%	0.004%
18	4.773	1156	1161	1163	rBV2	337	323	0.03%	0.003%
19	4.860	1185	1188	1192	rBV3	390	323	0.03%	0.003%
20	5.047	1229	1246	1282	rBV2	470584	1213469	100.00%	12.677%
21	5.522	1392	1394	1399	rVB	506	330	0.03%	0.003%
22	5.548	1399	1402	1404	rBV2	764	346	0.03%	0.004%
23	5.571	1405	1409	1412	rBV	6588	3904	0.32%	0.041%
24	5.619	1412	1424	1449	rBV	395888	799888	65.92%	8.356%
25	5.915	1504	1516	1534	rBV5	7802	17012	1.40%	0.178%
26	6.014	1544	1547	1550	rBV2	500	370	0.03%	0.004%
27	6.072	1551	1565	1596	rVV	266831	545048	44.92%	5.694%
28	6.416	1669	1672	1678	rVB4	551	497	0.04%	0.005%
29	6.471	1684	1689	1691	rBV	348	236	0.02%	0.002%
30	6.513	1698	1702	1703	rBV3	340	230	0.02%	0.002%
31	6.603	1727	1730	1734	rBV3	427	350	0.03%	0.004%
32	6.702	1758	1761	1763	rVB	391	193	0.02%	0.002%
33	6.989	1838	1850	1876	rBV2	137158	253947	20.93%	2.653%
34	7.140	1895	1897	1901	rVB2	717	455	0.04%	0.005%
35	7.182	1908	1910	1912	rBV2	461	270	0.02%	0.003%
36	7.236	1925	1927	1930	rVB4	755	350	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022022.D
 Acq On : 30 Aug 2021 23:06
 Operator : SY/MD
 Sample : M3566-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	7.320	1941	1953	1971	rBV	578370	999016	82.33%	10.437%
38	7.625	2037	2048	2071	rBV2	92274	163035	13.44%	1.703%
39	7.947	2142	2148	2156	rVB6	2072	2696	0.22%	0.028%
40	7.998	2161	2164	2166	rVB2	639	286	0.02%	0.003%
41	8.030	2169	2174	2176	rBV3	299	249	0.02%	0.003%
42	8.091	2178	2193	2226	rBV	314072	583051	48.05%	6.091%
43	8.622	2356	2358	2364	rVB2	527	428	0.04%	0.004%
44	8.728	2388	2391	2396	rVB3	526	411	0.03%	0.004%
45	8.792	2408	2411	2415	rVB2	511	362	0.03%	0.004%
46	8.854	2418	2430	2455	rBV	602331	993464	81.87%	10.379%
47	9.046	2488	2490	2493	rVB2	698	385	0.03%	0.004%
48	9.063	2493	2495	2497	rVV2	479	207	0.02%	0.002%
49	9.323	2572	2576	2578	rBV	283	226	0.02%	0.002%
50	9.410	2600	2603	2605	rBV	410	200	0.02%	0.002%
51	9.468	2617	2621	2622	rBV2	318	208	0.02%	0.002%
52	9.603	2659	2663	2665	rBV2	606	260	0.02%	0.003%
53	9.648	2674	2677	2681	rBV2	317	204	0.02%	0.002%
54	9.805	2723	2726	2732	rVB2	415	249	0.02%	0.003%
55	9.837	2732	2736	2741	rBV2	421	430	0.04%	0.004%
56	9.972	2776	2778	2784	rVB2	422	300	0.02%	0.003%
57	10.001	2784	2787	2791	rVB2	250	204	0.02%	0.002%
58	10.030	2791	2796	2800	rBV3	372	367	0.03%	0.004%
59	10.133	2820	2828	2837	rVV3	2063	2982	0.25%	0.031%
60	10.217	2843	2854	2876	rBV	385548	618024	50.93%	6.456%
61	10.316	2883	2885	2887	rBV2	759	427	0.04%	0.004%
62	10.362	2897	2899	2901	rBV3	647	392	0.03%	0.004%
63	10.381	2901	2905	2915	rVB5	2577	4335	0.36%	0.045%
64	10.461	2926	2930	2934	rBV3	558	461	0.04%	0.005%
65	10.503	2939	2943	2949	rBV2	436	466	0.04%	0.005%
66	10.551	2955	2958	2960	rVB2	434	238	0.02%	0.002%
67	10.574	2960	2965	2967	rBV2	304	331	0.03%	0.003%
68	10.606	2973	2975	2978	rVB2	643	288	0.02%	0.003%
69	10.680	2993	2998	3000	rBV	370	261	0.02%	0.003%
70	10.773	3023	3027	3028	rBV2	357	223	0.02%	0.002%
71	10.789	3029	3032	3035	rVV3	566	306	0.03%	0.003%
72	10.921	3065	3073	3082	rVB5	2420	3761	0.31%	0.039%
73	11.001	3093	3098	3099	rBV	330	235	0.02%	0.002%
74	11.037	3106	3109	3115	rVB3	647	627	0.05%	0.007%
75	11.140	3138	3141	3143	rBV2	500	411	0.03%	0.004%
76	11.201	3158	3160	3164	rVB2	503	349	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022022.D
 Acq On : 30 Aug 2021 23:06
 Operator : SY/MD
 Sample : M3566-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

77	11.252	3164	3176	3196	rBV	641896	1005854	82.89%	10.508%
78	11.477	3243	3246	3247	rBV2	597	291	0.02%	0.003%
79	11.542	3256	3266	3268	rBV4	938	1095	0.09%	0.011%
80	11.628	3281	3293	3313	rBV	584597	939362	77.41%	9.813%
81	11.808	3346	3349	3350	rBV	426	194	0.02%	0.002%
82	11.857	3360	3364	3368	rBV5	587	472	0.04%	0.005%
83	11.905	3376	3379	3383	rVV2	266	236	0.02%	0.002%
84	11.934	3385	3388	3391	rVB3	505	303	0.02%	0.003%
85	11.966	3395	3398	3402	rVB3	379	217	0.02%	0.002%
86	11.992	3403	3406	3410	rVV3	481	351	0.03%	0.004%
87	12.011	3410	3412	3415	rVV	362	213	0.02%	0.002%
88	12.056	3424	3426	3429	rVB	578	313	0.03%	0.003%
89	12.104	3435	3441	3446	rBV5	687	787	0.06%	0.008%
90	12.316	3505	3507	3511	rBV2	437	265	0.02%	0.003%
91	12.522	3568	3571	3574	rBV	316	199	0.02%	0.002%
92	13.004	3717	3721	3723	rVV3	492	368	0.03%	0.004%
93	13.027	3726	3728	3731	rVB2	369	194	0.02%	0.002%
94	13.101	3749	3751	3755	rBV2	383	308	0.03%	0.003%
95	13.140	3759	3763	3766	rVV2	329	281	0.02%	0.003%
96	13.307	3812	3815	3817	rBV	600	336	0.03%	0.004%
97	13.480	3865	3869	3871	rVB2	353	224	0.02%	0.002%
98	13.516	3874	3880	3899	rVB3	3702	6279	0.52%	0.066%
99	13.828	3974	3977	3983	rVB3	500	335	0.03%	0.003%
100	13.969	4016	4021	4025	rBV2	405	496	0.04%	0.005%




Sum of corrected areas: 9572224

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022022.D
Acq On : 30 Aug 2021 23:06
Operator : SY/MD
Sample : M3566-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

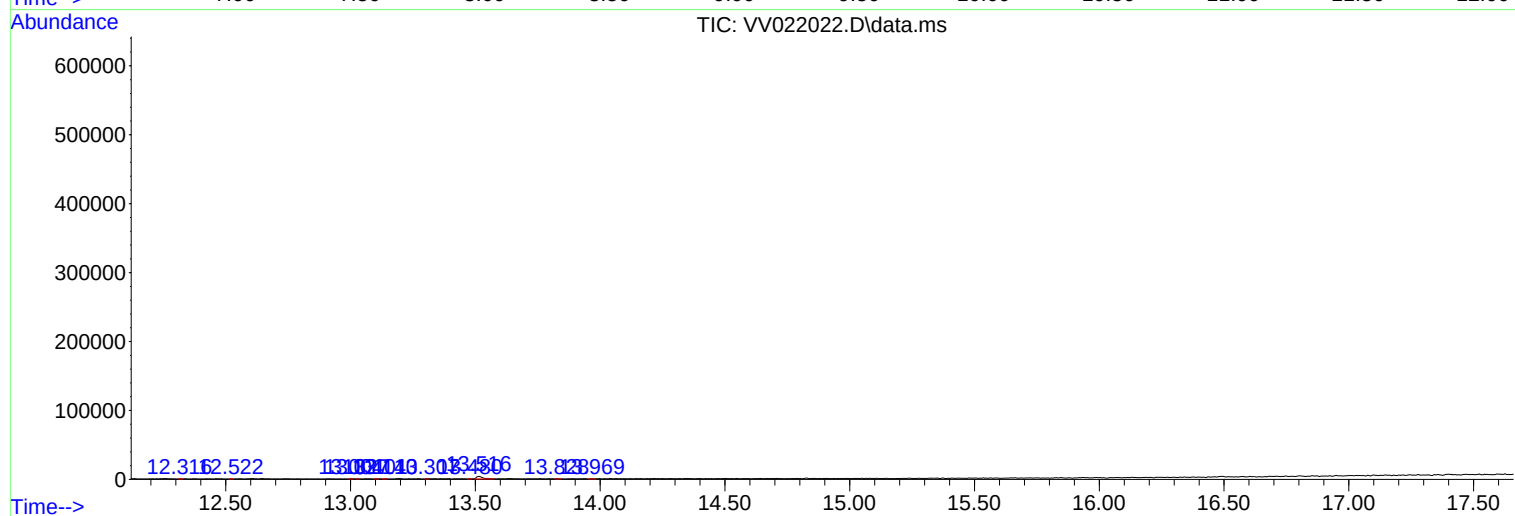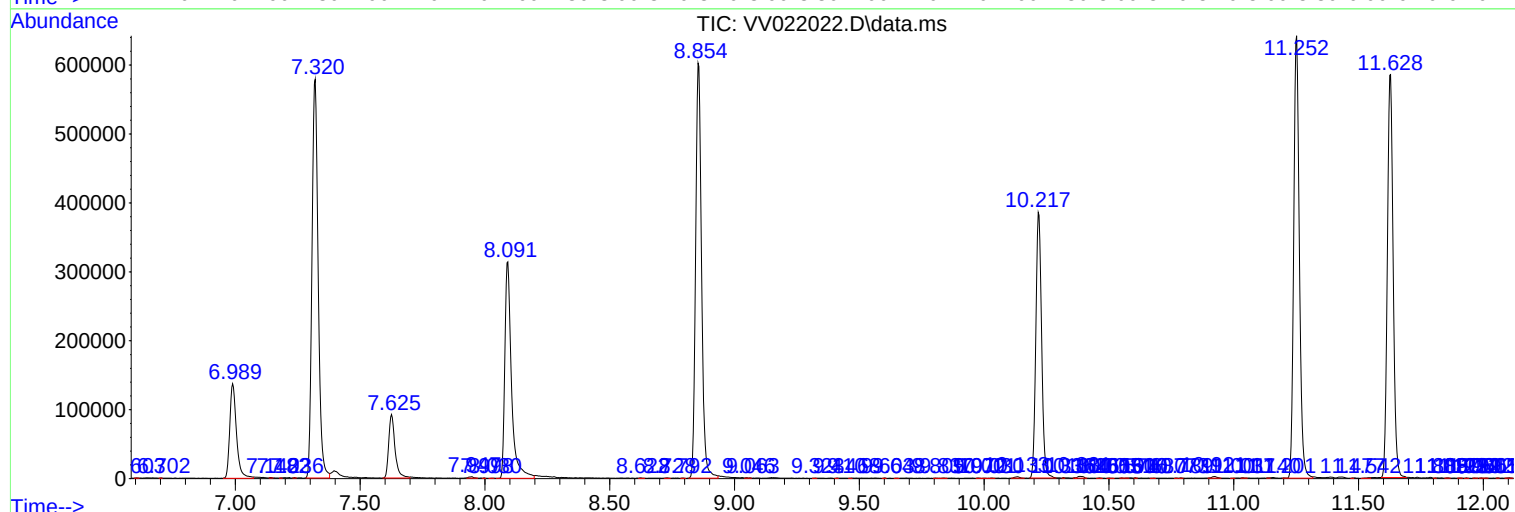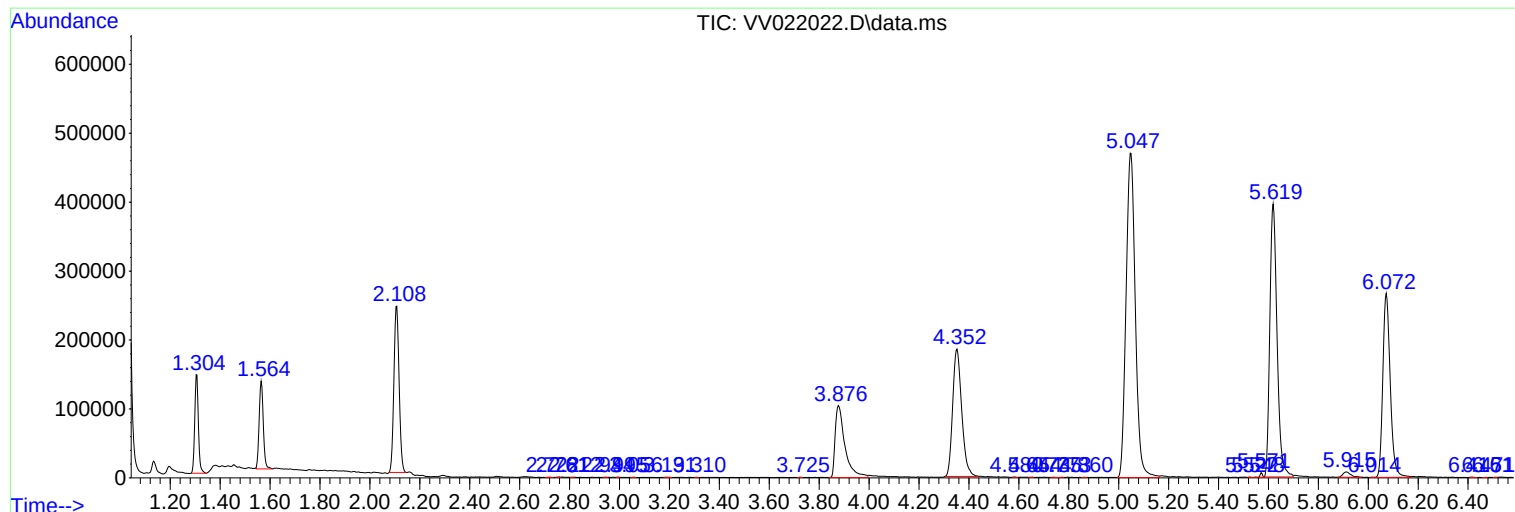

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022022.D
Acq On : 30 Aug 2021 23:06
Operator : SY/MD
Sample : M3566-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022022.D
Acq On : 30 Aug 2021 23:06
Operator : SY/MD
Sample : M3566-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
