

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022023.D
 Acq On : 30 Aug 2021 23:30
 Operator : SY/MD
 Sample : M3566-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rBV	148136	143411	12.10%	1.533%
2	1.564	156	163	177	rVB	129532	149109	12.58%	1.594%
3	2.104	322	331	345	rBV	241726	351799	29.69%	3.760%
4	2.503	451	455	457	rBV4	890	729	0.06%	0.008%
5	2.580	474	479	481	rBV2	539	393	0.03%	0.004%
6	2.593	481	483	486	rVB2	321	171	0.01%	0.002%
7	2.661	502	504	508	rBV3	277	174	0.01%	0.002%
8	2.699	513	516	518	rBV3	430	234	0.02%	0.003%
9	2.773	530	539	550	rVB5	3047	5683	0.48%	0.061%
10	2.979	601	603	608	rBV2	300	239	0.02%	0.003%
11	3.066	624	630	633	rBV2	369	460	0.04%	0.005%
12	3.117	641	646	649	rBV3	339	316	0.03%	0.003%
13	3.211	671	675	678	rBV2	526	433	0.04%	0.005%
14	3.288	697	699	701	rVV	475	194	0.02%	0.002%
15	3.313	704	707	712	rVB	405	308	0.03%	0.003%
16	3.490	759	762	765	rBV3	188	136	0.01%	0.001%
17	3.564	783	785	787	rBV	232	146	0.01%	0.002%
18	3.709	828	830	836	rVB2	284	277	0.02%	0.003%
19	3.741	836	840	845	rBV2	350	297	0.03%	0.003%
20	3.876	872	882	915	rBV	96002	258771	21.84%	2.766%
21	4.352	1015	1030	1061	rBV	180306	462591	39.04%	4.945%
22	4.606	1107	1109	1111	rVB3	628	218	0.02%	0.002%
23	4.776	1160	1162	1164	rVB	496	173	0.01%	0.002%
24	4.789	1164	1166	1168	rBV	265	128	0.01%	0.001%
25	4.821	1173	1176	1178	rVV	385	311	0.03%	0.003%
26	4.847	1182	1184	1189	rVV3	482	368	0.03%	0.004%
27	4.870	1189	1191	1194	rVB	239	154	0.01%	0.002%
28	5.046	1229	1246	1286	rBV2	455056	1185058	100.00%	12.667%
29	5.323	1330	1332	1335	rBV2	363	222	0.02%	0.002%
30	5.410	1357	1359	1361	rBV2	512	239	0.02%	0.003%
31	5.493	1381	1385	1389	rVB3	445	280	0.02%	0.003%
32	5.516	1389	1392	1398	rBV3	361	509	0.04%	0.005%
33	5.619	1412	1424	1453	rBV	394192	805578	67.98%	8.611%
34	5.850	1494	1496	1498	rBV3	393	125	0.01%	0.001%
35	5.992	1538	1540	1541	rBV3	416	152	0.01%	0.002%
36	6.072	1551	1565	1598	rBV2	262856	541238	45.67%	5.785%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022023.D
 Acq On : 30 Aug 2021 23:30
 Operator : SY/MD
 Sample : M3566-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.390	1662	1664	1665	rBV	303	153	0.01%	0.002%
38	6.464	1682	1687	1689	rBV2	373	271	0.02%	0.003%
39	6.532	1705	1708	1711	rBV2	217	142	0.01%	0.002%
40	6.593	1726	1727	1732	rVB2	280	151	0.01%	0.002%
41	6.616	1732	1734	1738	rBV2	603	301	0.03%	0.003%
42	6.644	1738	1743	1746	rBV3	619	680	0.06%	0.007%
43	6.686	1753	1756	1758	rBV2	404	236	0.02%	0.003%
44	6.725	1763	1768	1771	rVB3	257	205	0.02%	0.002%
45	6.828	1796	1800	1807	rBV2	411	402	0.03%	0.004%
46	6.944	1832	1836	1839	rBV2	533	408	0.03%	0.004%
47	6.989	1839	1850	1875	rBV	134907	248889	21.00%	2.660%
48	7.140	1895	1897	1900	rVB2	423	180	0.02%	0.002%
49	7.210	1912	1919	1921	rBV5	737	924	0.08%	0.010%
50	7.320	1941	1953	1973	rBV	556769	978605	82.58%	10.460%
51	7.625	2038	2048	2079	rVB	90851	159344	13.45%	1.703%
52	7.873	2122	2125	2129	rBV4	295	205	0.02%	0.002%
53	7.892	2129	2131	2134	rVB	370	156	0.01%	0.002%
54	7.985	2157	2160	2162	rBV3	761	440	0.04%	0.005%
55	8.034	2171	2175	2180	rBV3	315	259	0.02%	0.003%
56	8.091	2182	2193	2228	rBV	294866	554566	46.80%	5.928%
57	8.442	2299	2302	2305	rBV3	547	377	0.03%	0.004%
58	8.609	2352	2354	2358	rVB3	396	166	0.01%	0.002%
59	8.628	2358	2360	2365	rVB	345	202	0.02%	0.002%
60	8.696	2378	2381	2385	rBV2	395	284	0.02%	0.003%
61	8.715	2385	2387	2389	rVB	464	197	0.02%	0.002%
62	8.853	2418	2430	2457	rBV	590729	980064	82.70%	10.476%
63	9.262	2555	2557	2560	rVV3	556	319	0.03%	0.003%
64	9.300	2564	2569	2573	rBV2	392	336	0.03%	0.004%
65	9.349	2581	2584	2588	rBV	251	160	0.01%	0.002%
66	9.394	2595	2598	2601	rBV	216	157	0.01%	0.002%
67	9.564	2645	2651	2654	rBV3	489	435	0.04%	0.005%
68	9.583	2654	2657	2659	rVB2	360	202	0.02%	0.002%
69	9.879	2746	2749	2754	rVB2	465	325	0.03%	0.003%
70	9.931	2761	2765	2766	rBV2	388	242	0.02%	0.003%
71	9.959	2772	2774	2778	rVB2	412	238	0.02%	0.003%
72	10.008	2787	2789	2791	rBV	257	144	0.01%	0.002%
73	10.066	2804	2807	2811	rVB2	303	192	0.02%	0.002%
74	10.104	2817	2819	2820	rBV	349	134	0.01%	0.001%
75	10.130	2820	2827	2839	rVB4	1717	2989	0.25%	0.032%
76	10.175	2839	2841	2843	rBV2	392	132	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022023.D
 Acq On : 30 Aug 2021 23:30
 Operator : SY/MD
 Sample : M3566-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

77	10.220	2843	2855	2874	rBV	375367	592241	49.98%	6.330%
78	10.390	2901	2908	2920	rVB4	3220	4905	0.41%	0.052%
79	10.615	2974	2978	2983	rVB4	463	369	0.03%	0.004%
80	10.776	3025	3028	3031	rBV2	401	190	0.02%	0.002%
81	10.831	3041	3045	3047	rBV	412	237	0.02%	0.003%
82	10.850	3048	3051	3055	rBV2	428	290	0.02%	0.003%
83	10.918	3069	3072	3082	rVB6	2139	3134	0.26%	0.033%
84	11.091	3124	3126	3130	rBV2	439	306	0.03%	0.003%
85	11.194	3156	3158	3162	rVB2	636	269	0.02%	0.003%
86	11.252	3164	3176	3196	rBV	628312	986090	83.21%	10.540%
87	11.625	3280	3292	3315	rBV	581743	917185	77.40%	9.804%
88	11.837	3355	3358	3361	rBV2	452	311	0.03%	0.003%
89	12.101	3436	3440	3442	rBV2	394	327	0.03%	0.003%
90	12.172	3460	3462	3465	rVB2	333	148	0.01%	0.002%
91	12.223	3474	3478	3484	rBV3	376	311	0.03%	0.003%
92	12.361	3517	3521	3523	rVB3	372	260	0.02%	0.003%
93	12.377	3523	3526	3528	rBV2	266	163	0.01%	0.002%
94	12.416	3534	3538	3539	rBV	356	247	0.02%	0.003%
95	12.545	3575	3578	3582	rVB2	393	267	0.02%	0.003%
96	13.278	3801	3806	3809	rBV	473	396	0.03%	0.004%
97	13.451	3858	3860	3863	rBV2	278	176	0.01%	0.002%
98	13.474	3863	3867	3872	rVV3	397	331	0.03%	0.004%
99	13.522	3872	3882	3888	rBV5	1784	2652	0.22%	0.028%
100	13.625	3911	3914	3916	rBV2	192	131	0.01%	0.001%




Sum of corrected areas: 9355372

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022023.D
Acq On : 30 Aug 2021 23:30
Operator : SY/MD
Sample : M3566-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

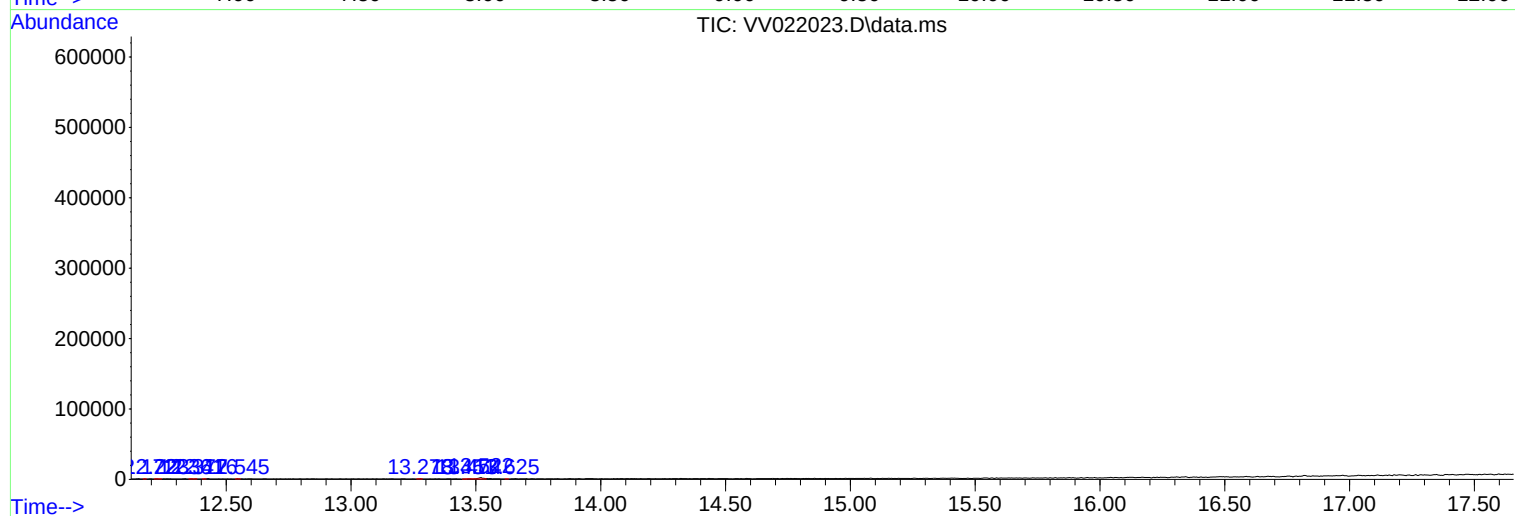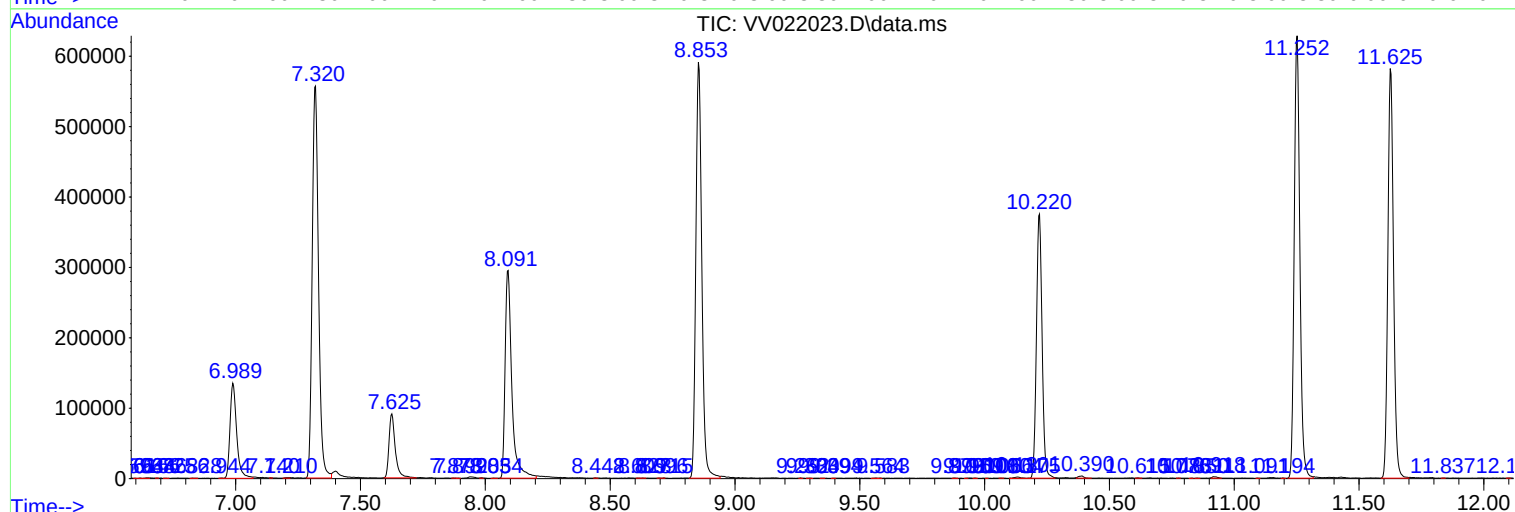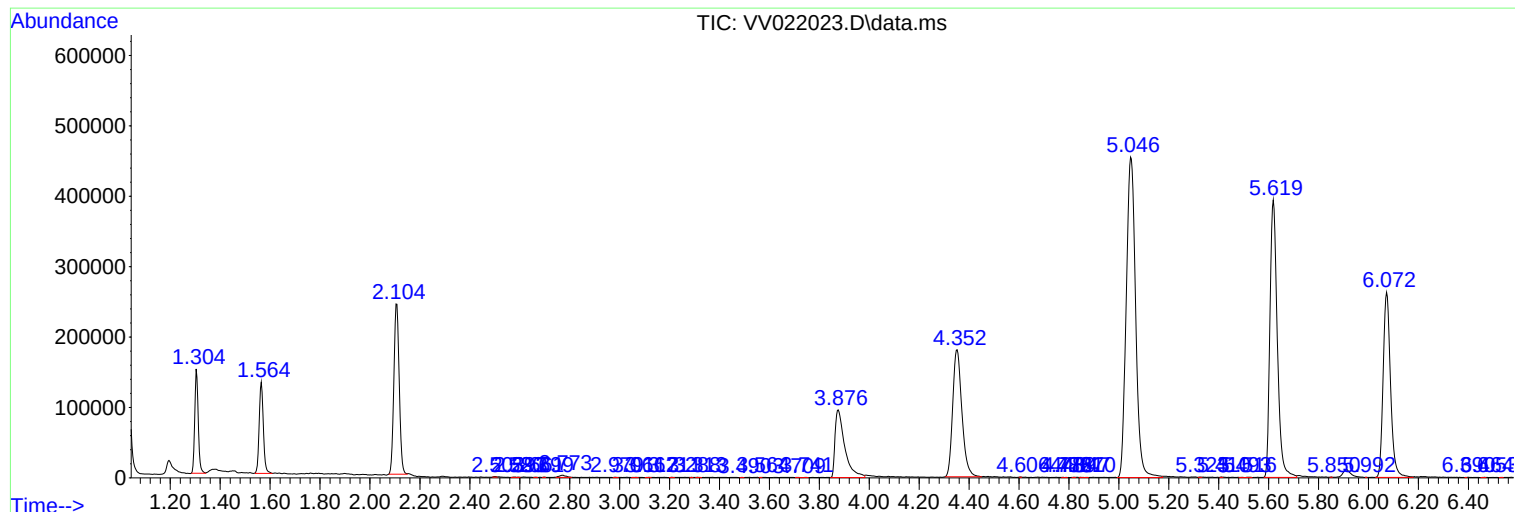

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022023.D
Acq On : 30 Aug 2021 23:30
Operator : SY/MD
Sample : M3566-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022023.D
Acq On : 30 Aug 2021 23:30
Operator : SY/MD
Sample : M3566-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------