

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022024.D
 Acq On : 30 Aug 2021 23:54
 Operator : SY/MD
 Sample : M3566-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	148086	147655	12.35%	1.561%
2	1.564	156	163	179	rVB	124662	143593	12.01%	1.518%
3	2.105	322	331	345	rBV	250723	364830	30.51%	3.857%
4	2.439	433	435	438	rBV2	386	274	0.02%	0.003%
5	2.503	451	455	457	rBV4	1154	1020	0.09%	0.011%
6	2.552	468	470	474	rBV	275	177	0.01%	0.002%
7	2.847	559	562	563	rBV	520	243	0.02%	0.003%
8	3.021	613	616	619	rBV	267	214	0.02%	0.002%
9	3.130	646	650	652	rBV2	370	227	0.02%	0.002%
10	3.172	661	663	665	rBV2	354	168	0.01%	0.002%
11	3.211	673	675	678	rBV2	342	204	0.02%	0.002%
12	3.326	708	711	716	rBV2	299	290	0.02%	0.003%
13	3.429	738	743	746	rBV2	347	322	0.03%	0.003%
14	3.587	789	792	795	rBV2	182	141	0.01%	0.001%
15	3.876	872	882	918	rBV	103172	272927	22.83%	2.886%
16	4.352	1014	1030	1062	rBV	185975	468786	39.21%	4.956%
17	4.619	1111	1113	1114	rBV	328	154	0.01%	0.002%
18	4.696	1135	1137	1143	rVV2	353	346	0.03%	0.004%
19	4.728	1144	1147	1150	rVB2	484	299	0.03%	0.003%
20	4.783	1160	1164	1166	rBV2	257	221	0.02%	0.002%
21	4.799	1167	1169	1172	rVB2	443	185	0.02%	0.002%
22	4.883	1193	1195	1199	rBV2	276	188	0.02%	0.002%
23	4.905	1199	1202	1207	rVB2	343	293	0.02%	0.003%
24	4.934	1207	1211	1215	rBV3	438	428	0.04%	0.005%
25	4.969	1219	1222	1229	rBV	513	498	0.04%	0.005%
26	5.047	1229	1246	1281	rBV2	466017	1195693	100.00%	12.642%
27	5.265	1311	1314	1316	rBV3	694	390	0.03%	0.004%
28	5.410	1356	1359	1362	rBV	377	304	0.03%	0.003%
29	5.494	1383	1385	1388	rBV2	308	143	0.01%	0.002%
30	5.529	1391	1396	1397	rBV2	341	195	0.02%	0.002%
31	5.619	1412	1424	1457	rBV	401393	807206	67.51%	8.534%
32	5.912	1504	1515	1529	rBV3	15729	33224	2.78%	0.351%
33	6.072	1552	1565	1595	rBV	263077	538950	45.07%	5.698%
34	6.349	1648	1651	1654	rBV	509	330	0.03%	0.003%
35	6.368	1655	1657	1658	rVV	384	153	0.01%	0.002%
36	6.394	1662	1665	1668	rBV2	251	188	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022024.D
 Acq On : 30 Aug 2021 23:54
 Operator : SY/MD
 Sample : M3566-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.516	1698	1703	1708	rBV3	752	858	0.07%	0.009%
38	6.612	1731	1733	1736	rVB	403	187	0.02%	0.002%
39	6.632	1736	1739	1740	rBV	451	264	0.02%	0.003%
40	6.719	1764	1766	1769	rVB2	536	245	0.02%	0.003%
41	6.741	1769	1773	1778	rVB3	331	264	0.02%	0.003%
42	6.767	1778	1781	1783	rBV	636	341	0.03%	0.004%
43	6.847	1802	1806	1807	rBV	545	281	0.02%	0.003%
44	6.873	1810	1814	1817	rVB3	282	230	0.02%	0.002%
45	6.921	1825	1829	1830	rBV2	187	132	0.01%	0.001%
46	6.937	1832	1834	1836	rVB2	377	148	0.01%	0.002%
47	6.989	1839	1850	1875	rBV	135662	248143	20.75%	2.624%
48	7.320	1940	1953	1971	rBV	566473	988192	82.65%	10.448%
49	7.625	2037	2048	2075	rBV	93096	166040	13.89%	1.756%
50	7.921	2138	2140	2141	rBV	446	130	0.01%	0.001%
51	7.973	2154	2156	2157	rVB	534	147	0.01%	0.002%
52	8.091	2182	2193	2225	rBV	300067	571652	47.81%	6.044%
53	8.625	2356	2359	2362	rVB2	379	225	0.02%	0.002%
54	8.654	2365	2368	2372	rVV4	572	329	0.03%	0.003%
55	8.693	2376	2380	2381	rBV2	389	270	0.02%	0.003%
56	8.712	2384	2386	2388	rBV	211	147	0.01%	0.002%
57	8.738	2392	2394	2396	rBV2	295	146	0.01%	0.002%
58	8.854	2419	2430	2463	rVV	594888	982317	82.15%	10.386%
59	9.108	2507	2509	2510	rBV	366	157	0.01%	0.002%
60	9.127	2513	2515	2516	rBV	345	124	0.01%	0.001%
61	9.201	2536	2538	2540	rVB2	460	189	0.02%	0.002%
62	9.233	2546	2548	2553	rVB3	436	272	0.02%	0.003%
63	9.358	2585	2587	2589	rBV	299	158	0.01%	0.002%
64	9.394	2596	2598	2604	rBV2	163	150	0.01%	0.002%
65	9.458	2613	2618	2619	rBV2	397	307	0.03%	0.003%
66	9.603	2660	2663	2664	rBV	311	124	0.01%	0.001%
67	9.661	2679	2681	2686	rBV2	297	160	0.01%	0.002%
68	9.760	2710	2712	2716	rBV3	234	146	0.01%	0.002%
69	9.870	2742	2746	2748	rBV	191	173	0.01%	0.002%
70	9.895	2751	2754	2755	rBV	247	126	0.01%	0.001%
71	10.024	2791	2794	2796	rBV	315	213	0.02%	0.002%
72	10.101	2811	2818	2819	rBV	310	257	0.02%	0.003%
73	10.136	2821	2829	2836	rVB3	1542	2696	0.23%	0.029%
74	10.217	2841	2854	2875	rBV	368303	590796	49.41%	6.246%
75	10.384	2897	2906	2919	rVB4	2889	5290	0.44%	0.056%
76	10.432	2919	2921	2923	rBV3	260	139	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022024.D
 Acq On : 30 Aug 2021 23:54
 Operator : SY/MD
 Sample : M3566-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.506	2940	2944	2949	rBV3	496	448	0.04%	0.005%
78	10.590	2966	2970	2974	rBV3	533	618	0.05%	0.007%
79	10.715	3007	3009	3012	rBV	224	130	0.01%	0.001%
80	10.734	3012	3015	3017	rVV	345	179	0.01%	0.002%
81	10.850	3049	3051	3053	rBV	481	233	0.02%	0.002%
82	10.918	3067	3072	3085	rVB4	2024	3184	0.27%	0.034%
83	11.117	3131	3134	3137	rVB2	292	165	0.01%	0.002%
84	11.140	3137	3141	3143	rBV2	598	511	0.04%	0.005%
85	11.252	3164	3176	3201	rBV	632709	988060	82.63%	10.447%
86	11.423	3227	3229	3230	rBV	901	390	0.03%	0.004%
87	11.477	3243	3246	3249	rBV3	510	382	0.03%	0.004%
88	11.628	3281	3293	3314	rBV	573991	917578	76.74%	9.701%
89	11.834	3354	3357	3359	rBV2	546	354	0.03%	0.004%
90	12.242	3480	3484	3486	rBV3	443	369	0.03%	0.004%
91	12.400	3530	3533	3535	rBV	266	147	0.01%	0.002%
92	12.525	3568	3572	3575	rBV	490	398	0.03%	0.004%
93	12.828	3660	3666	3670	rBV3	554	468	0.04%	0.005%
94	13.040	3729	3732	3734	rBV2	466	247	0.02%	0.003%
95	13.281	3806	3807	3813	rBV3	311	317	0.03%	0.003%
96	13.493	3871	3873	3875	rBV2	411	206	0.02%	0.002%
97	13.699	3936	3937	3940	rBV	271	148	0.01%	0.002%
98	13.734	3944	3948	3953	rVB3	506	483	0.04%	0.005%
99	13.757	3953	3955	3956	rBV	300	119	0.01%	0.001%
100	14.046	4042	4045	4047	rBV3	704	449	0.04%	0.005%




Sum of corrected areas: 9458207

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022024.D
Acq On : 30 Aug 2021 23:54
Operator : SY/MD
Sample : M3566-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
DBKJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

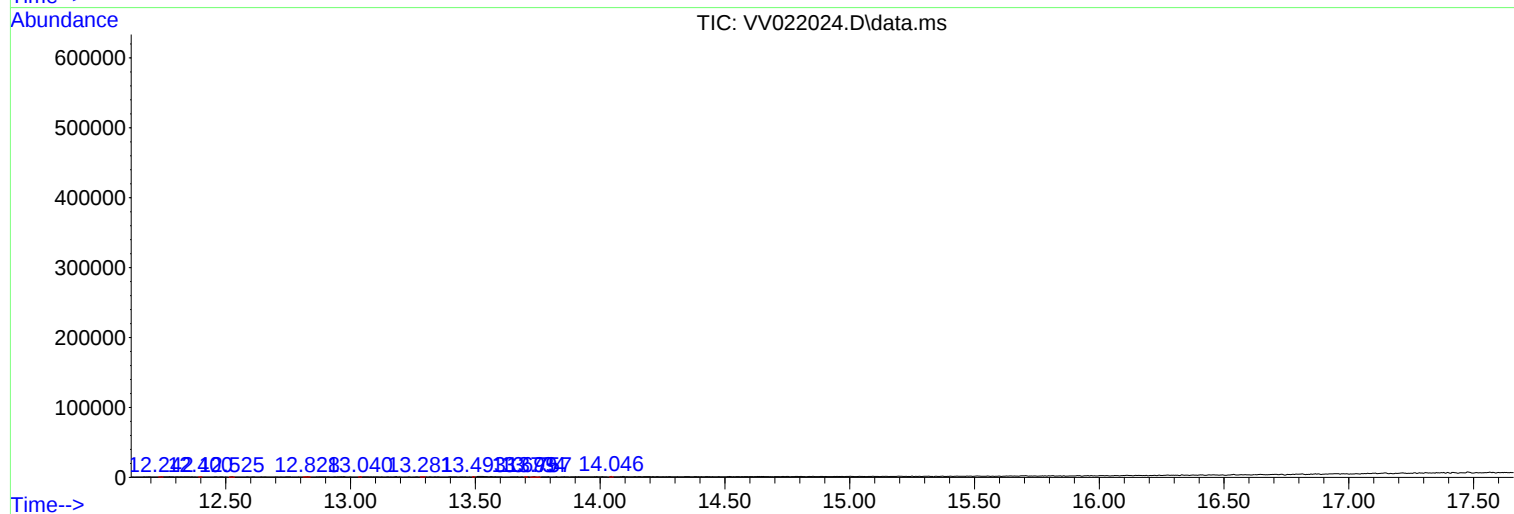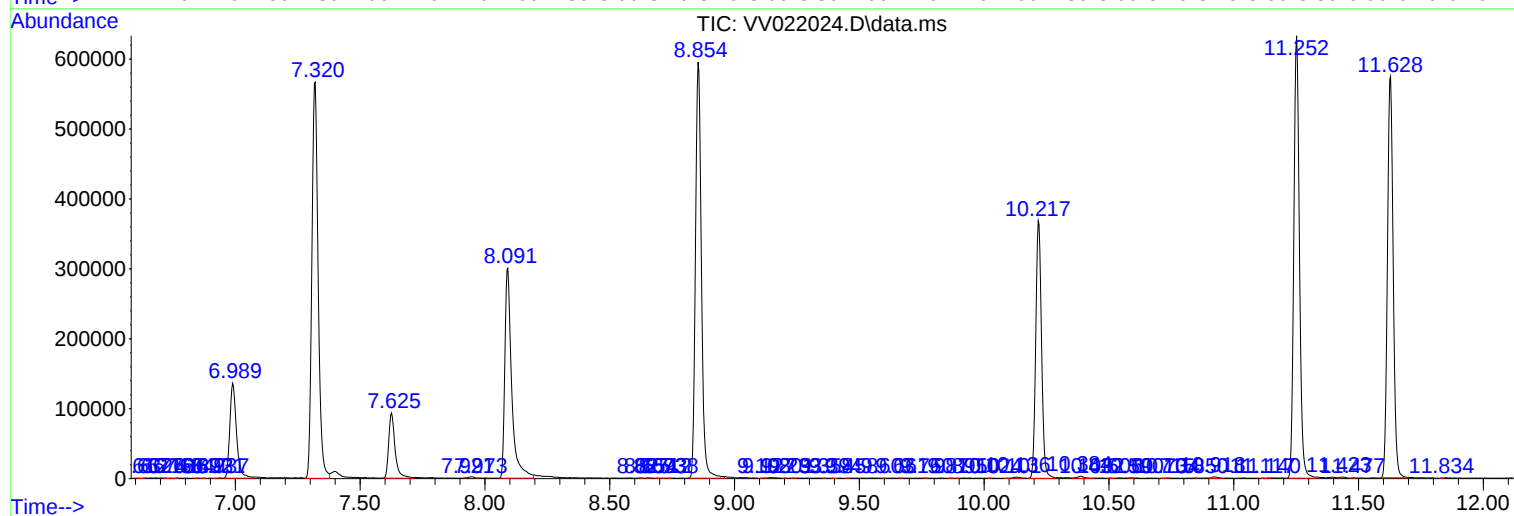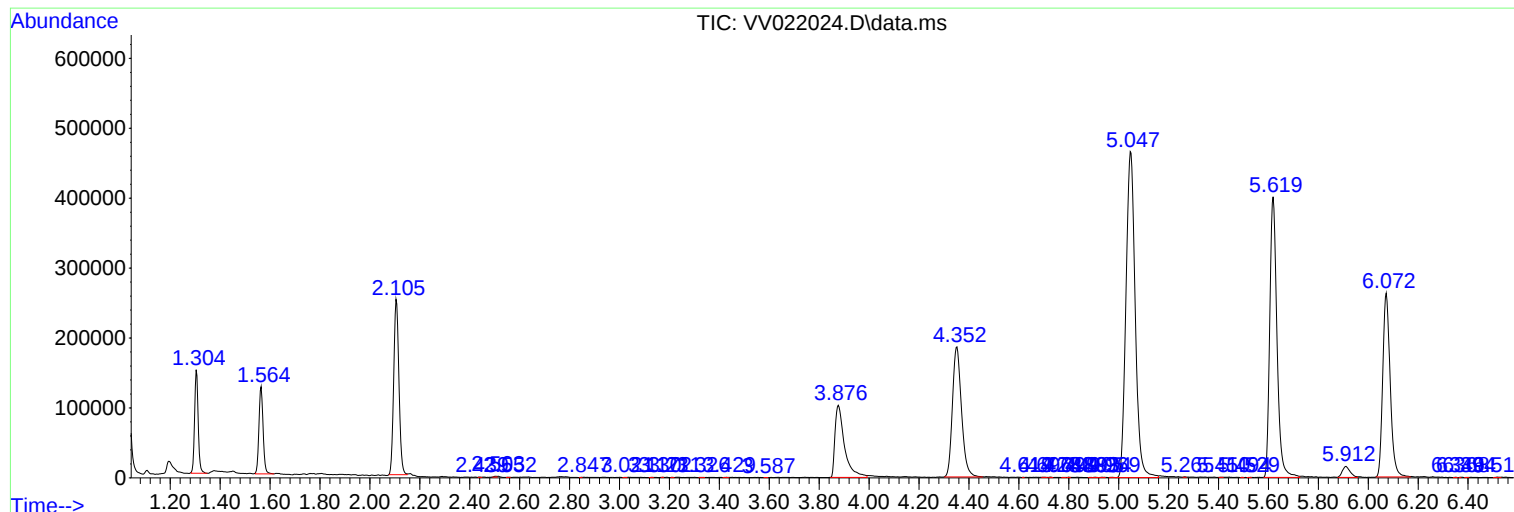

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022024.D
Acq On : 30 Aug 2021 23:54
Operator : SY/MD
Sample : M3566-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022024.D
Acq On : 30 Aug 2021 23:54
Operator : SY/MD
Sample : M3566-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKJ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
