

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022025.D
 Acq On : 31 Aug 2021 00:19
 Operator : SY/MD
 Sample : M3566-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022025.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	148538	150916	12.66%	1.597%
2	1.565	156	163	176	rVB	130980	146523	12.29%	1.550%
3	2.105	322	331	344	rBV	254124	364113	30.55%	3.853%
4	2.574	475	477	480	rBV2	344	167	0.01%	0.002%
5	2.680	508	510	512	rBV2	358	148	0.01%	0.002%
6	2.728	522	525	526	rBV2	460	221	0.02%	0.002%
7	2.828	551	556	557	rBV2	488	355	0.03%	0.004%
8	3.082	633	635	637	rBV	303	138	0.01%	0.001%
9	3.108	641	643	647	rVB2	362	209	0.02%	0.002%
10	3.130	647	650	653	rVB2	242	153	0.01%	0.002%
11	3.278	695	696	700	rBV2	249	150	0.01%	0.002%
12	3.327	708	711	712	rBV	400	235	0.02%	0.002%
13	3.362	719	722	725	rBV	231	146	0.01%	0.002%
14	3.564	782	785	791	rBV2	421	402	0.03%	0.004%
15	3.597	791	795	801	rVB3	413	397	0.03%	0.004%
16	3.638	804	808	811	rVB3	299	294	0.02%	0.003%
17	3.741	837	840	842	rBV	231	126	0.01%	0.001%
18	3.822	862	865	868	rBV	314	232	0.02%	0.002%
19	3.876	872	882	915	rBV	99858	267497	22.44%	2.830%
20	4.352	1014	1030	1056	rBV2	186901	471374	39.55%	4.988%
21	4.622	1111	1114	1115	rBV2	450	283	0.02%	0.003%
22	4.658	1122	1125	1128	rVB	446	276	0.02%	0.003%
23	4.735	1146	1149	1151	rBV3	548	319	0.03%	0.003%
24	4.748	1151	1153	1156	rBV2	216	141	0.01%	0.001%
25	4.889	1194	1197	1200	rBV	427	248	0.02%	0.003%
26	5.047	1229	1246	1277	rBV2	464181	1191966	100.00%	12.612%
27	5.542	1398	1400	1402	rBV	278	140	0.01%	0.001%
28	5.619	1412	1424	1451	rBV	402387	805717	67.60%	8.525%
29	5.908	1503	1514	1530	rBV	18695	39664	3.33%	0.420%
30	6.072	1551	1565	1593	rBV	263747	542161	45.48%	5.736%
31	6.297	1633	1635	1638	rBV	416	196	0.02%	0.002%
32	6.314	1638	1640	1643	rVB2	432	190	0.02%	0.002%
33	6.336	1645	1647	1649	rVV2	898	392	0.03%	0.004%
34	6.365	1653	1656	1657	rBV2	307	182	0.02%	0.002%
35	6.433	1673	1677	1678	rBV	213	140	0.01%	0.001%
36	6.449	1680	1682	1686	rBV2	379	278	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022025.D
 Acq On : 31 Aug 2021 00:19
 Operator : SY/MD
 Sample : M3566-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.523	1699	1705	1706	rBV4	604	522	0.04%	0.006%
38	6.555	1711	1715	1718	rBV4	246	205	0.02%	0.002%
39	6.593	1724	1727	1730	rBV2	268	225	0.02%	0.002%
40	6.622	1733	1736	1738	rBV	207	132	0.01%	0.001%
41	6.635	1738	1740	1742	rVB2	408	156	0.01%	0.002%
42	6.651	1742	1745	1747	rBV	516	351	0.03%	0.004%
43	6.703	1756	1761	1763	rBV	460	387	0.03%	0.004%
44	6.773	1780	1783	1784	rBV	530	198	0.02%	0.002%
45	6.812	1792	1795	1797	rVB	301	147	0.01%	0.002%
46	6.905	1821	1824	1827	rBV2	285	193	0.02%	0.002%
47	6.989	1839	1850	1875	rBV	135206	249256	20.91%	2.637%
48	7.317	1941	1952	1972	rBV	568699	981483	82.34%	10.385%
49	7.625	2037	2048	2073	rBV	91395	164963	13.84%	1.745%
50	7.908	2133	2136	2139	rBV3	347	221	0.02%	0.002%
51	7.937	2139	2145	2155	rBV2	1217	2132	0.18%	0.023%
52	8.047	2176	2179	2180	rBV2	233	139	0.01%	0.001%
53	8.092	2182	2193	2221	rBV2	294087	560168	47.00%	5.927%
54	8.429	2296	2298	2301	rBV2	450	223	0.02%	0.002%
55	8.606	2351	2353	2354	rBV	347	199	0.02%	0.002%
56	8.670	2370	2373	2374	rBV	533	277	0.02%	0.003%
57	8.796	2408	2412	2417	rVB2	357	336	0.03%	0.004%
58	8.854	2418	2430	2459	rBV	601007	993567	83.36%	10.513%
59	9.133	2512	2517	2518	rBV4	441	311	0.03%	0.003%
60	9.204	2537	2539	2542	rVB2	310	141	0.01%	0.001%
61	9.333	2577	2579	2582	rVB2	345	150	0.01%	0.002%
62	9.506	2631	2633	2635	rBV	466	219	0.02%	0.002%
63	9.545	2642	2645	2647	rBV2	320	165	0.01%	0.002%
64	9.651	2674	2678	2681	rBV2	308	197	0.02%	0.002%
65	9.712	2694	2697	2701	rBV	354	276	0.02%	0.003%
66	9.764	2712	2713	2717	rVB2	306	162	0.01%	0.002%
67	9.844	2735	2738	2739	rBV	262	161	0.01%	0.002%
68	9.873	2743	2747	2749	rBV	319	249	0.02%	0.003%
69	10.130	2821	2827	2835	rBV4	1656	2363	0.20%	0.025%
70	10.220	2843	2855	2877	rBV	358498	577272	48.43%	6.108%
71	10.464	2929	2931	2933	rBV	436	165	0.01%	0.002%
72	10.529	2947	2951	2952	rBV2	323	200	0.02%	0.002%
73	10.619	2977	2979	2981	rVB	410	128	0.01%	0.001%
74	10.693	2997	3002	3005	rBV3	495	482	0.04%	0.005%
75	10.809	3036	3038	3044	rBV2	428	325	0.03%	0.003%
76	10.837	3044	3047	3052	rVB2	428	339	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV022025.D
 Acq On : 31 Aug 2021 00:19
 Operator : SY/MD
 Sample : M3566-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.924	3066	3074	3082	rBV5	1714	2736	0.23%	0.029%
78	11.024	3102	3105	3108	rBV	451	349	0.03%	0.004%
79	11.127	3134	3137	3140	rBV	206	141	0.01%	0.001%
80	11.153	3140	3145	3151	rVV5	751	838	0.07%	0.009%
81	11.252	3164	3176	3199	rBV	630275	986900	82.80%	10.442%
82	11.484	3245	3248	3253	rVB4	620	443	0.04%	0.005%
83	11.509	3253	3256	3261	rVB2	610	368	0.03%	0.004%
84	11.558	3268	3271	3274	rBV3	528	355	0.03%	0.004%
85	11.625	3280	3292	3319	rBV	580296	929785	78.00%	9.838%
86	11.812	3346	3350	3356	rBV4	589	527	0.04%	0.006%
87	12.014	3410	3413	3416	rBV2	377	280	0.02%	0.003%
88	12.034	3416	3419	3421	rBV	306	184	0.02%	0.002%
89	12.210	3471	3474	3476	rBV2	350	199	0.02%	0.002%
90	12.268	3488	3492	3497	rVB3	433	351	0.03%	0.004%
91	12.291	3497	3499	3501	rBV	261	164	0.01%	0.002%
92	12.365	3519	3522	3525	rBB	368	201	0.02%	0.002%
93	12.519	3568	3570	3574	rVB2	301	146	0.01%	0.002%
94	12.622	3600	3602	3606	rVB	491	288	0.02%	0.003%
95	12.882	3680	3683	3685	rBV	242	161	0.01%	0.002%
96	13.435	3848	3855	3857	rBV	421	480	0.04%	0.005%
97	13.902	3994	4000	4002	rBV2	530	591	0.05%	0.006%
98	14.043	4042	4044	4046	rBV	419	205	0.02%	0.002%
99	14.230	4100	4102	4107	rVB2	637	323	0.03%	0.003%
100	15.030	4349	4351	4352	rBV2	484	188	0.02%	0.002%




Sum of corrected areas: 9451077

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022025.D
Acq On : 31 Aug 2021 00:19
Operator : SY/MD
Sample : M3566-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

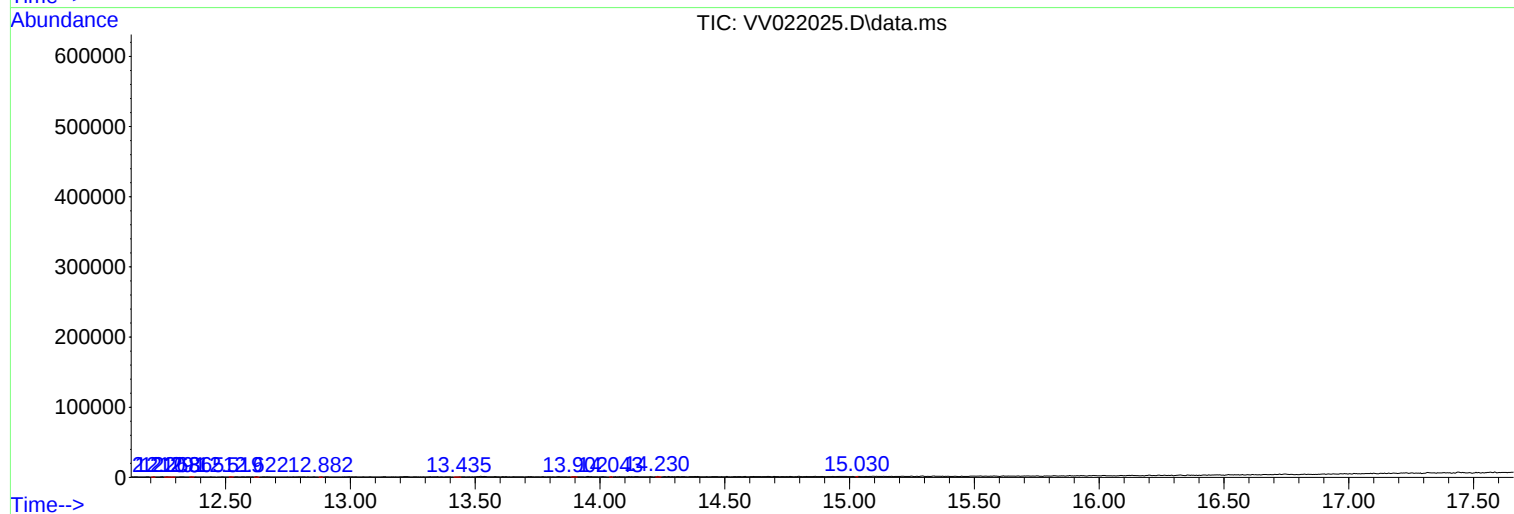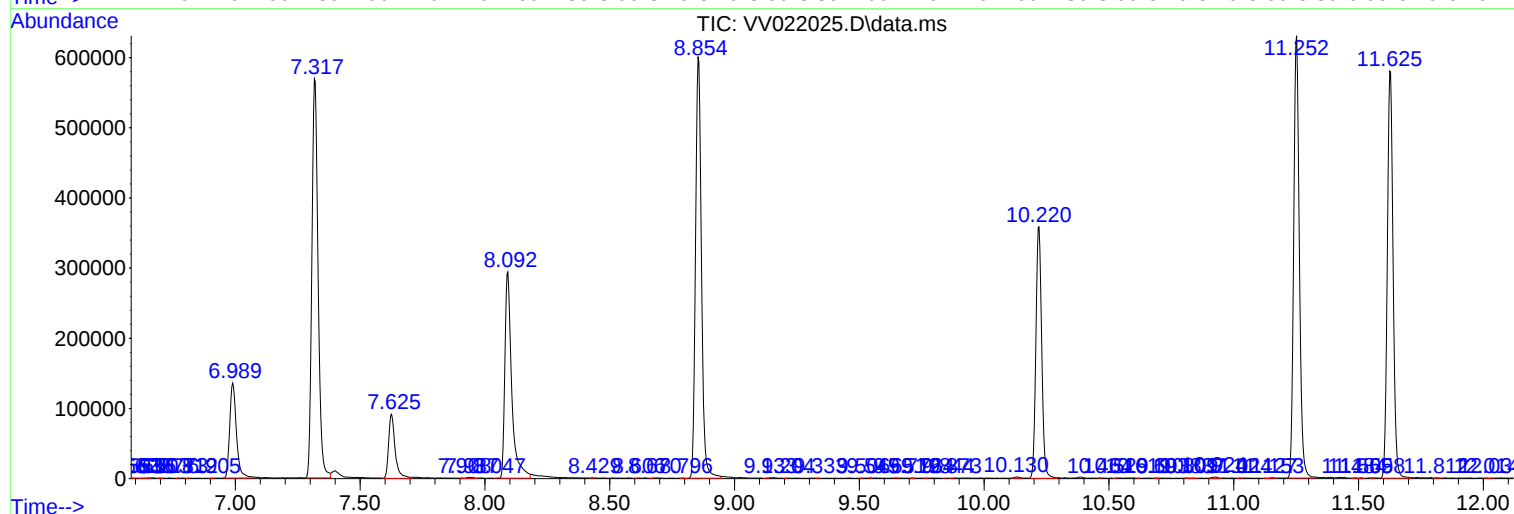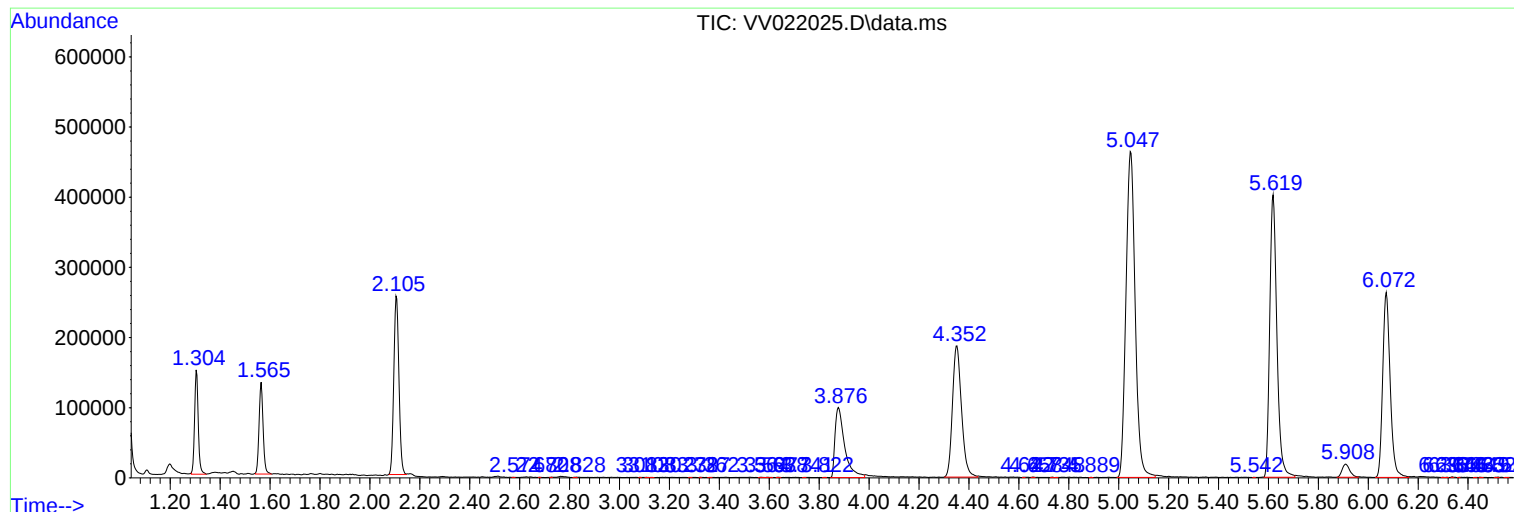

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022025.D
Acq On : 31 Aug 2021 00:19
Operator : SY/MD
Sample : M3566-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
Data File : VV022025.D
Acq On : 31 Aug 2021 00:19
Operator : SY/MD
Sample : M3566-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
