


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083021\
 Data File : VV021990.D
 Acq On : 30 Aug 2021 09:00
 Operator : SY/MD
 Sample : BFB224
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB224

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis
 Last Update : Tue Aug 31 04:25:57 2021

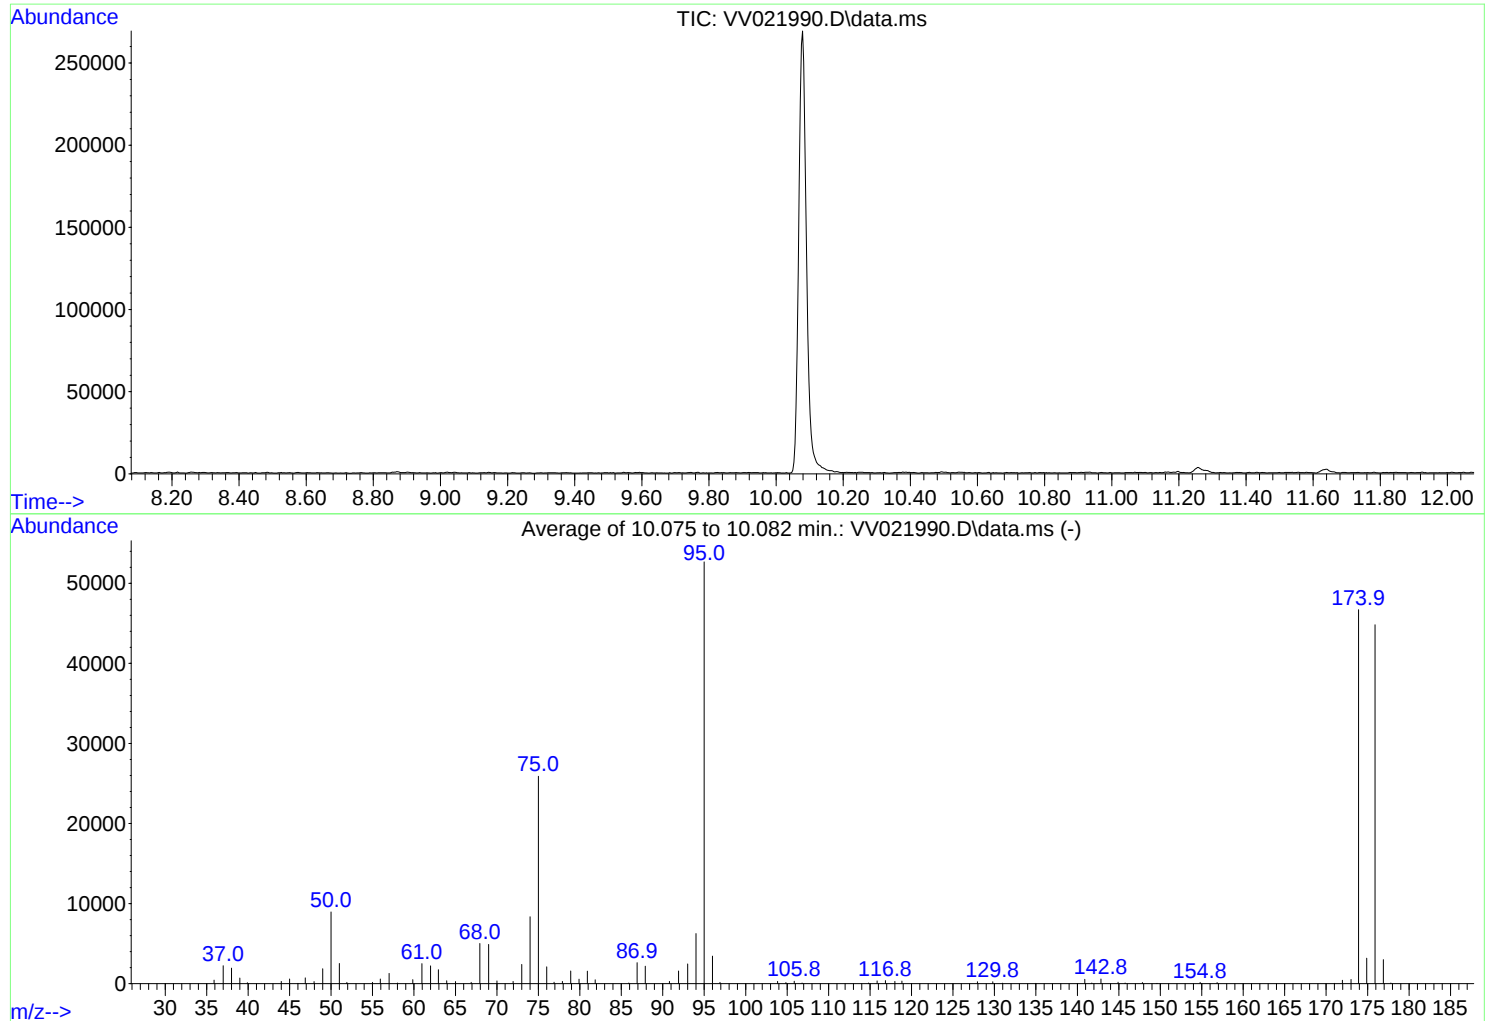

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	8946	PASS
75	95	30	80	49.2	25901	PASS
95	95	100	100	100.0	52680	PASS
96	95	5	9	6.5	3441	PASS
173	174	0.00	2	1.1	516	PASS
174	95	50	120	88.6	46699	PASS
175	174	5	9	6.8	3187	PASS
176	174	95	105	96.0	44816	PASS
177	176	5	10	6.7	3001	PASS

m/z	Abundance
35.90	460.0
37.00	2386.0
38.00	1982.0
39.00	711.0
39.90	309.0
44.00	675.0
45.00	654.0
46.90	772.0
47.90	252.0
49.00	1920.0
50.00	9226.0
51.00	2582.0
51.90	162.0
55.00	148.0
55.90	589.0
57.00	1289.0
58.00	110.0
59.90	507.0
60.90	2581.0
62.00	2239.0
62.90	1772.0
63.90	386.0
65.00	276.0
66.90	171.0
67.90	5140.0
69.00	5047.0
70.00	375.0
72.00	280.0
73.00	2501.0
74.00	8633.0
75.00	26872.0
76.00	2158.0
76.80	184.0
77.90	278.0
78.90	1623.0
79.90	574.0
80.90	1597.0
81.80	493.0
85.90	133.0
86.90	2758.0
87.90	2227.0
90.80	296.0
91.90	1596.0
93.00	2560.0
94.00	6518.0
95.00	54512.0
96.00	3570.0
96.90	138.0
103.90	292.0
104.80	141.0
105.90	299.0
106.80	118.0
114.80	110.0
115.90	358.0
116.90	405.0
118.00	302.0
118.80	318.0
127.90	260.0
129.80	257.0
131.00	101.0
140.90	564.0
141.70	107.0
142.80	611.0
144.90	210.0
145.70	105.0
147.80	133.0
154.80	169.0
156.90	150.0
172.00	441.0
173.00	522.0
173.90	48376.0
174.90	3274.0
175.90	46392.0
176.90	3124.0
177.80	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

m/z	Abundance
35.90	394.0
37.00	2128.0
38.00	1674.0
39.00	730.0
39.90	284.0
44.00	596.0
45.00	558.0
46.00	107.0
46.90	707.0
48.00	254.0
49.00	1675.0
50.00	8601.0
51.00	2433.0
51.90	137.0
54.90	179.0
56.00	526.0
57.00	1302.0
58.00	113.0
59.80	451.0
61.00	2381.0
62.00	2286.0
62.90	1670.0
64.00	352.0
65.00	257.0
66.90	188.0
67.90	4746.0
69.00	4751.0
70.00	332.0
72.00	315.0
73.00	2301.0
74.00	7744.0
75.00	24688.0
76.00	1999.0
77.00	185.0
77.90	306.0
78.90	1533.0
79.90	518.0
80.90	1427.0
81.80	470.0
85.90	119.0
86.90	2400.0
87.90	2030.0
90.80	274.0
91.90	1511.0
93.00	2407.0
94.00	5743.0
95.00	49928.0
96.00	3213.0
96.90	105.0
97.00	104.0
103.90	286.0
104.80	129.0
105.90	327.0
106.80	129.0
114.80	162.0
115.80	264.0
116.80	359.0
118.00	314.0
118.90	309.0
128.00	217.0
129.80	201.0
130.90	113.0
140.90	557.0
141.80	134.0
142.80	619.0
144.90	198.0
147.80	149.0
154.80	139.0
156.80	129.0
171.90	411.0
173.00	517.0
173.90	46256.0
174.90	2973.0
175.90	43648.0
176.90	2955.0
177.80	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

Scan 2799 (10.040 min): VV021990.D\data.ms
BFB224

m/z	Abundance
40.00	180.0
44.00	363.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224

m/z	Abundance
35.90	464.0
37.00	2199.0
38.00	2134.0
39.00	681.0
39.90	304.0
44.00	689.0
45.00	546.0
46.90	715.0
47.90	268.0
49.00	2011.0
50.00	9012.0
51.00	2558.0
51.90	183.0
55.10	150.0
55.90	611.0
57.00	1229.0
59.90	555.0
60.90	2542.0
62.00	2134.0
63.00	1793.0
63.90	350.0
65.00	242.0
66.90	136.0
68.00	5167.0
69.00	4911.0
70.00	345.0
71.90	247.0
73.00	2420.0
74.00	8691.0
75.00	26144.0
76.00	2130.0
76.90	194.0
77.90	244.0
78.90	1588.0
79.90	596.0
80.90	1654.0
81.90	483.0
86.90	2706.0
87.90	2299.0
90.80	265.0
91.90	1609.0
93.00	2404.0
94.00	6480.0
95.00	53600.0
96.00	3541.0
96.90	158.0
103.80	254.0
104.90	134.0
105.80	260.0
115.90	400.0
116.80	409.0
118.00	215.0
118.90	320.0
127.90	233.0
129.80	263.0
135.00	109.0
140.90	530.0
142.90	540.0
144.90	152.0
145.80	137.0
148.00	130.0
149.60	109.0
154.80	168.0
156.90	155.0
171.00	107.0
172.00	434.0
173.00	509.0
173.90	45464.0
174.90	3315.0
175.90	44408.0
176.90	2923.0

Instrument :
MSVOA_V
ClientSampleId :
BFB224