




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027583.D
 Acq On : 30 Aug 2022 14:00
 Operator : SY/MD
 Sample : N4367-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 31 04:47:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 31 04:45:39 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

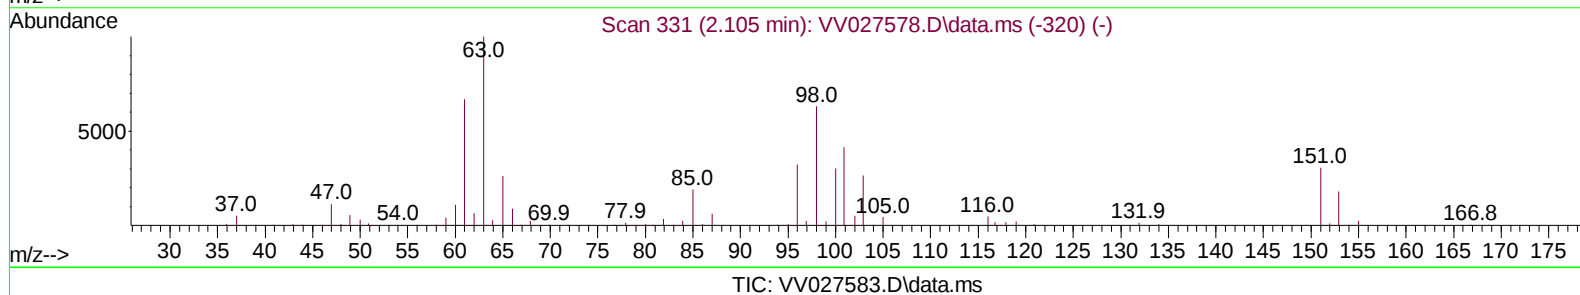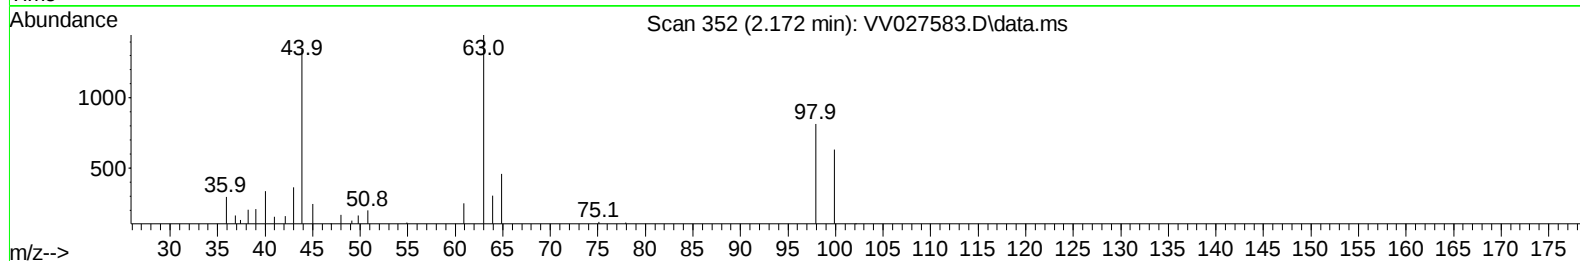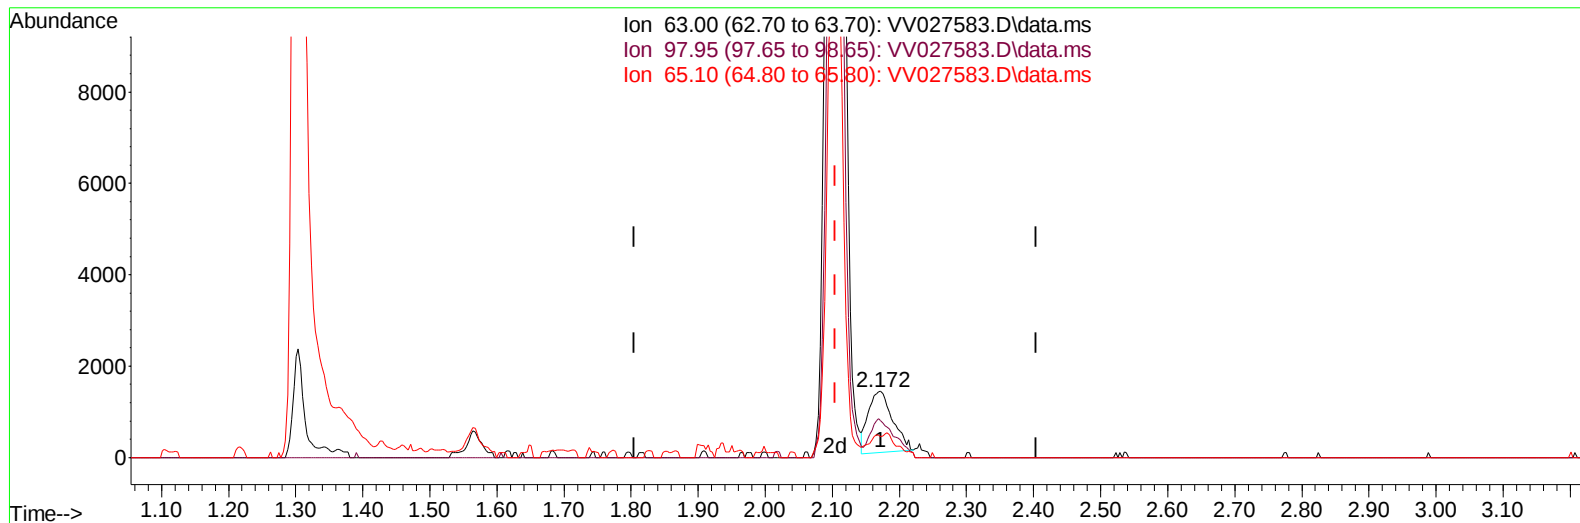

TIC: VV027583.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.172min (+ 0.067) 0.15 ug/L

response 3399

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	63.40
65.10	22.40	21.62
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027583.D
 Acq On : 30 Aug 2022 14:00
 Operator : SY/MD
 Sample : N4367-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 31 04:47:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 31 04:45:39 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

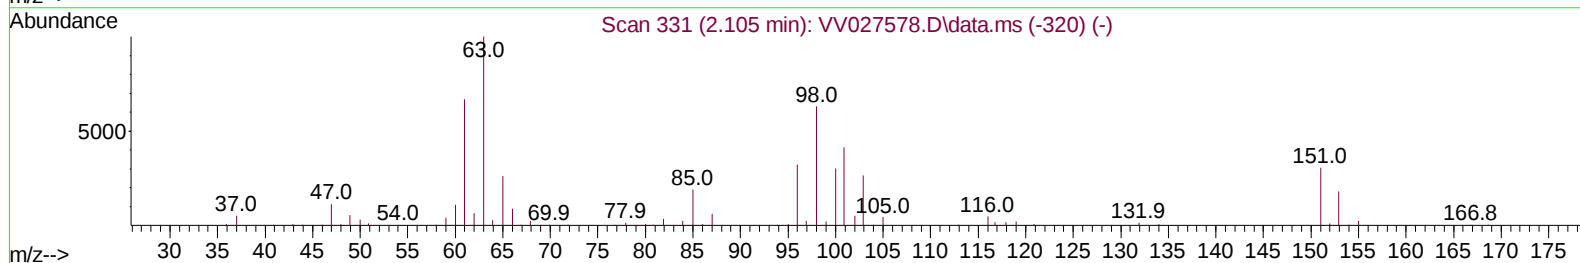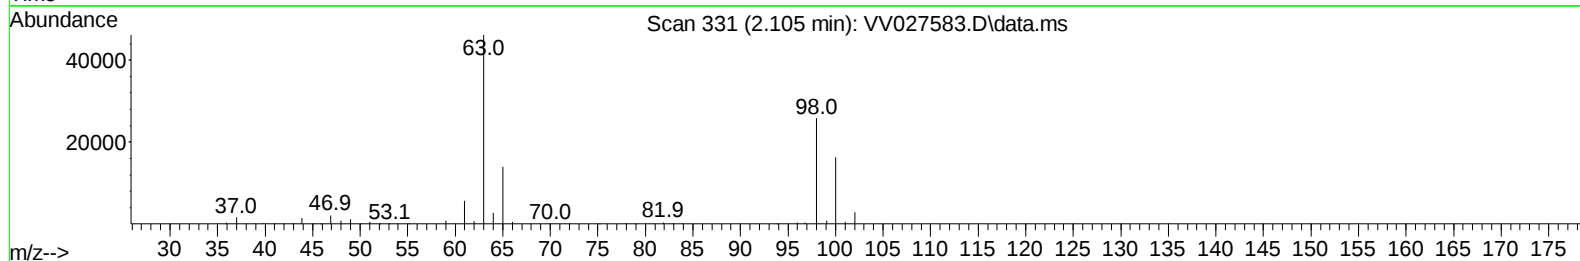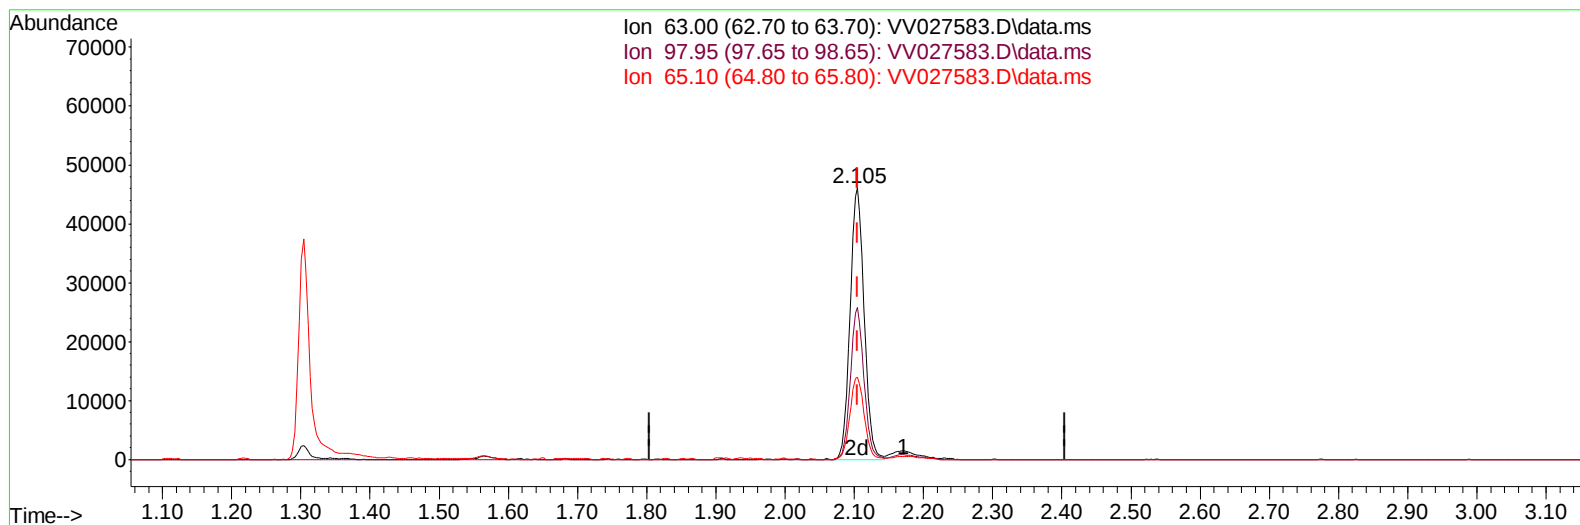

TIC: VV027583.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.105min (-0.000) 2.84 ug/L m

response 65665

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	3.28#
65.10	22.40	1.12#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027583.D
 Acq On : 30 Aug 2022 14:00
 Operator : SY/MD
 Sample : N4367-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 31 04:47:57 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 31 04:45:39 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.616	114		139371	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		138973	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		57151	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		45261	4.563	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.200%	
7) Chloroethane-d5	1.564	69		39209	5.401	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.000%	
11) 1,1-Dichloroethene-d2	2.105	63		65665m	2.839	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.800%#	
20) 2-Butanone-d5	3.895	46		57719	46.758	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.520%	
24) Chloroform-d	4.346	84		93304	4.704	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%	
26) 1,2-Dichloroethane-d4	5.030	65		44617	5.200	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.000%	
32) Benzene-d6	5.047	84		167313	4.347	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.000%	
36) 1,2-Dichloropropane-d6	6.069	67		54917	4.907	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.200%	
41) Toluene-d8	7.317	98		120506	3.467	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	69.400%#	
43) trans-1,3-Dichloroprop...	7.625	79		15016	3.919	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.400%	
46) 2-Hexanone-d5	8.091	63		56508	44.799	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.600%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		33587	4.713	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152		38672	4.565	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.200%	
Target Compounds							
16) Methylene chloride	2.503	84		13752	0.865	ug/L	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027583.D
Acq On : 30 Aug 2022 14:00
Operator : SY/MD
Sample : N4367-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 31 04:47:57 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Aug 31 04:45:39 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022

