




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027584.D
 Acq On : 30 Aug 2022 14:24
 Operator : SY/MD
 Sample : N4368-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F06

Manual IntegrationsAPPROVED

Quant Time: Aug 31 04:48:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 31 04:45:39 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

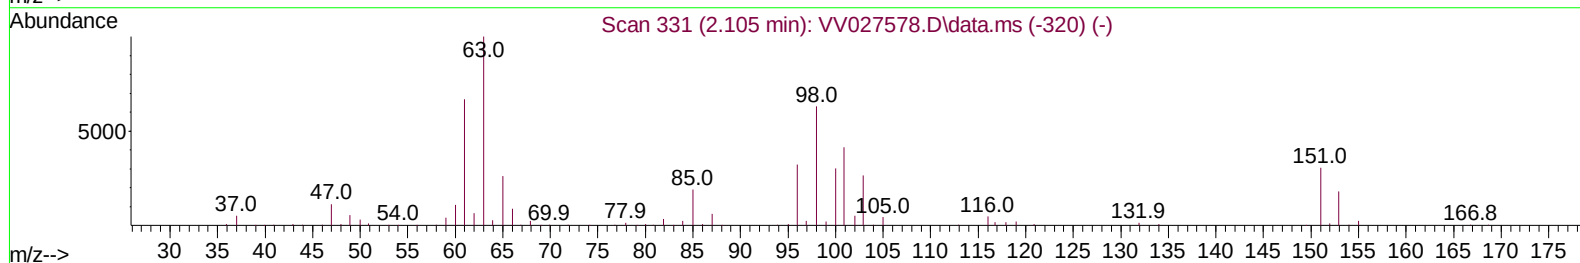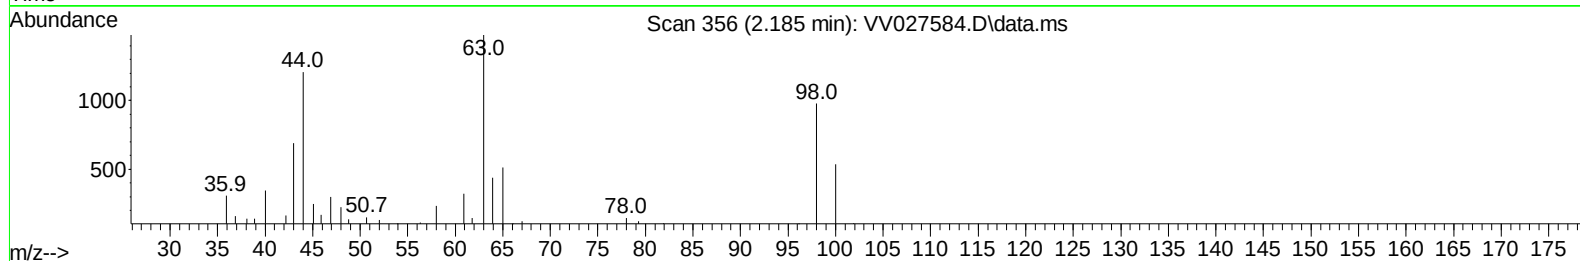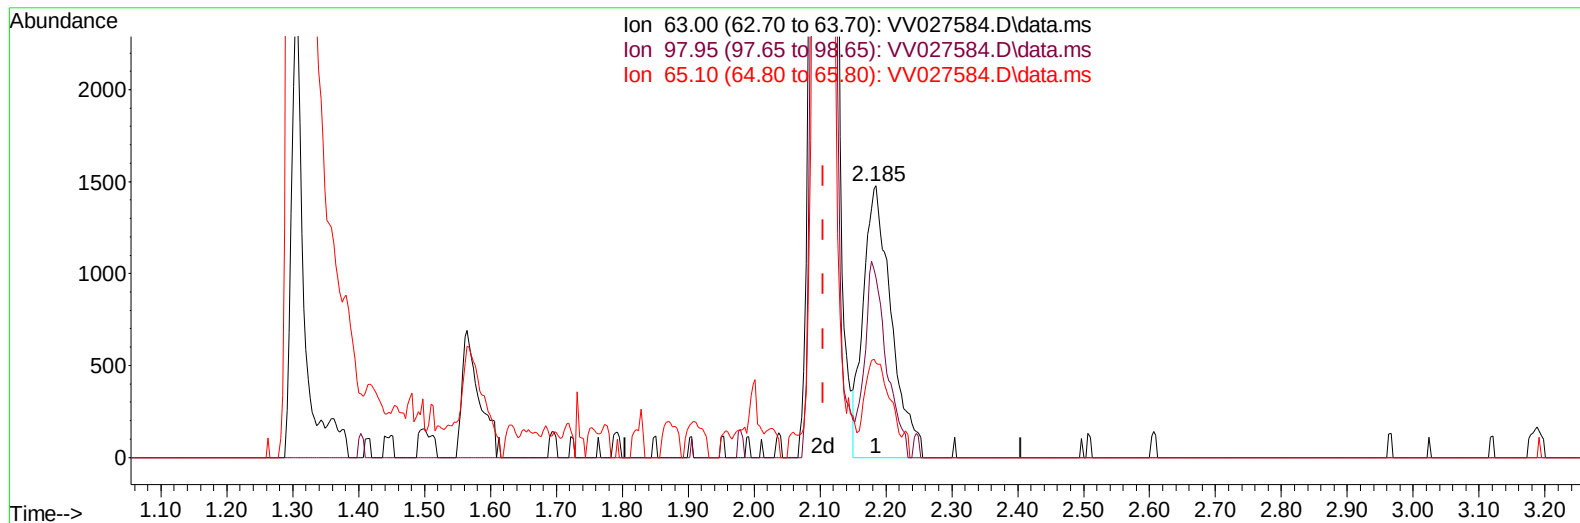

TIC: VV027584.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.185min (+ 0.080) 0.17 ug/L

response 4355

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	55.96
65.10	22.40	22.73
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027584.D
 Acq On : 30 Aug 2022 14:24
 Operator : SY/MD
 Sample : N4368-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F06

Manual IntegrationsAPPROVED

Quant Time: Aug 31 04:48:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 31 04:45:39 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

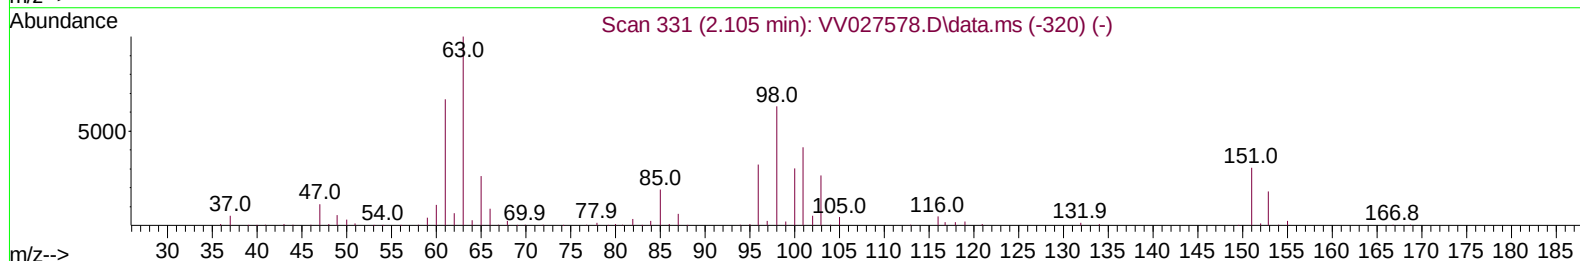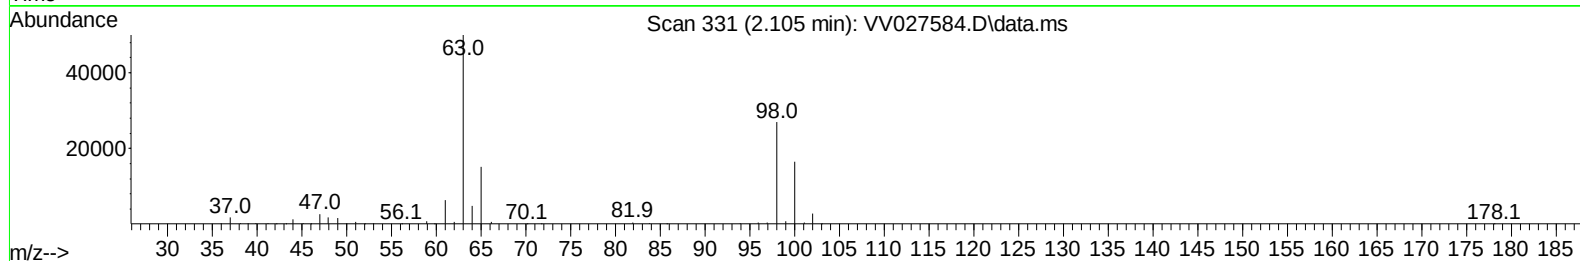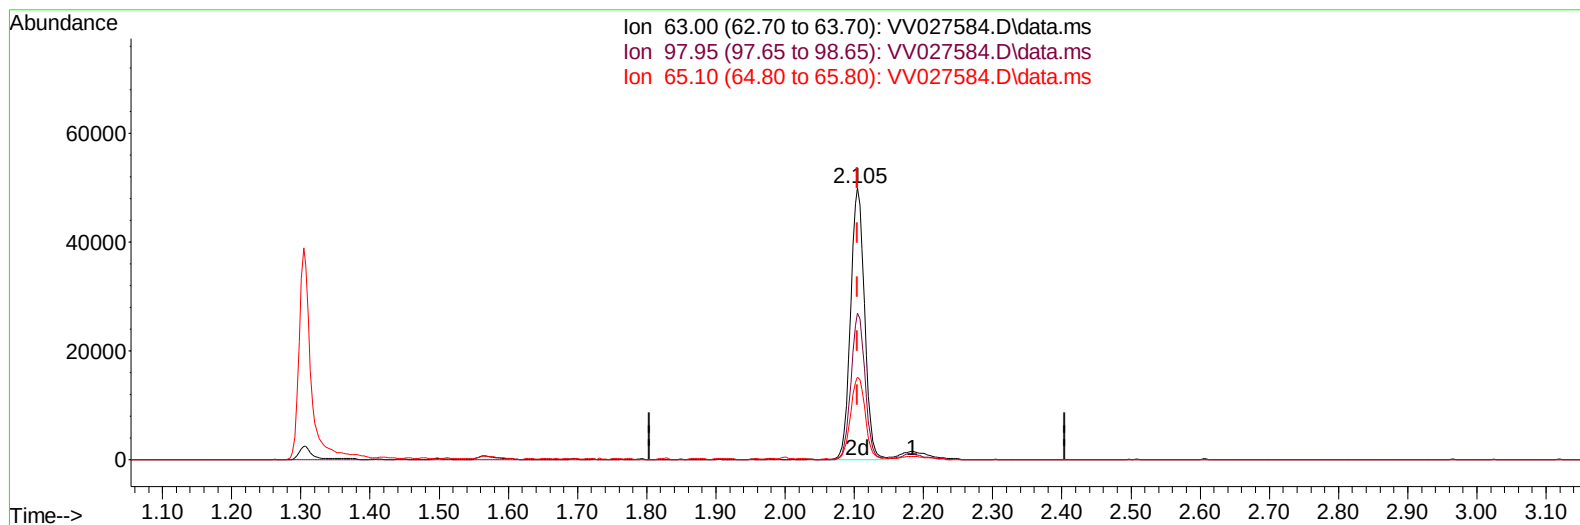

TIC: VV027584.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.105min (+ 0.000) 2.80 ug/L m

response 69960

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	3.48#
65.10	22.40	1.42#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027584.D
 Acq On : 30 Aug 2022 14:24
 Operator : SY/MD
 Sample : N4368-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5F06

Manual IntegrationsAPPROVED

Quant Time: Aug 31 04:48:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 31 04:45:39 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	150782	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	149645	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	59617	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	47070	4.386	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	87.800%		
7) Chloroethane-d5	1.564	69	40147	5.112	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	102.200%		
11) 1,1-Dichloroethene-d2	2.105	63	69960m	2.796	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	56.000%#		
20) 2-Butanone-d5	3.899	46	66548	49.830	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	99.660%		
24) Chloroform-d	4.349	84	99031	4.615	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	92.400%		
26) 1,2-Dichloroethane-d4	5.034	65	45575	4.910	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	98.200%		
32) Benzene-d6	5.047	84	179975	4.342	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	86.800%		
36) 1,2-Dichloropropane-d6	6.069	67	60801	5.045	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	101.000%		
41) Toluene-d8	7.317	98	134692	3.599	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	72.000%		
43) trans-1,3-Dichloroprop...	7.625	79	16180	3.921	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	78.400%		
46) 2-Hexanone-d5	8.092	63	64869	47.760	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	95.520%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	39919	5.202	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	104.000%		
66) 1,2-Dichlorobenzene-d4	11.622	152	44100	4.990	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	99.800%		
Target Compounds						
30) Cyclohexane	4.680	56	9150	0.519	ug/L	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027584.D
Acq On : 30 Aug 2022 14:24
Operator : SY/MD
Sample : N4368-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5F06

Manual IntegrationsAPPROVED

Quant Time: Aug 31 04:48:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Aug 31 04:45:39 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022

