




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027587.D
 Acq On : 30 Aug 2022 15:38
 Operator : SY/MD
 Sample : N4368-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 31 04:48:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 31 04:45:39 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

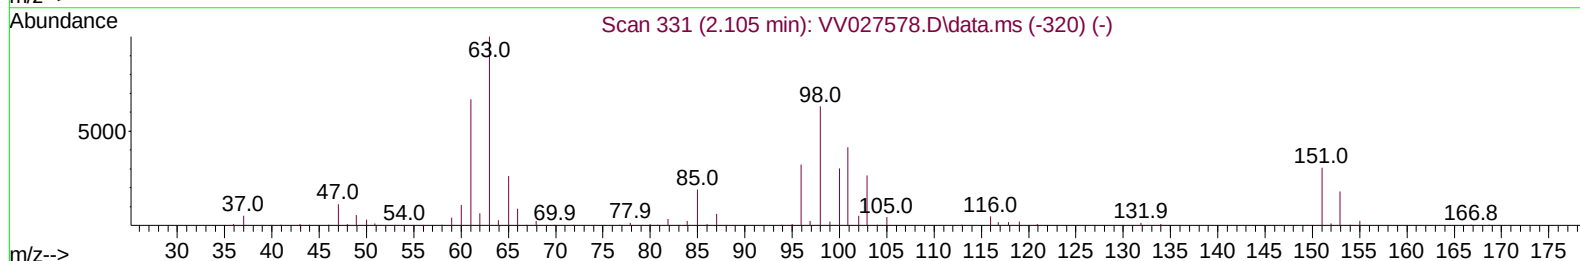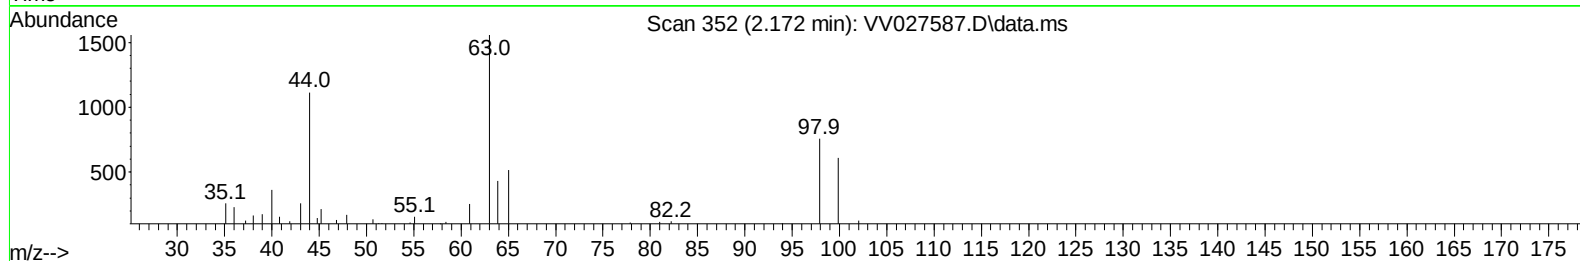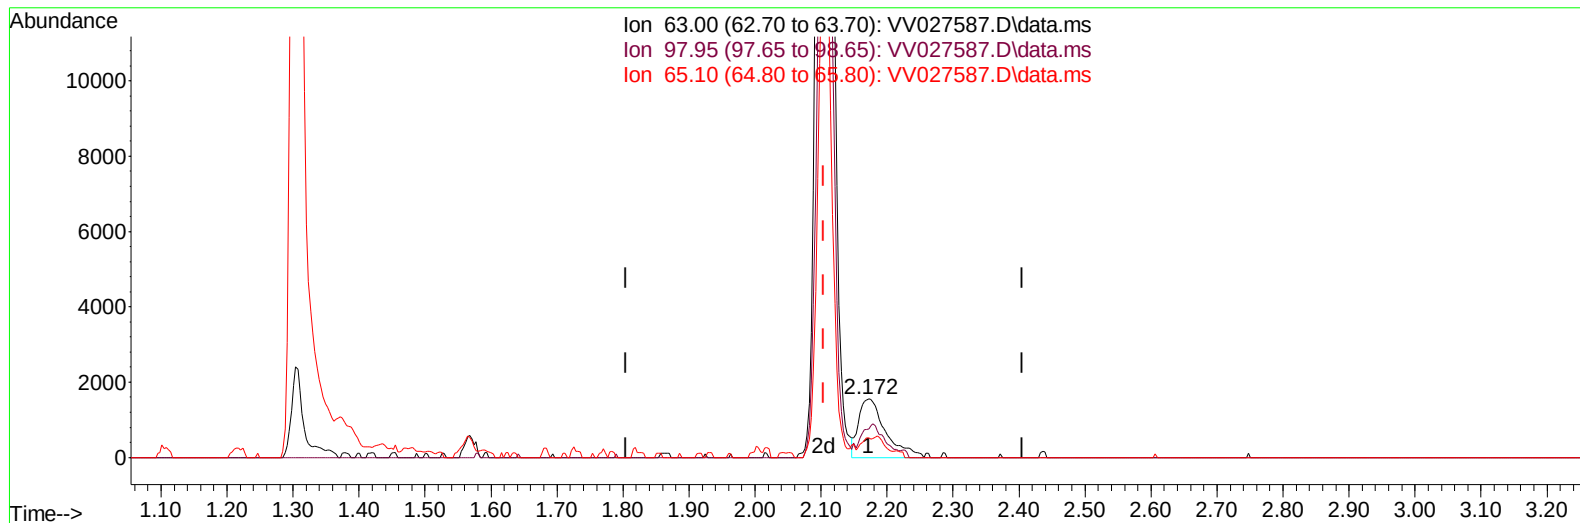

TIC: VV027587.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.172min (+ 0.068) 0.18 ug/L

response 4398

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	53.14
65.10	22.40	17.99
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027587.D
Acq On : 30 Aug 2022 15:38
Operator : SY/MD
Sample : N4368-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 31 04:48:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Aug 31 04:45:39 2022
Response via : Initial Calibration

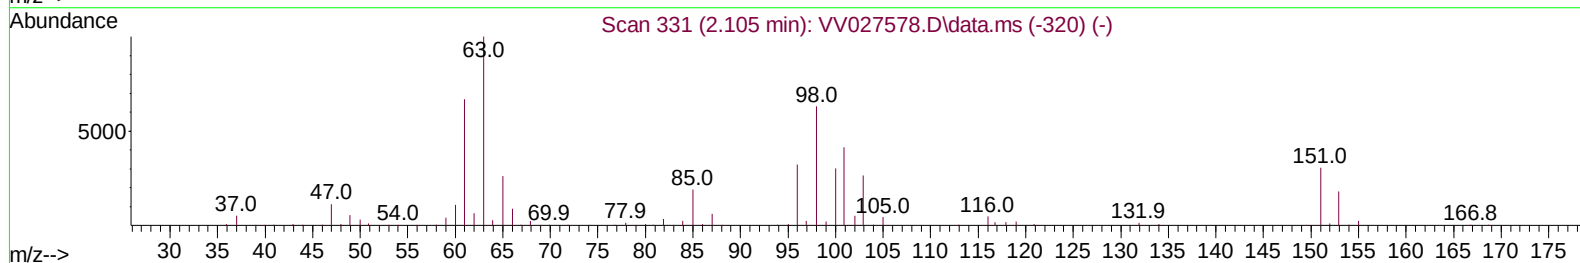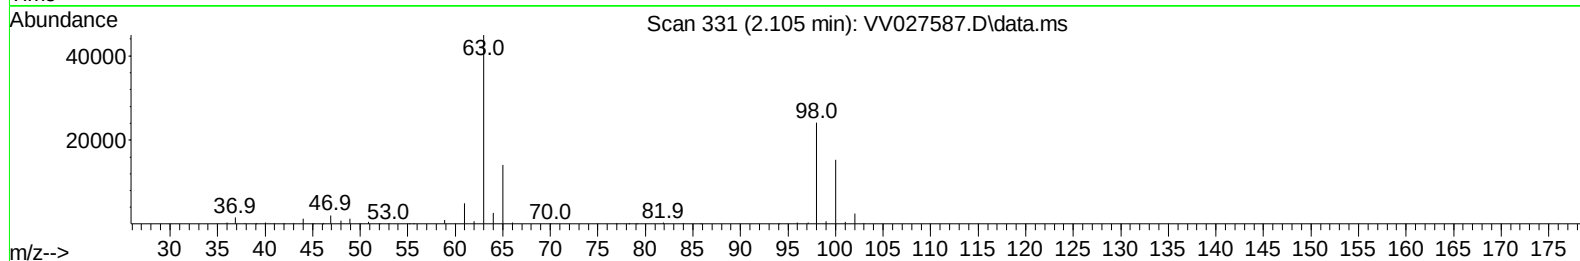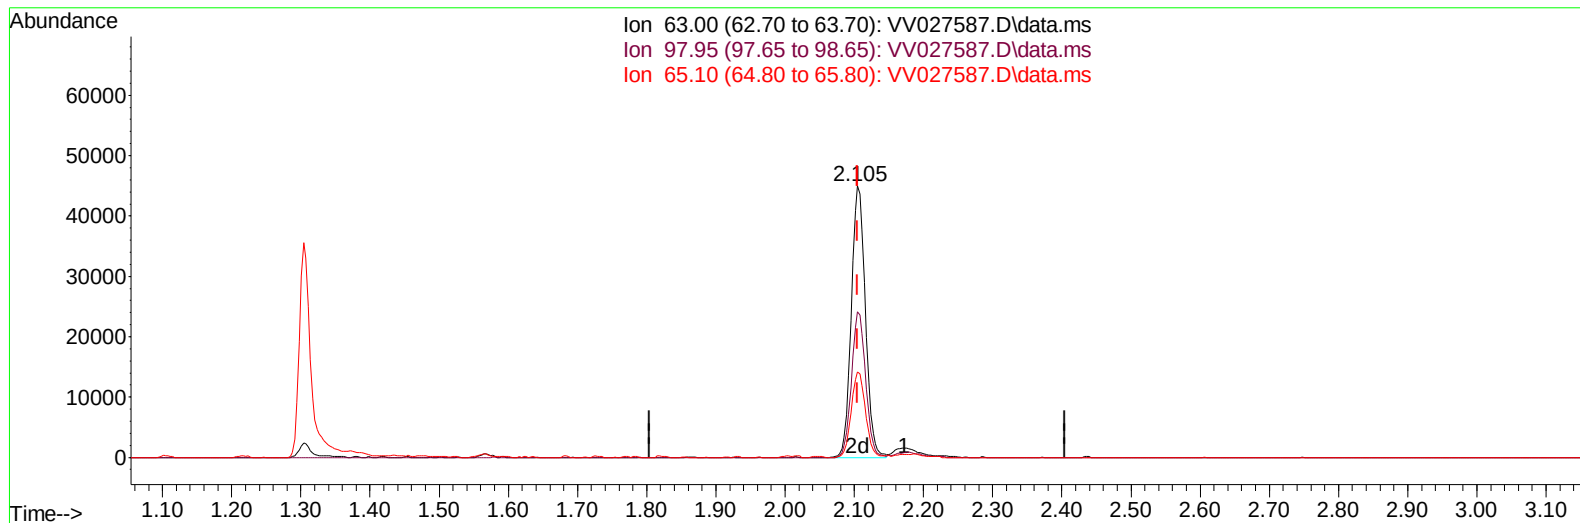

TIC: VV027587.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.105min (+ 0.000) 2.61 ug/L m

response 63270

Ion	Exp%	Act%
63.00	100.00	100.00
97.95	70.00	3.69#
65.10	22.40	1.25#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027587.D
 Acq On : 30 Aug 2022 15:38
 Operator : SY/MD
 Sample : N4368-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Quant Time: Aug 31 04:48:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 31 04:45:39 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.616	114		145810	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		146136	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		57347	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		41765	4.025	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.400%	
7) Chloroethane-d5	1.565	69		36741	4.838	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	96.800%	
11) 1,1-Dichloroethene-d2	2.105	63		63270m	2.615	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	52.200%#	
20) 2-Butanone-d5	3.899	46		63478	49.152	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.300%	
24) Chloroform-d	4.349	84		91362	4.403	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.000%	
26) 1,2-Dichloroethane-d4	5.034	65		43628	4.860	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.200%	
32) Benzene-d6	5.050	84		164392	4.061	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.200%	
36) 1,2-Dichloropropane-d6	6.069	67		54731	4.651	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.000%	
41) Toluene-d8	7.317	98		118925	3.254	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	65.000%#	
43) trans-1,3-Dichloroprop...	7.629	79		15134	3.756	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.200%	
46) 2-Hexanone-d5	8.092	63		57666	43.476	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.960%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84		36166	4.826	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152		39989	4.704	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.000%	
Target Compounds							
16) Methylene chloride	2.507	84		20365	1.224	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027587.D
Acq On : 30 Aug 2022 15:38
Operator : SY/MD
Sample : N4368-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Aug 31 04:48:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Aug 31 04:45:39 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022

