




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027597.D
 Acq On : 30 Aug 2022 19:44
 Operator : SY/MD
 Sample : N4400-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVP1

Manual IntegrationsAPPROVED

Quant Time: Aug 31 04:51:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 31 04:45:39 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

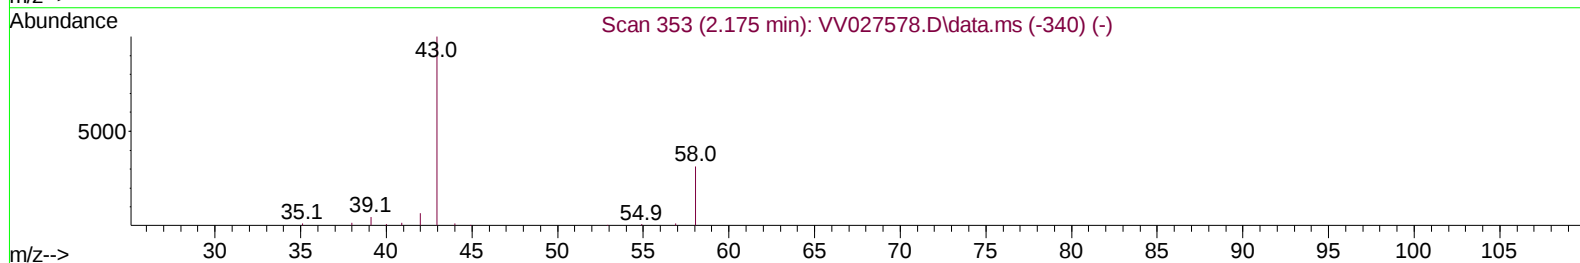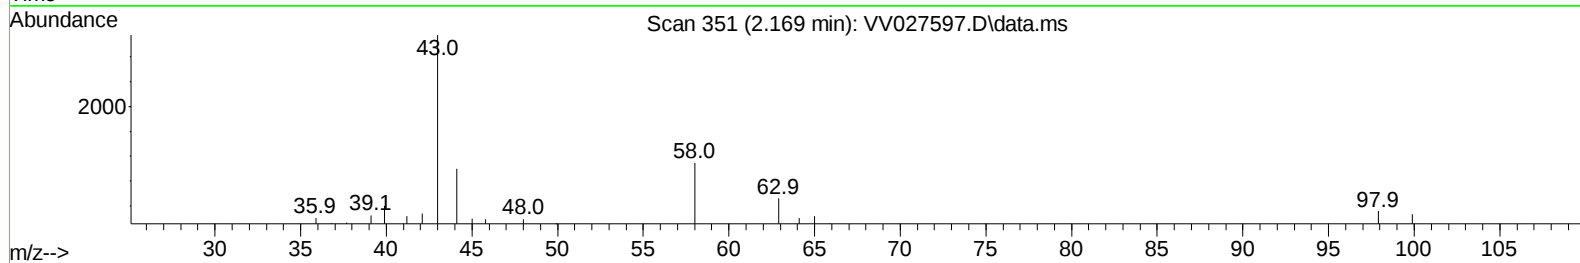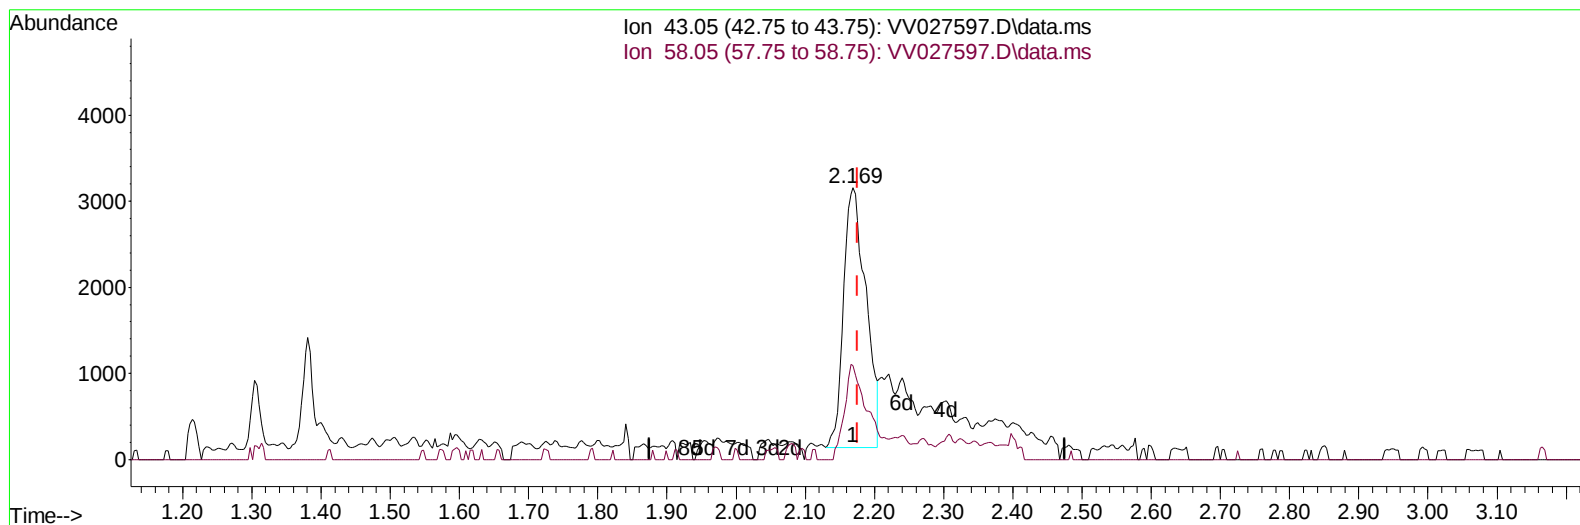

TIC: VV027597.D\data.ms

(13) Acetone (T)

2.169min (-0.006) 5.87 ug/L

response 6807

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	31.10	38.58
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027597.D
 Acq On : 30 Aug 2022 19:44
 Operator : SY/MD
 Sample : N4400-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVP1

Manual IntegrationsAPPROVED

Quant Time: Aug 31 04:51:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 31 04:45:39 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

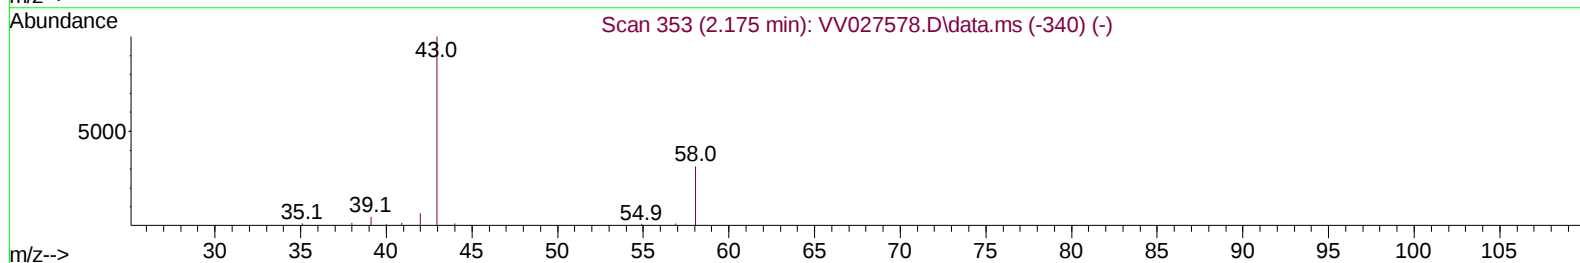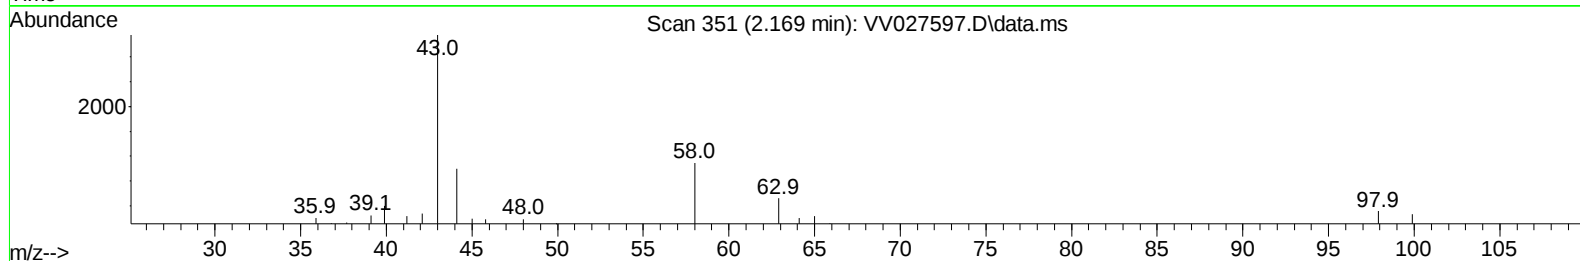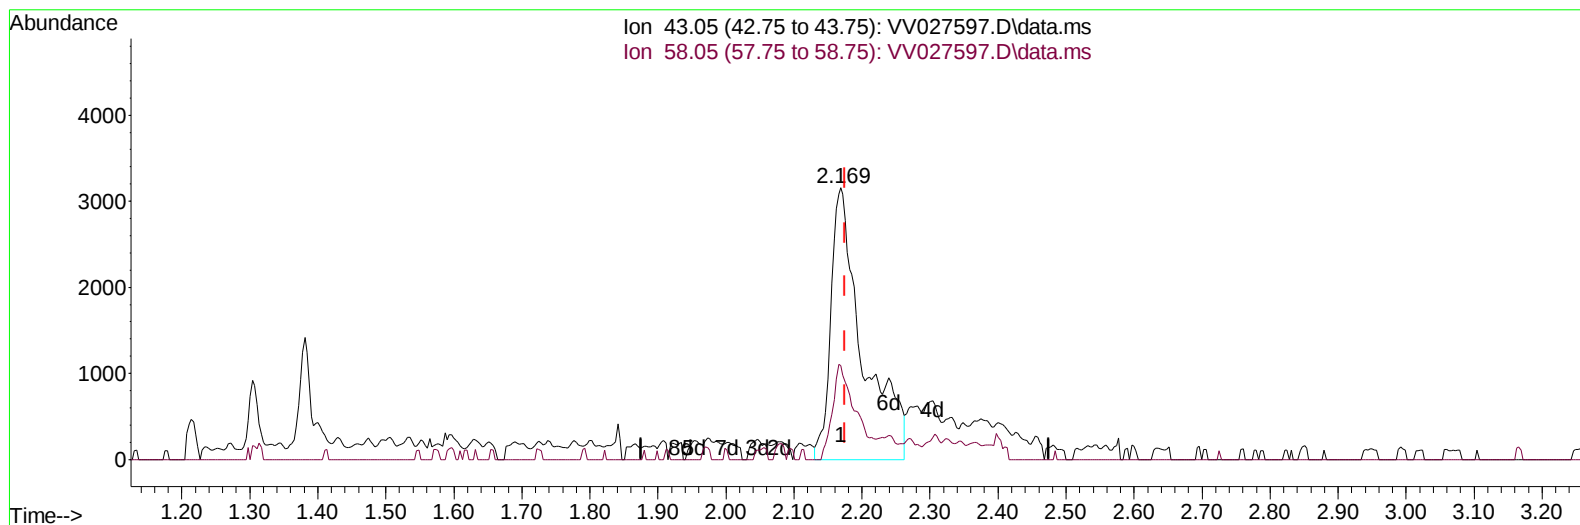

TIC: VV027597.D\data.ms

(13) Acetone (T)

2.169min (-0.006) 8.86 ug/L m

response 10267

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	31.10	25.58
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027597.D
 Acq On : 30 Aug 2022 19:44
 Operator : SY/MD
 Sample : N4400-22
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBVP1

Manual IntegrationsAPPROVED

Quant Time: Aug 31 04:51:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 31 04:45:39 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
 Supervised By :Mahesh Dadoda 08/31/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.616	114		136980	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117		140910	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		55899	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.304	65		45658	4.683	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	93.600%	
7) Chloroethane-d5	1.564	69		37901	5.312	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.200%	
11) 1,1-Dichloroethene-d2	2.105	63		64651	2.844	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.800%#	
20) 2-Butanone-d5	3.895	46		52771	43.496	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.000%	
24) Chloroform-d	4.346	84		90750	4.655	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%	
26) 1,2-Dichloroethane-d4	5.034	65		41383	4.907	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.200%	
32) Benzene-d6	5.047	84		164984	4.227	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.600%	
36) 1,2-Dichloropropane-d6	6.069	67		54769	4.827	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.600%	
41) Toluene-d8	7.317	98		121239	3.440	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.800%#	
43) trans-1,3-Dichloroprop...	7.628	79		13335	3.432	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.600%	
46) 2-Hexanone-d5	8.091	63		57124	44.665	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.320%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84		35912	4.970	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152		42108	5.082	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.600%	
Target Compounds							
13) Acetone	2.169	43		10267m	8.861	ug/L	
14) Carbon disulfide	2.291	76		4553	0.160	ug/L #	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027597.D
Acq On : 30 Aug 2022 19:44
Operator : SY/MD
Sample : N4400-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBVP1

Manual IntegrationsAPPROVED

Quant Time: Aug 31 04:51:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Aug 31 04:45:39 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 08/31/2022
Supervised By :Mahesh Dadoda 08/31/2022

