

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027579.D
 Acq On : 30 Aug 2022 12:15
 Operator : SY/MD
 Sample : VV0830WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK217

Quant Time: Aug 31 04:46:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 31 04:45:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	160012	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	160594	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	64599	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	55967	4.914	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.200%
7) Chloroethane-d5	1.565	69	47069	5.647	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	113.000%
11) 1,1-Dichloroethene-d2	2.105	63	80236	3.021	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.400%
20) 2-Butanone-d5	3.889	46	76465	53.953	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.900%
24) Chloroform-d	4.343	84	109187	4.795	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.000%
26) 1,2-Dichloroethane-d4	5.031	65	52555	5.335	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.600%
32) Benzene-d6	5.047	84	207104	4.656	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.200%
36) 1,2-Dichloropropane-d6	6.066	67	65892	5.095	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.000%
41) Toluene-d8	7.314	98	156249	3.890	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.800%
43) trans-1,3-Dichloroprop...	7.625	79	18480	4.173	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.400%
46) 2-Hexanone-d5	8.088	63	74055	50.806	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.620%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	41361	5.022	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.400%
66) 1,2-Dichlorobenzene-d4	11.622	152	50686	5.293	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.800%
Target Compounds						
16) Methylene chloride	2.507	84	16736	0.917	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027579.D
Acq On : 30 Aug 2022 12:15
Operator : SY/MD
Sample : VV0830WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK217

Quant Time: Aug 31 04:46:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Aug 31 04:45:39 2022
Response via : Initial Calibration

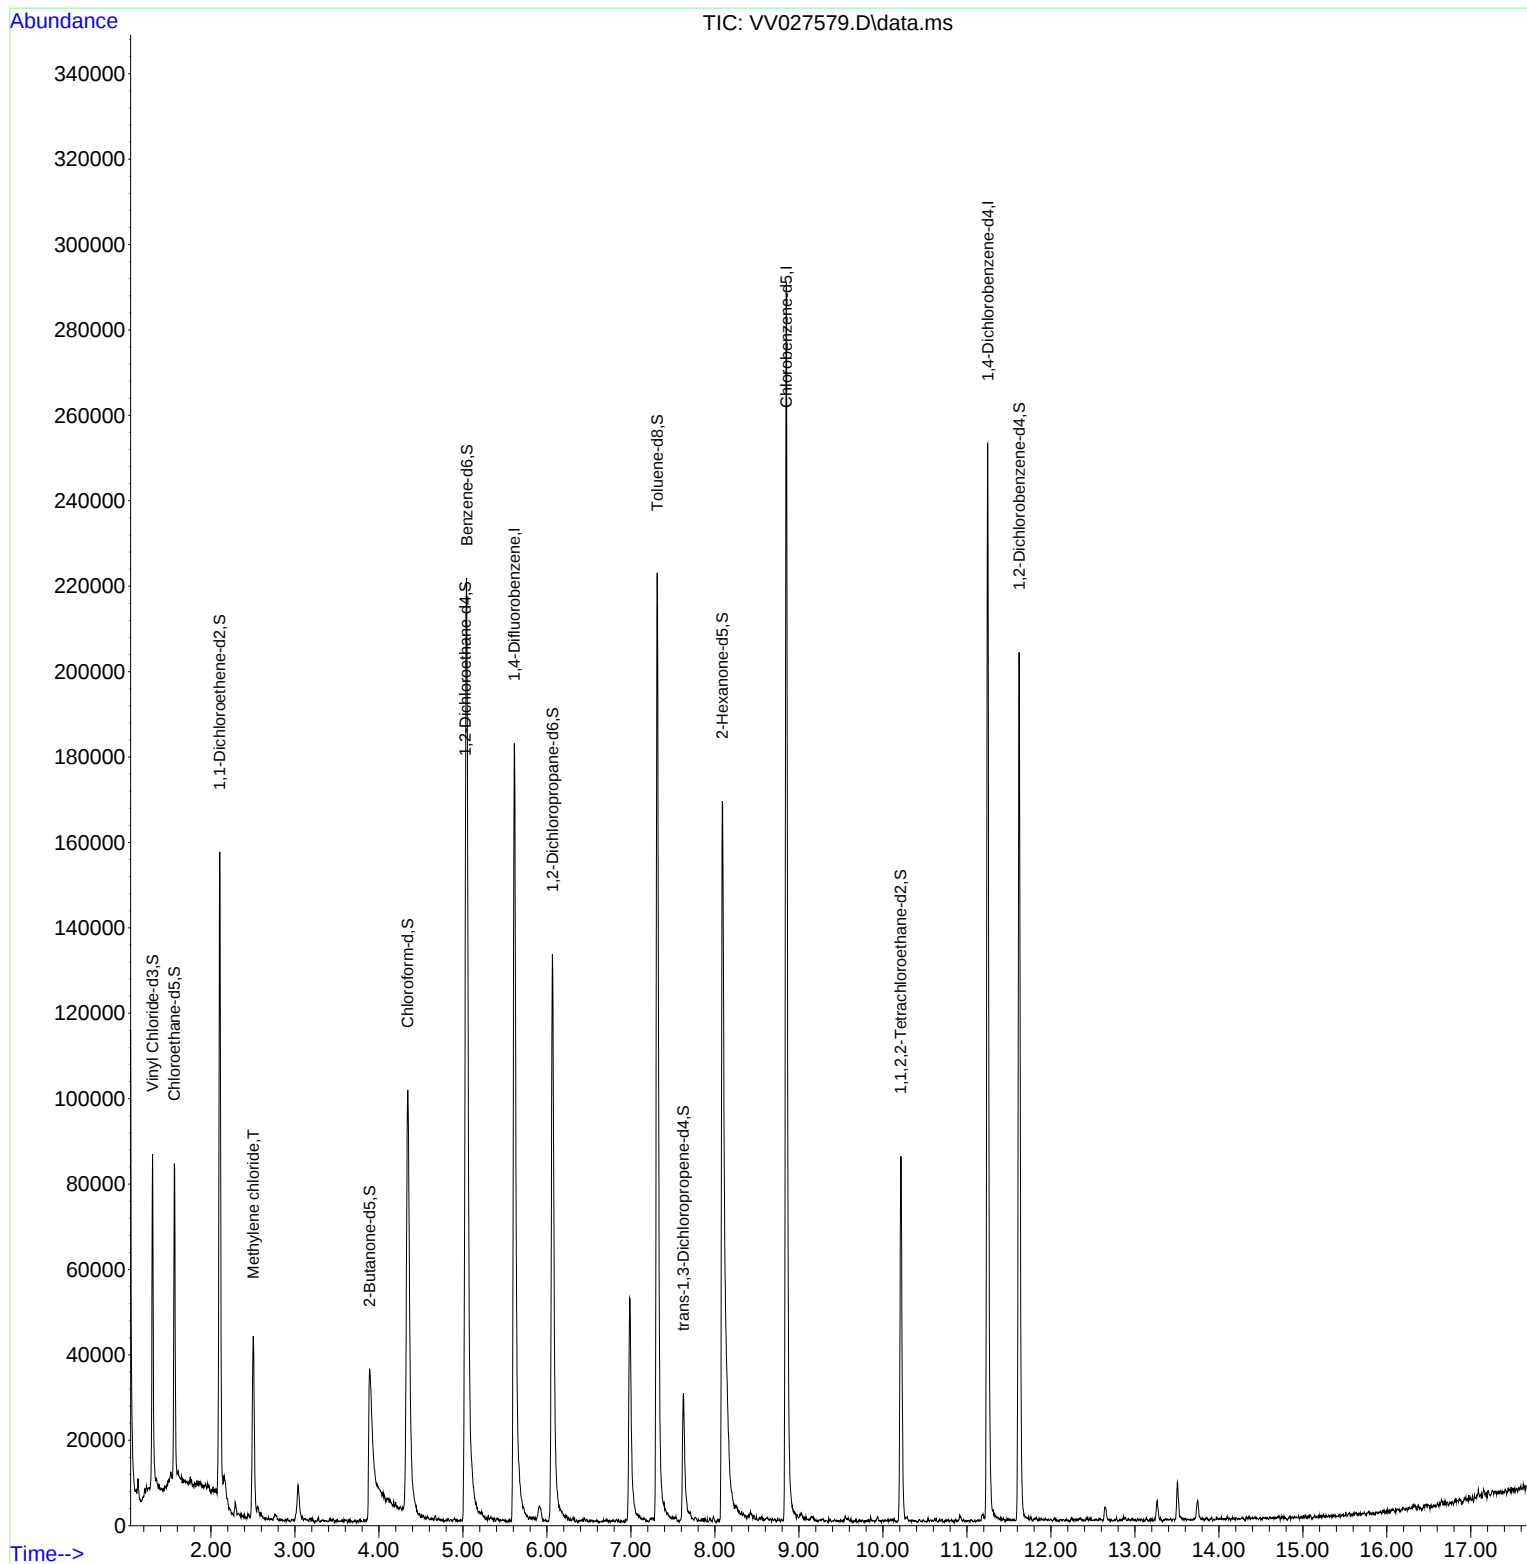

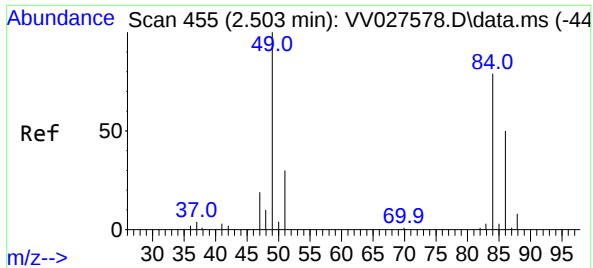

#16
Methylene chloride
Concen: 0.917 ug/L
RT: 2.507 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV027579.D
Acq: 30 Aug 2022 12:15

Instrument :
MSVOA_V
ClientSampleId :
VBLK217

Tgt Ion: 84 Resp: 16736
Ion Ratio Lower Upper
84 100
86 63.7 44.0 81.6
49 124.7 89.4 166.0

