

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027604.D
 Acq On : 30 Aug 2022 23:01
 Operator : SY/MD
 Sample : VV0830WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK218

Quant Time: Aug 31 07:12:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Aug 31 04:45:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	146478	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	145099	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	57627	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	48046	4.609	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.200%
7) Chloroethane-d5	1.564	69	41186	5.398	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	108.000%
11) 1,1-Dichloroethene-d2	2.105	63	68463	2.816	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.400%#
20) 2-Butanone-d5	3.895	46	63025	48.579	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.160%
24) Chloroform-d	4.346	84	99671	4.782	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
26) 1,2-Dichloroethane-d4	5.034	65	47841	5.305	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.200%
32) Benzene-d6	5.047	84	182041	4.529	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.600%
36) 1,2-Dichloropropane-d6	6.069	67	60008	5.136	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.800%
41) Toluene-d8	7.317	98	133938	3.691	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	73.800%
43) trans-1,3-Dichloroprop...	7.625	79	15694	3.923	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.400%
46) 2-Hexanone-d5	8.091	63	67852	51.521	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.040%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	38691	5.200	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	44090	5.161	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.200%
Target Compounds						Qvalue
16) Methylene chloride	2.506	84	12733	0.762	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027604.D
Acq On : 30 Aug 2022 23:01
Operator : SY/MD
Sample : VV0830WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK218


Quant Time: Aug 31 07:12:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Aug 31 04:45:39 2022
Response via : Initial Calibration

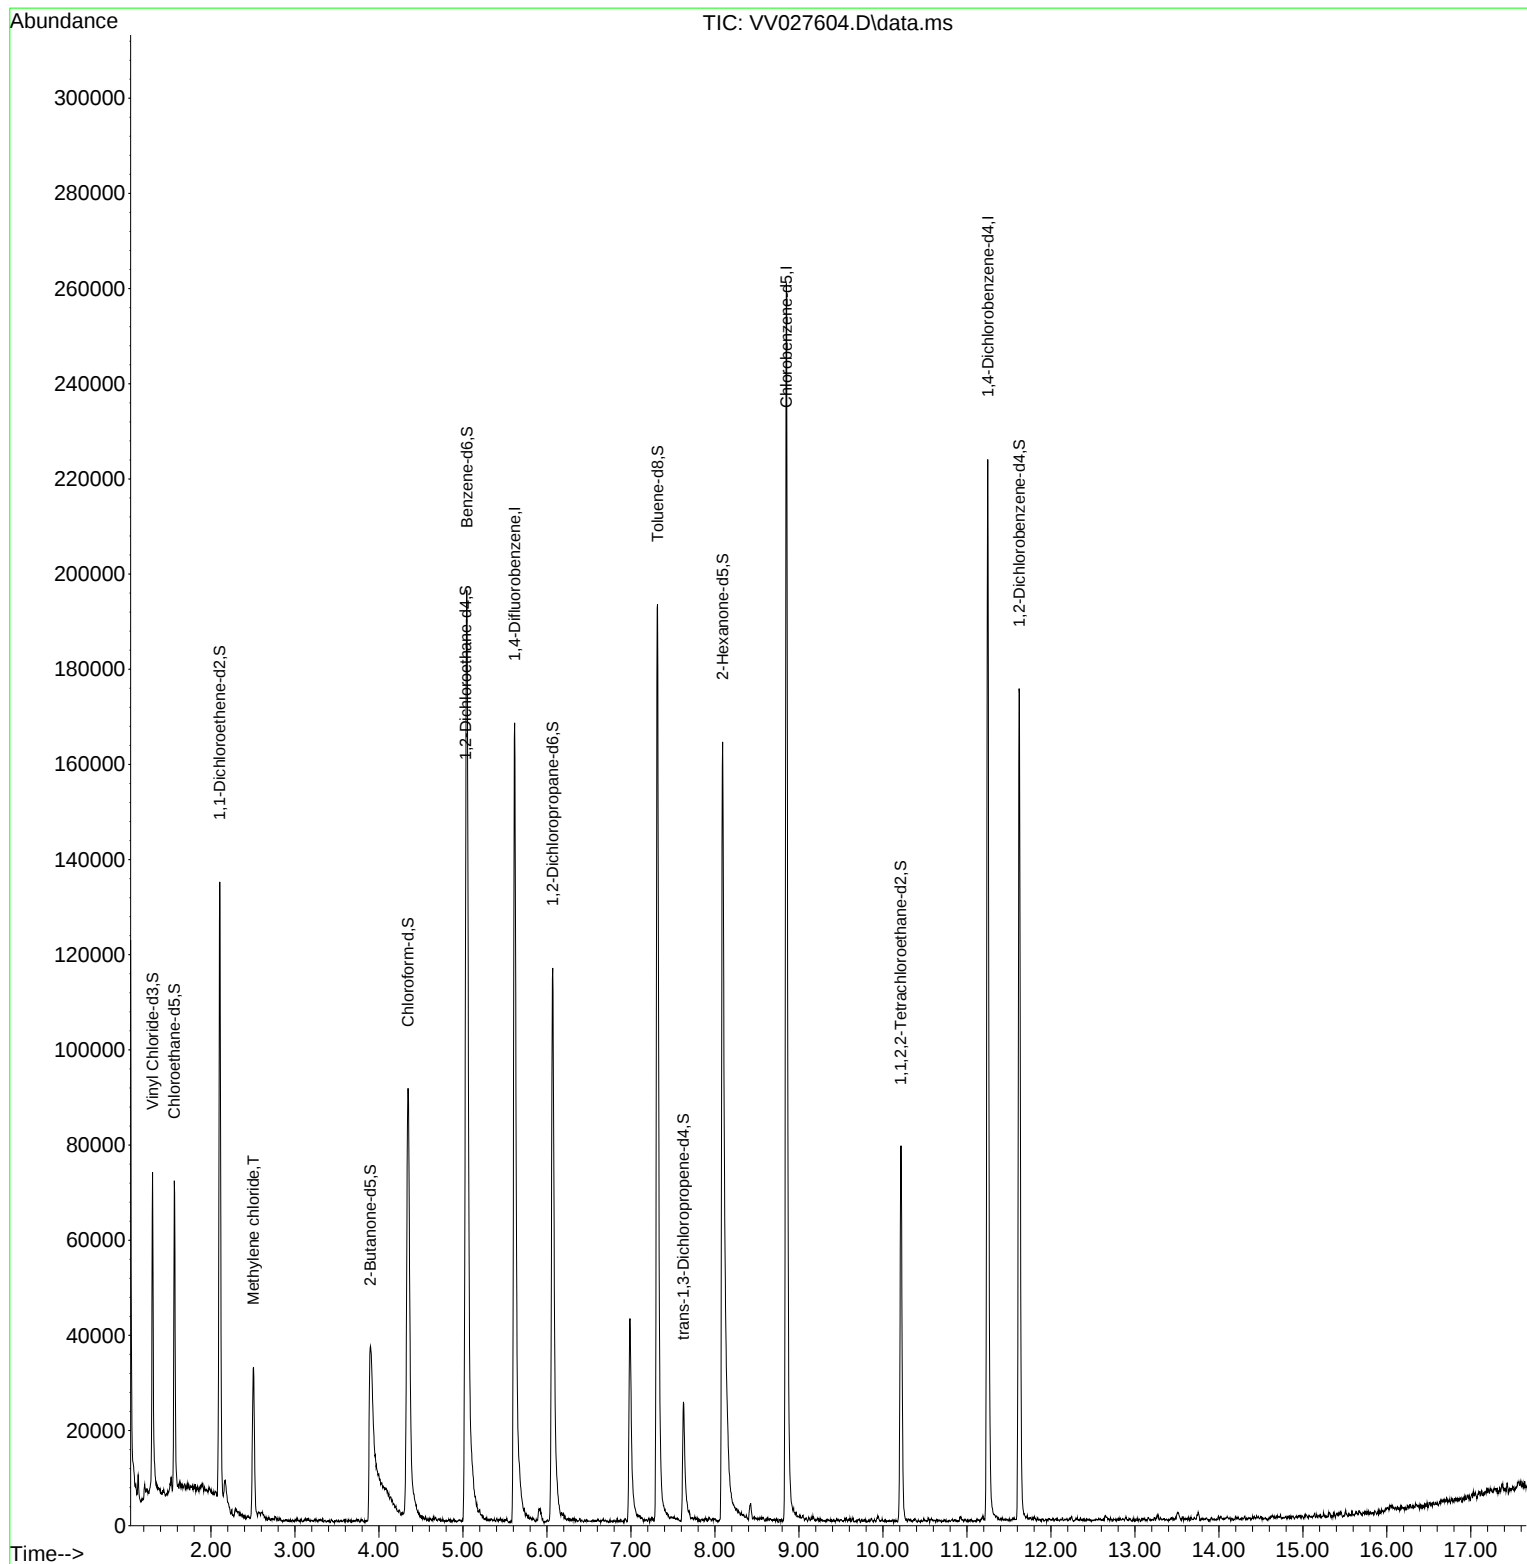

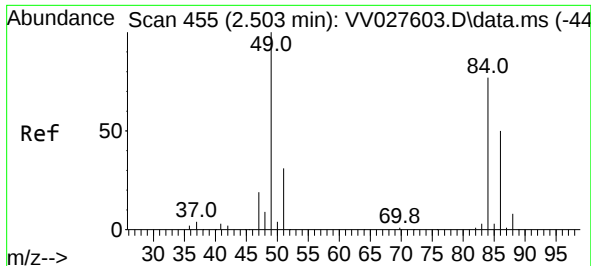

#16
Methylene chloride
Concen: 0.762 ug/L
RT: 2.506 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV027604.D
Acq: 30 Aug 2022 23:01

Instrument :
MSVOA_V
ClientSampleId :
VBLK218

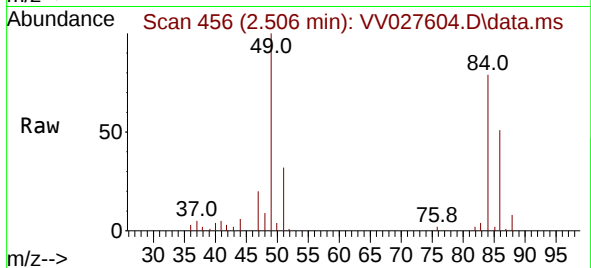

Tgt Ion: 84 Resp: 12733

Ion	Ratio	Lower	Upper
84	100		
86	64.4	44.0	81.6
49	126.3	89.4	166.0

