

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
 Data File : VV027579.D
 Acq On : 30 Aug 2022 12:15
 Operator : SY/MD
 Sample : VV0830WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK217

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rBV	76841	83276	14.19%	1.811%
2	1.565	156	163	173	rBV	73521	84860	14.46%	1.845%
3	2.105	321	331	343	rBV	150276	214356	36.53%	4.661%
4	2.503	445	455	468	rBV	42475	72666	12.38%	1.580%
5	3.037	609	621	635	rBV6	8204	16839	2.87%	0.366%
6	3.889	874	886	911	rBV	35545	123558	21.06%	2.687%
7	4.343	1013	1027	1062	rVB	98941	269688	45.96%	5.864%
8	5.044	1229	1245	1279	rBV3	220608	586729	100.00%	12.758%
9	5.613	1410	1422	1453	rBV	182172	408221	69.58%	8.877%
10	6.066	1549	1563	1586	rBV	132741	291223	49.64%	6.333%
11	6.986	1838	1849	1873	rBV	52177	108453	18.48%	2.358%
12	7.314	1939	1951	1973	rBV	221940	416748	71.03%	9.062%
13	7.625	2036	2048	2066	rBV2	29776	60305	10.28%	1.311%
14	8.088	2181	2192	2238	rBV	168583	462240	78.78%	10.051%
15	8.850	2417	2429	2456	rBV	289835	498506	84.96%	10.840%
16	10.214	2841	2853	2868	rBV	85642	142624	24.31%	3.101%
17	11.249	3164	3175	3193	rBV	251594	400645	68.28%	8.712%
18	11.622	3276	3291	3309	rBV	203380	330495	56.33%	7.187%
19	13.265	3794	3802	3811	rBV5	4618	7016	1.20%	0.153%
20	13.506	3867	3877	3886	rBV2	9059	14198	2.42%	0.309%
21	13.747	3944	3952	3958	rBV7	4091	6121	1.04%	0.133%




Sum of corrected areas: 4598767

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027579.D
Acq On : 30 Aug 2022 12:15
Operator : SY/MD
Sample : VV0830WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

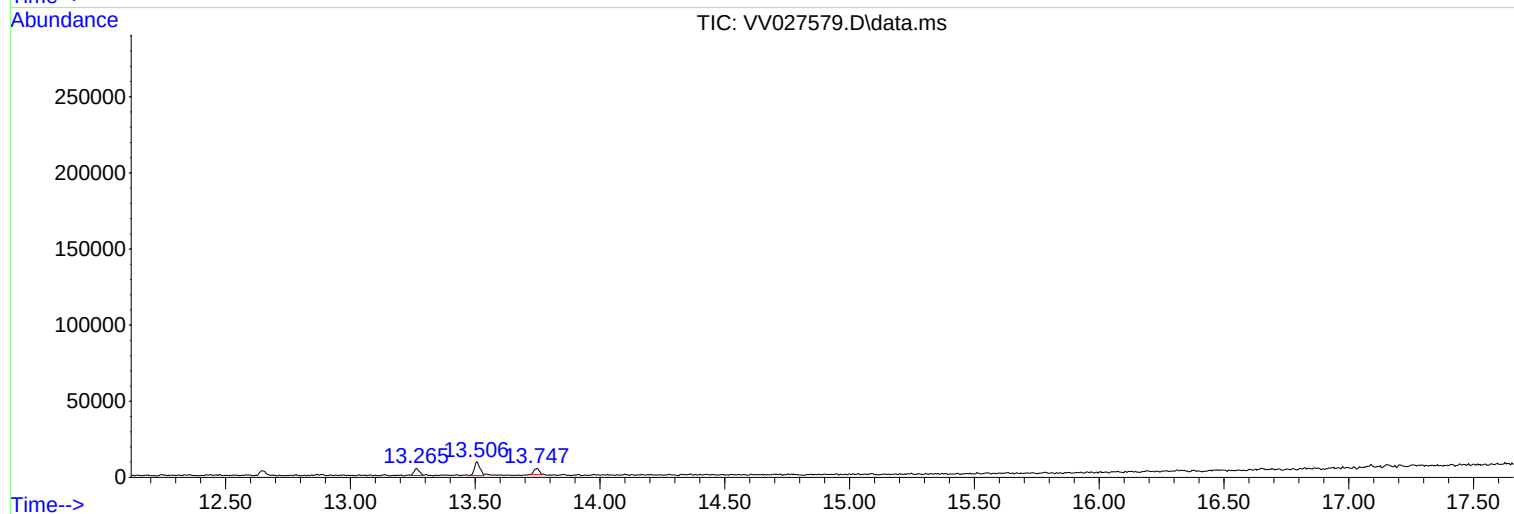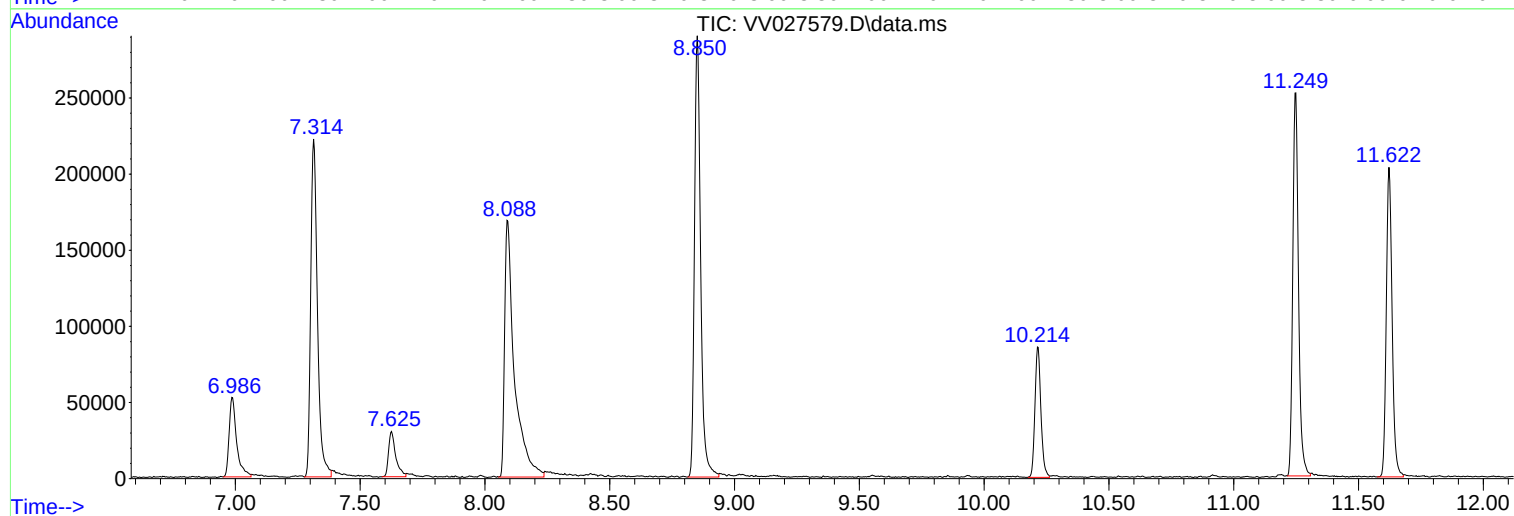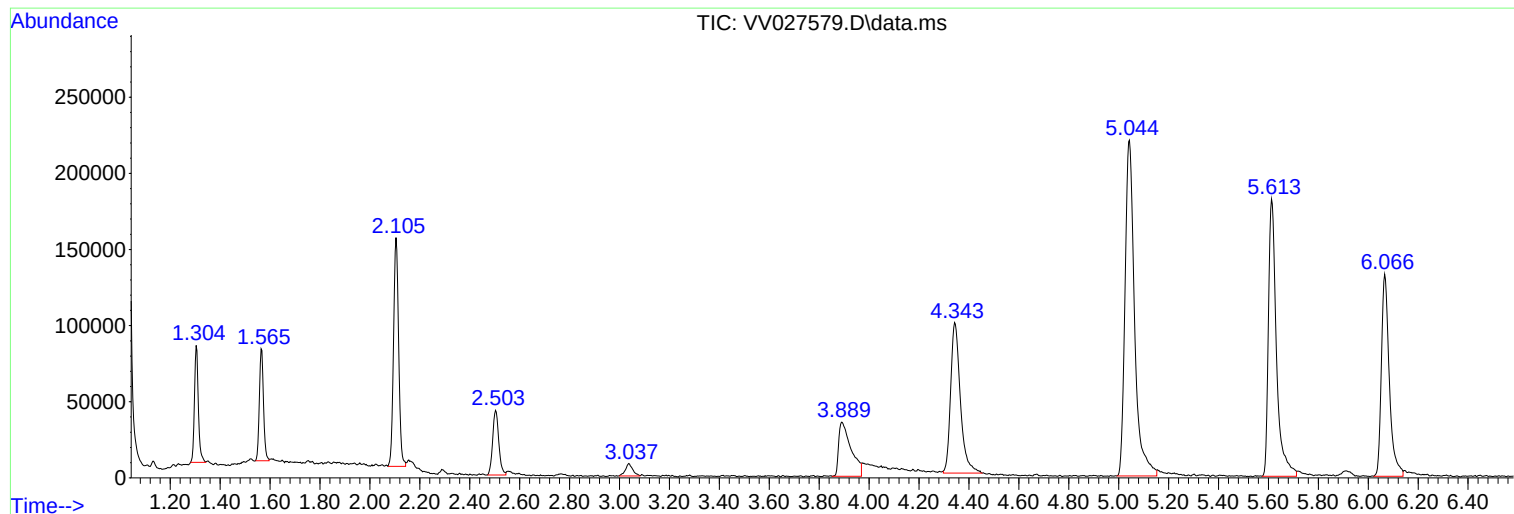

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027579.D
Acq On : 30 Aug 2022 12:15
Operator : SY/MD
Sample : VV0830WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV083022\
Data File : VV027579.D
Acq On : 30 Aug 2022 12:15
Operator : SY/MD
Sample : VV0830WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK217

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc